


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF091317\
 Data File : BF098492.D
 Acq On : 13 Sep 2017 16:17
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 02:14:50 2017

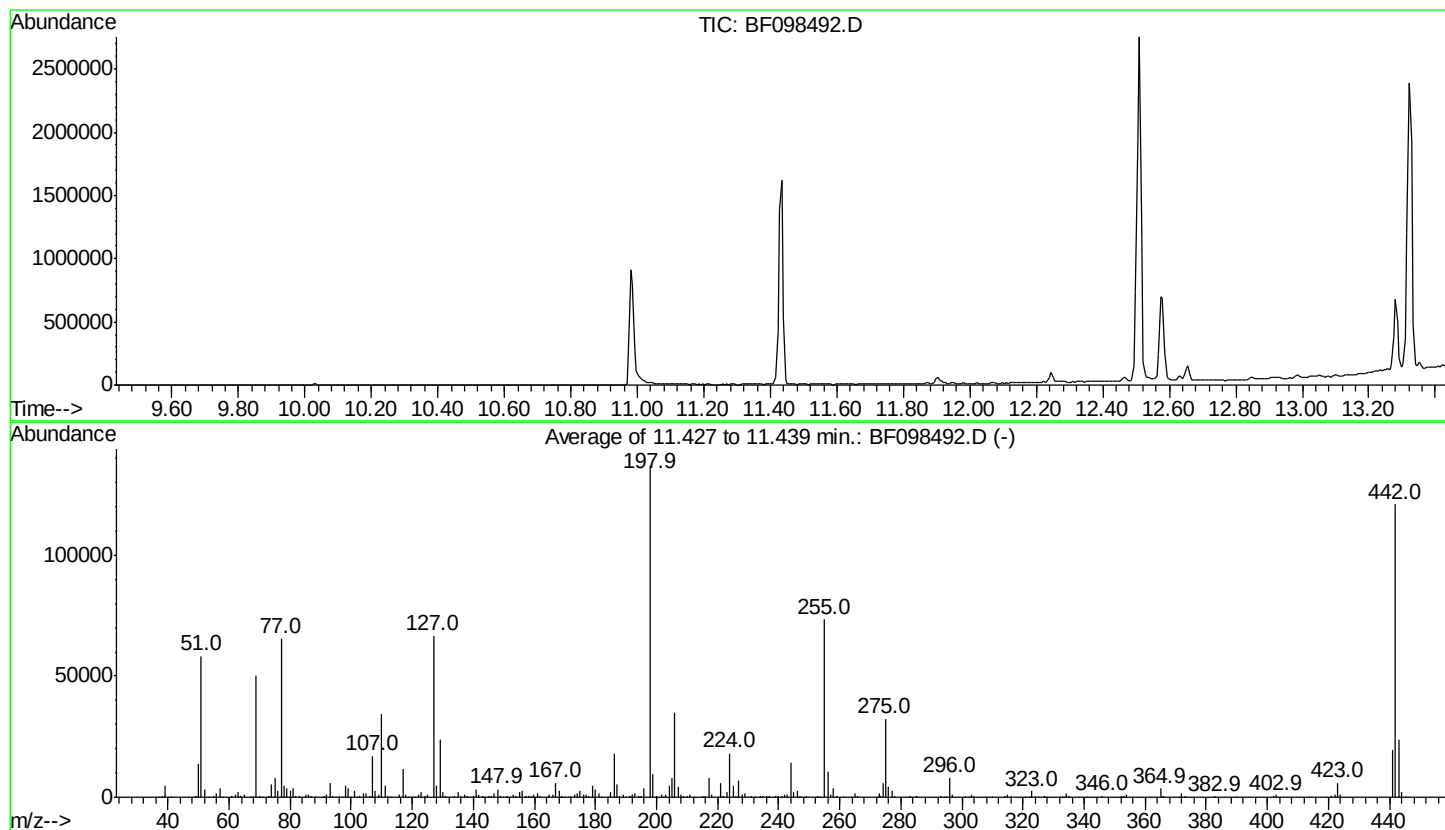

AutoFind: Scans 1588, 1589, 1590; Background Corrected with Scan 1582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	58391	PASS
68	69	0.00	2	1.6	796	PASS
69	198	0.00	100	36.5	50039	PASS
70	69	0.00	2	0.7	344	PASS
127	198	10	80	48.7	66685	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	136965	PASS
199	198	5	9	7.1	9682	PASS
275	198	10	60	23.6	32266	PASS
365	198	1	100	2.6	3566	PASS
441	442	0.01	24	16.1	19535	PASS
442	198	50	100	88.3	120978	PASS
443	442	15	24	19.5	23613	PASS