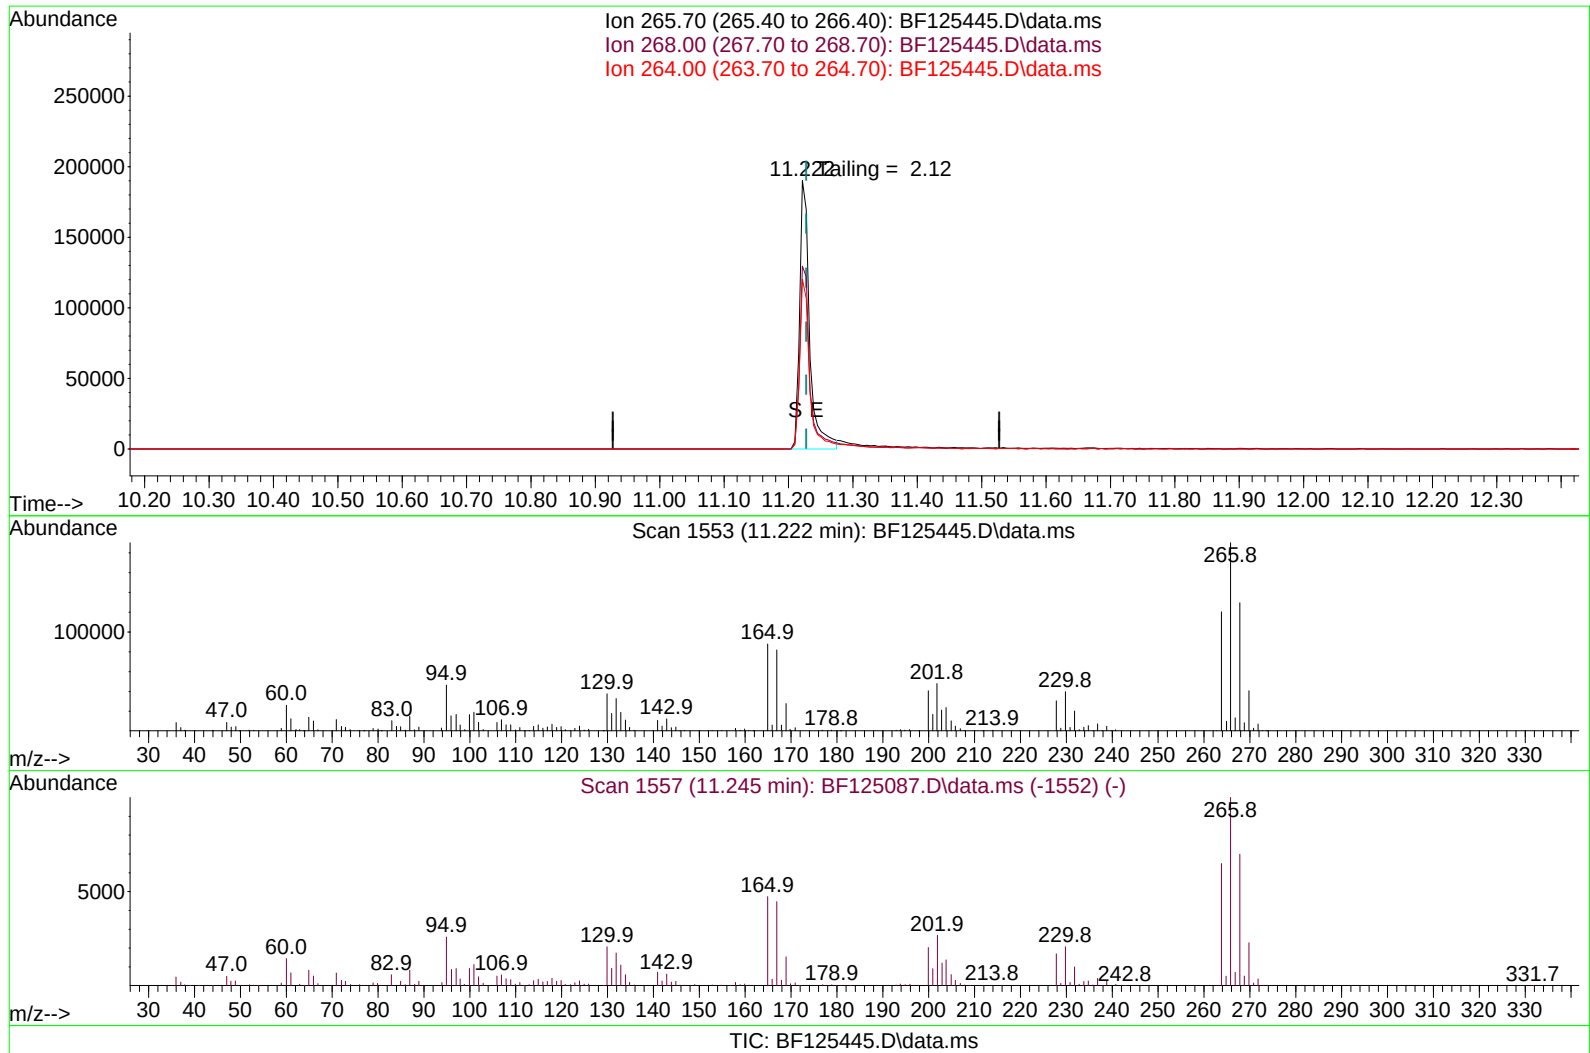


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF091321\  
Data File : BF125445.D  
Acq On : 13 Sep 2021 15:40  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1




Quant Time: Sep 13 17:51:25 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF081821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Sep 13 12:03:46 2021  
Response via : Initial Calibration

**(70) Pentachlorophenol (C)****11.222min (-0.006) 25410.84 ng****response 227279**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.10  | 68.14  |
| 264.00 | 69.90  | 63.28  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF091321\  
 Data File : BF125445.D  
 Acq On : 13 Sep 2021 15:40  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 17:51:25 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF081821.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Sep 13 12:03:46 2021  
 Response via : Initial Calibration

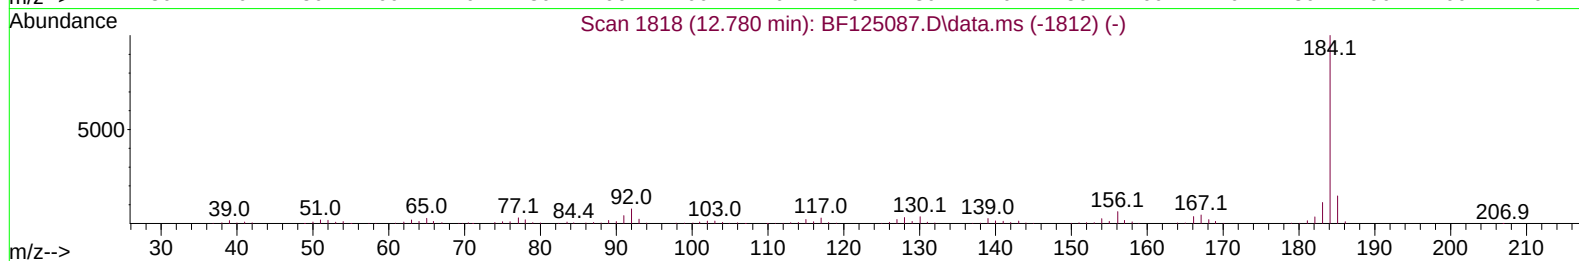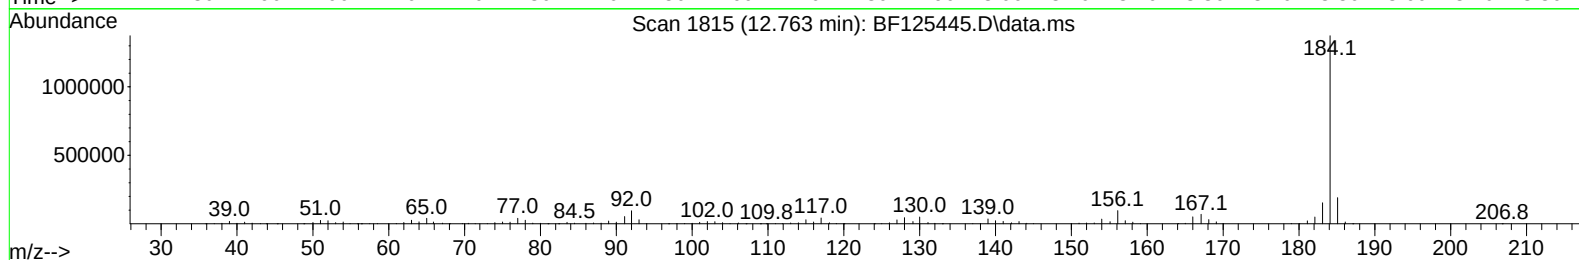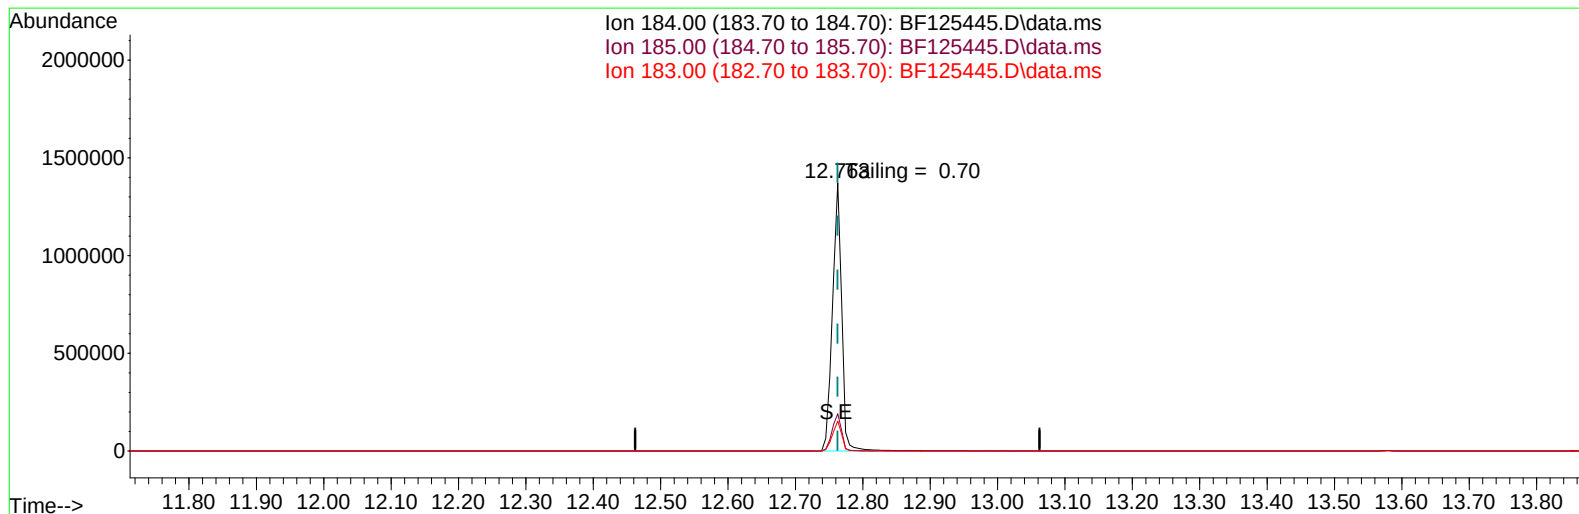

TIC: BF125445.D\data.ms

**(77) Benzidine**

12.763min (+ 0.000) 0.00 ng

response 1311489

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.50  | 13.92  |
| 183.00 | 10.10  | 11.19  |
| 0.00   | 0.00   | 0.00   |