
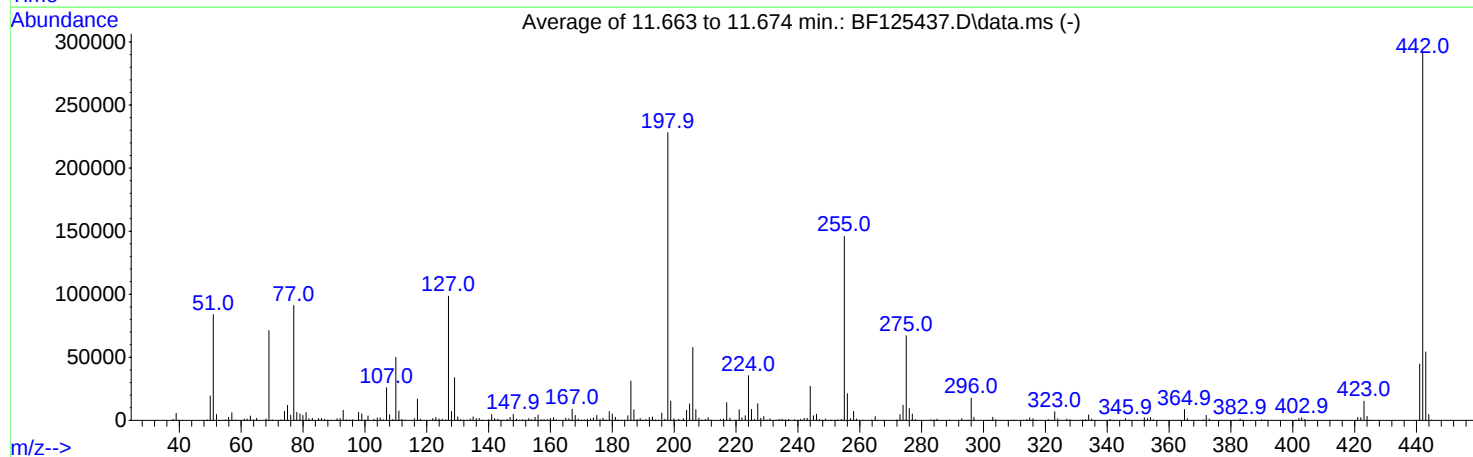


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091321\
 Data File : BF125437.D
 Acq On : 13 Sep 2021 10:25
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 13 12:03:46 2021

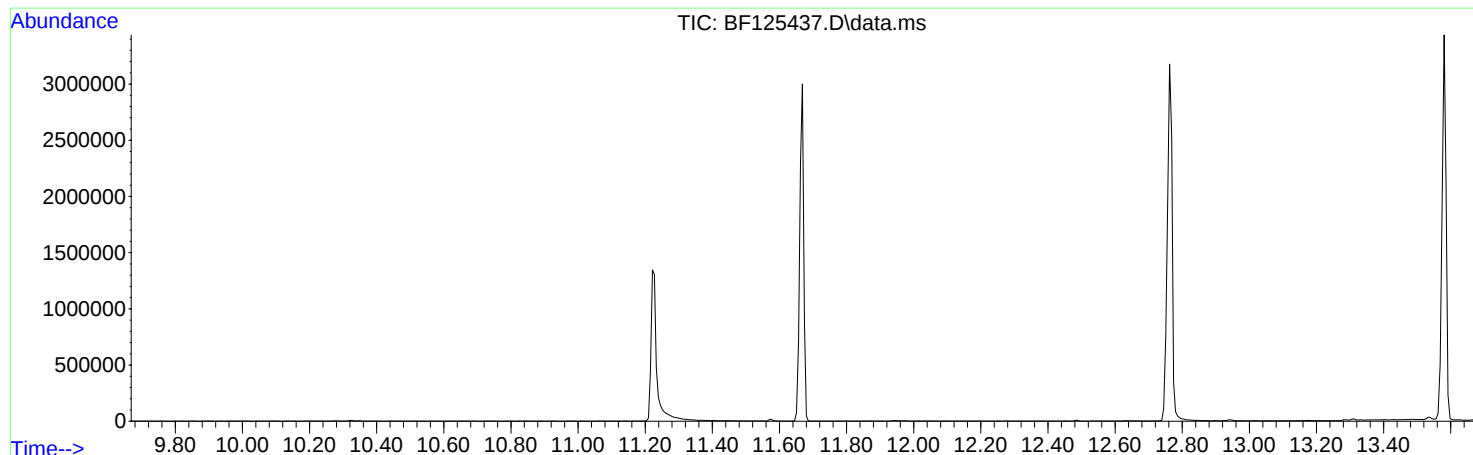




AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	83880	PASS
68	69	0.00	2	1.6	1144	PASS
69	198	0.00	100	31.2	71126	PASS
70	69	0.00	2	0.6	420	PASS
127	198	10	80	43.1	98437	PASS
197	198	0.00	2	0.4	939	PASS
198	198	100	100	100.0	228203	PASS
199	198	5	9	6.7	15197	PASS
275	198	10	60	29.4	67075	PASS
365	198	1	100	3.8	8583	PASS
441	198	0.01	100	19.6	44669	PASS
442	442	50	100	100.0	291669	PASS
443	442	15	24	18.6	54363	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091321\
 Data File : BF125437.D
 Acq On : 13 Sep 2021 10:25
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 13 12:10:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 13 12:03:46 2021
 Response via : Initial Calibration

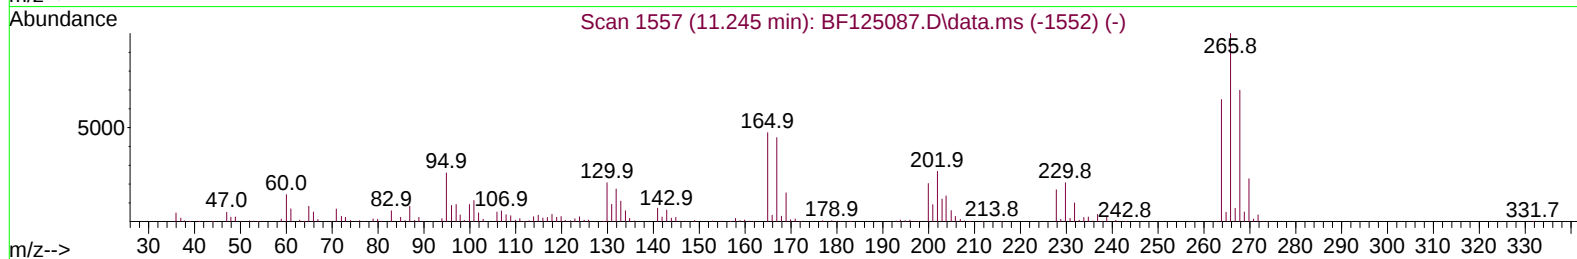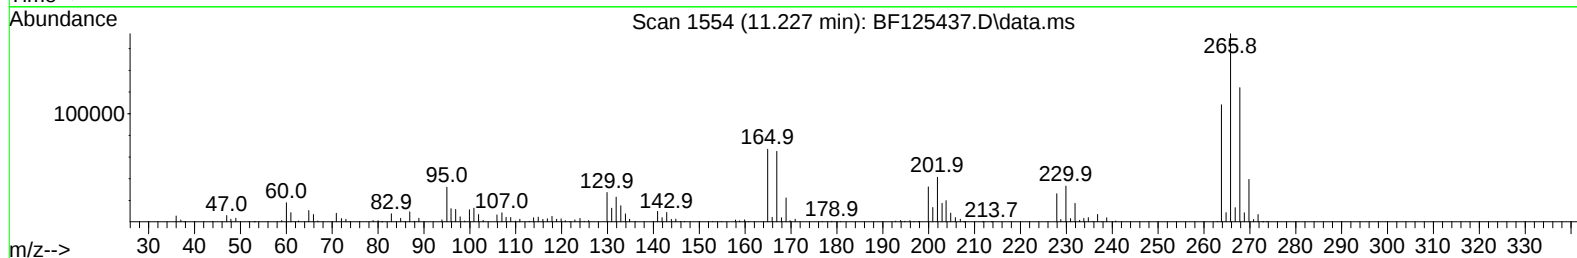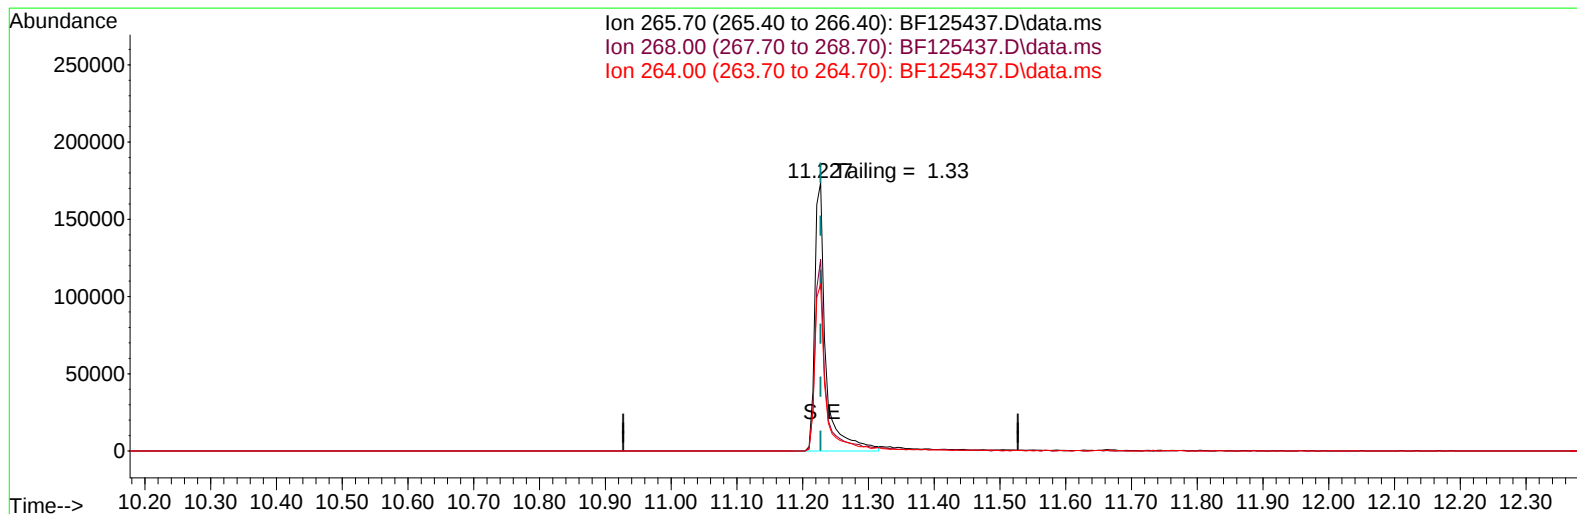

TIC: BF125437.D\data.ms

(70) Pentachlorophenol (C)

11.227min (+ 0.000) 32290.79 ng




response 210788

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	71.35
264.00	69.90	62.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091321\
Data File : BF125437.D
Acq On : 13 Sep 2021 10:25
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 13 12:10:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 13 12:03:46 2021
Response via : Initial Calibration

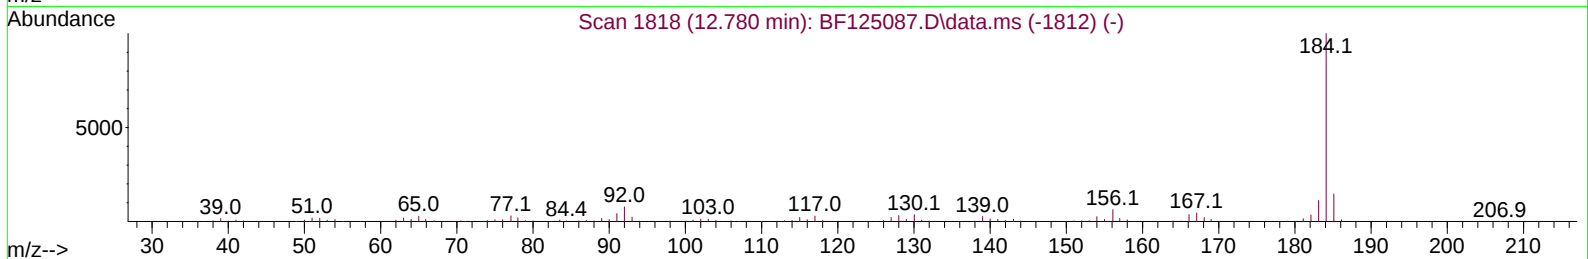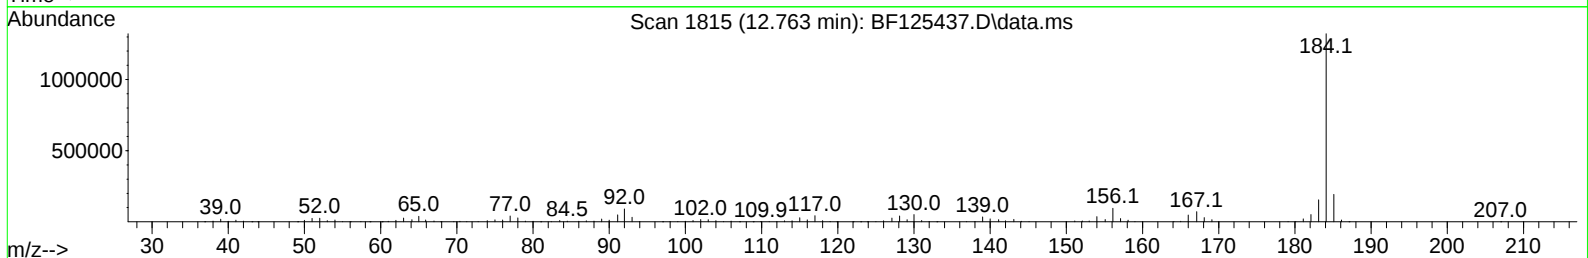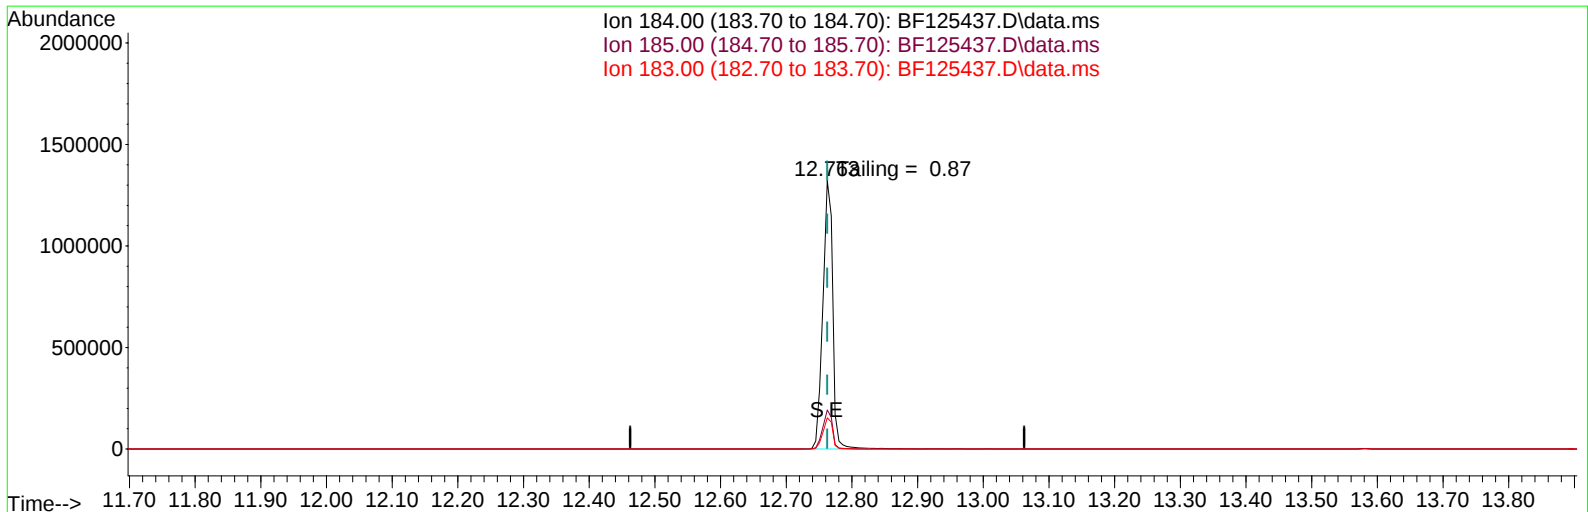

TIC: BF125437.D\data.ms

(77) Benzidine

12.763min (+ 0.000) 0.00 ng

response 1376253

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.54
183.00	10.10	11.65
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/13/2021	BNA_F	<u>BF125437.D</u>
Compound Name	Response	Retention Time
DDT	6604819	13.58
DDD	2549	13.28
DDE	2323	12.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4872	6609691	0.07

Instrument :
BNA_F
ClientSampleId :
DFTPP