
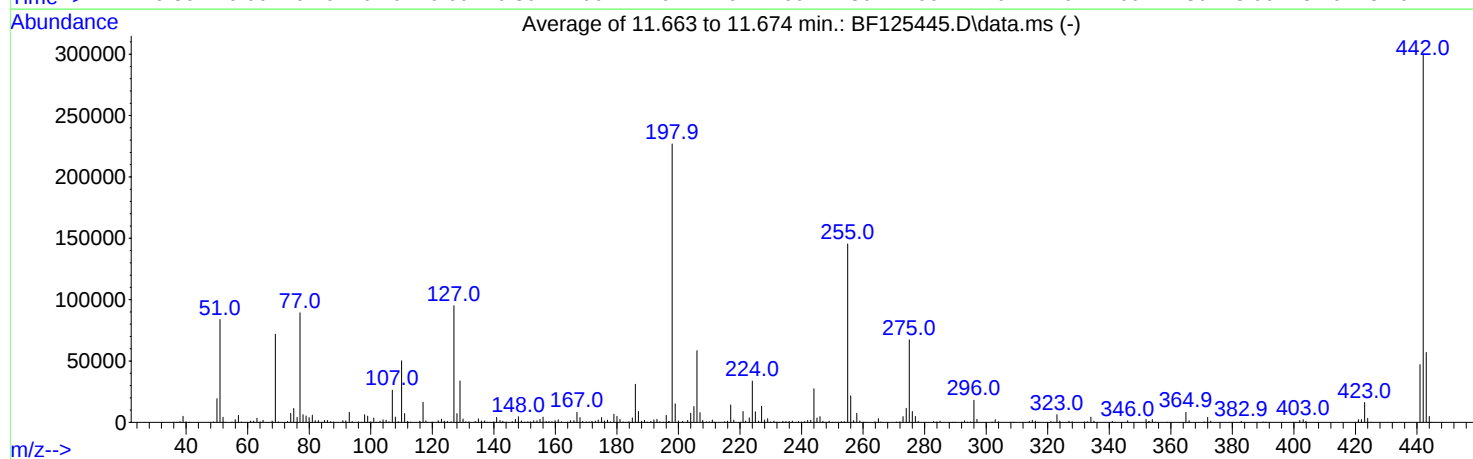


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091321\
 Data File : BF125445.D
 Acq On : 13 Sep 2021 15:40
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 13 12:03:46 2021

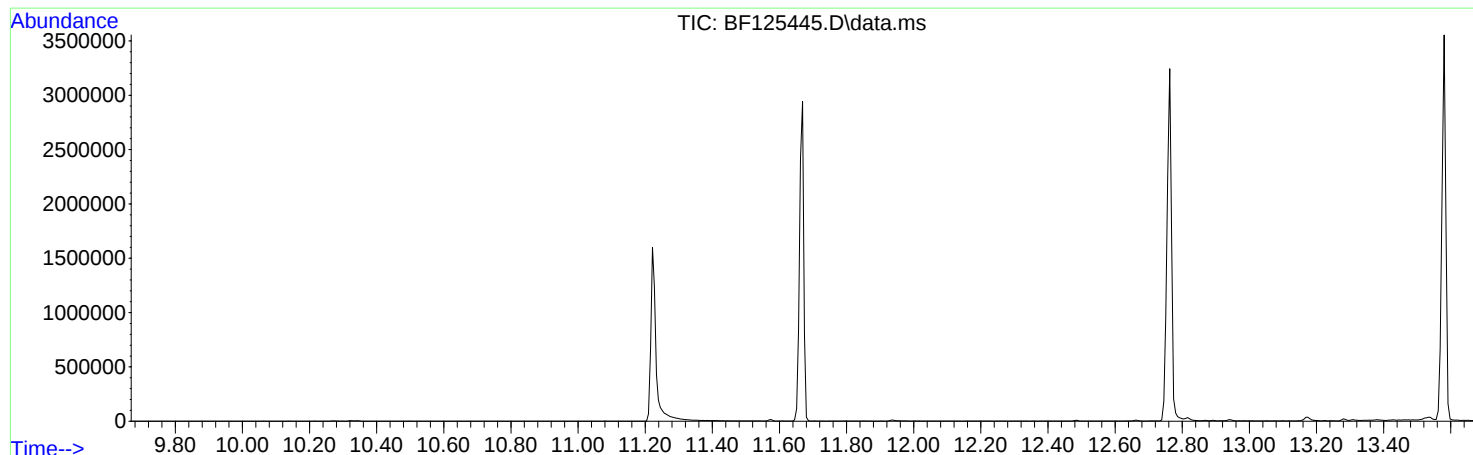




AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	83852	PASS
68	69	0.00	2	1.6	1115	PASS
69	198	0.00	100	31.7	71860	PASS
70	69	0.00	2	0.5	381	PASS
127	198	10	80	41.9	95032	PASS
197	198	0.00	2	0.3	664	PASS
198	198	100	100	100.0	226867	PASS
199	198	5	9	6.7	15170	PASS
275	198	10	60	29.6	67245	PASS
365	198	1	100	3.6	8264	PASS
441	198	0.01	100	20.7	47027	PASS
442	442	50	100	100.0	299733	PASS
443	442	15	24	19.0	57027	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091321\
 Data File : BF125445.D
 Acq On : 13 Sep 2021 15:40
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 13 17:51:25 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 13 12:03:46 2021
 Response via : Initial Calibration

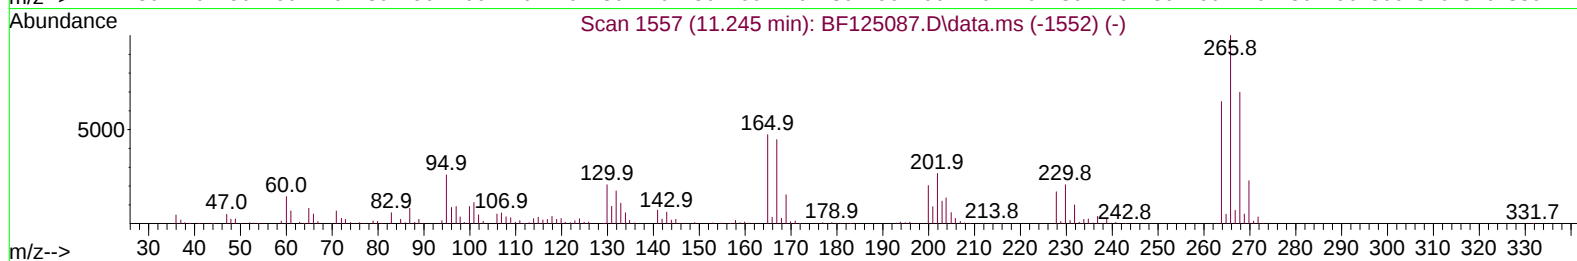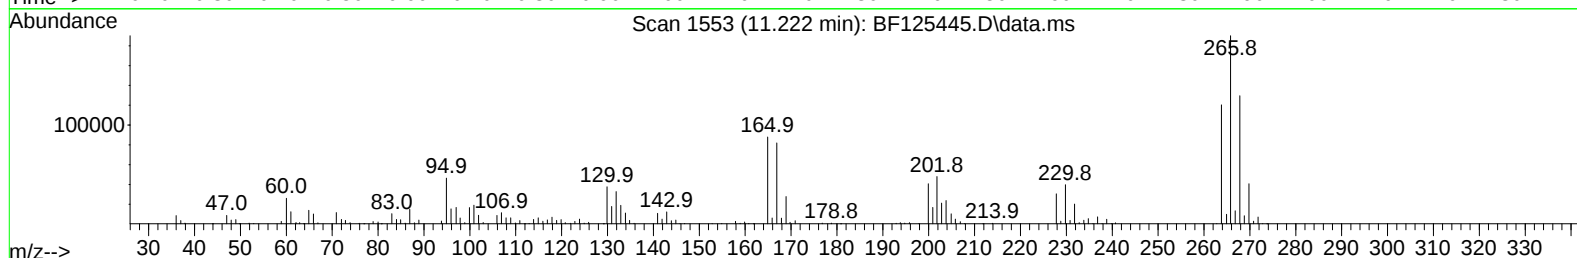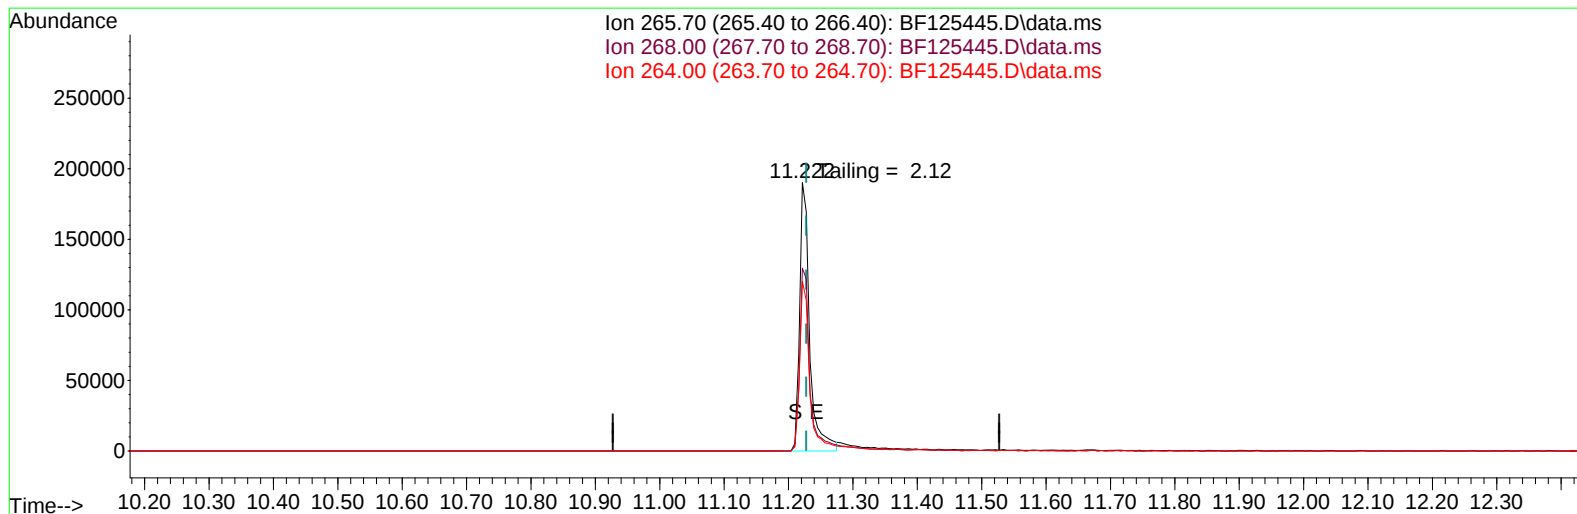

TIC: BF125445.D\data.ms

(70) Pentachlorophenol (C)

11.222min (-0.006) 25410.84 ng




response 227279

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	68.14
264.00	69.90	63.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091321\
Data File : BF125445.D
Acq On : 13 Sep 2021 15:40
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 13 17:51:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 13 12:03:46 2021
Response via : Initial Calibration

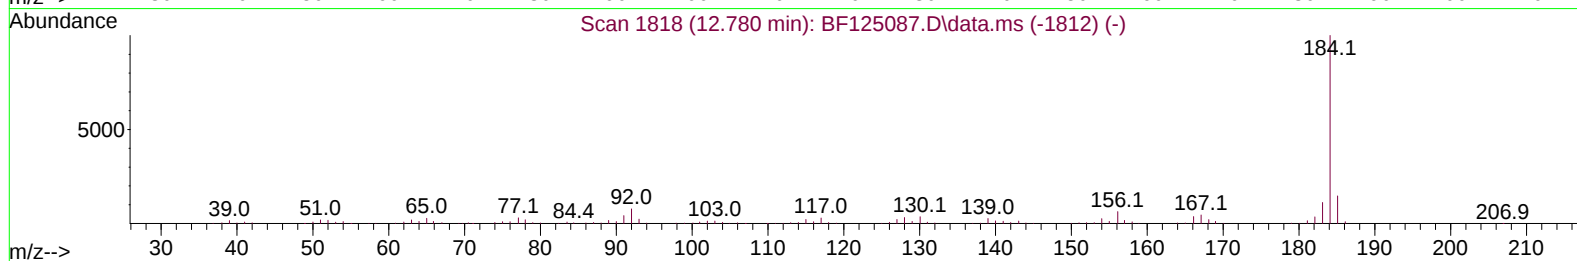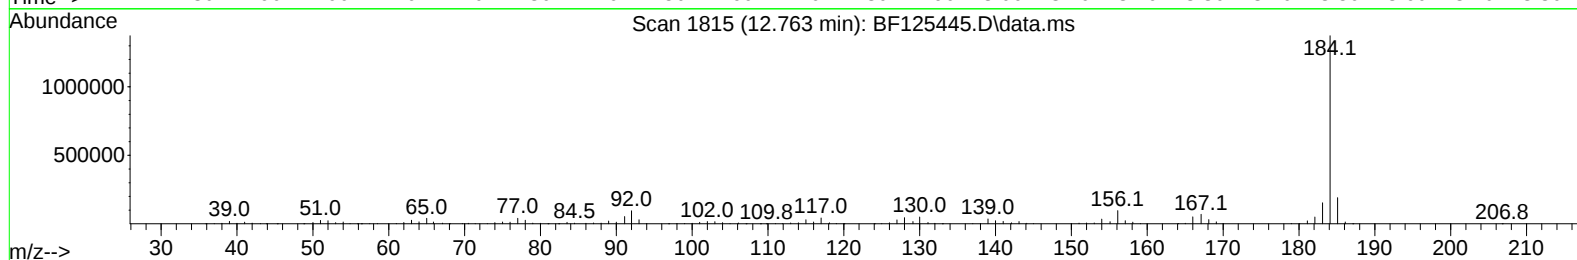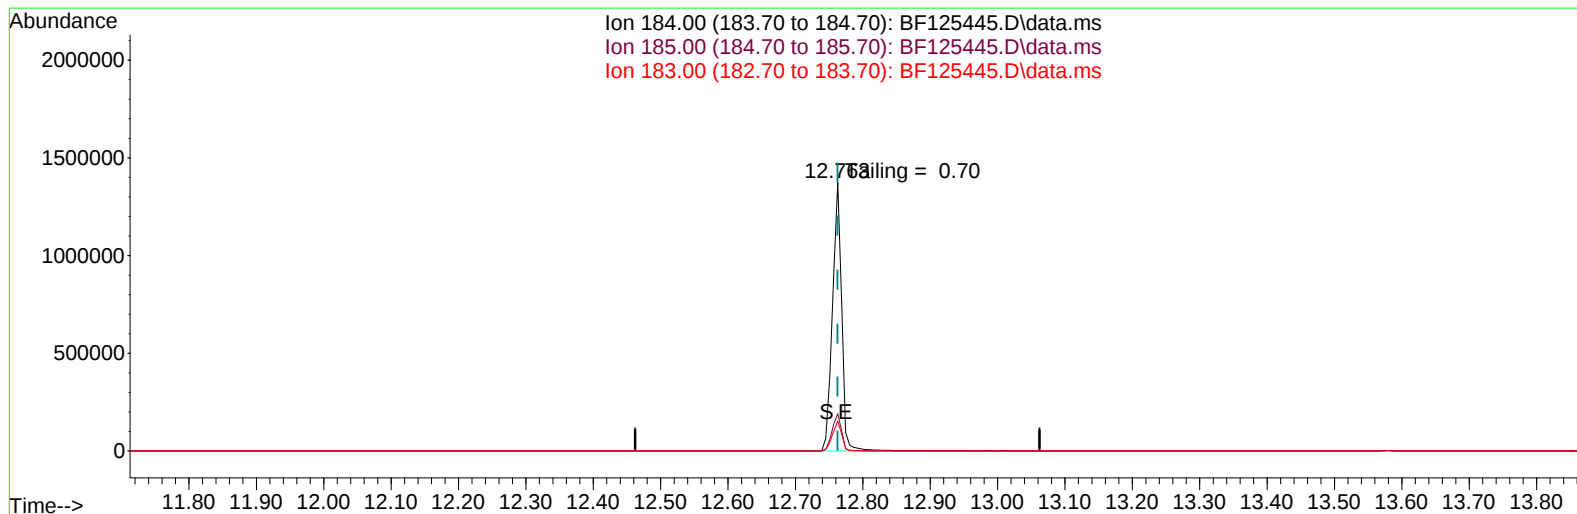

TIC: BF125445.D\data.ms

(77) Benzidine

12.763min (+ 0.000) 0.00 ng

response 1311489

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.92
183.00	10.10	11.19
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/13/2021	BNA_F	<u>BF125445.D</u>
Compound Name	Response	Retention Time
DDT	621105	13.58
DDD	4898	13.28
DDE	2573	12.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7471	628576	1.19

Instrument :
BNA_F
ClientSampleId :
DFTPP