
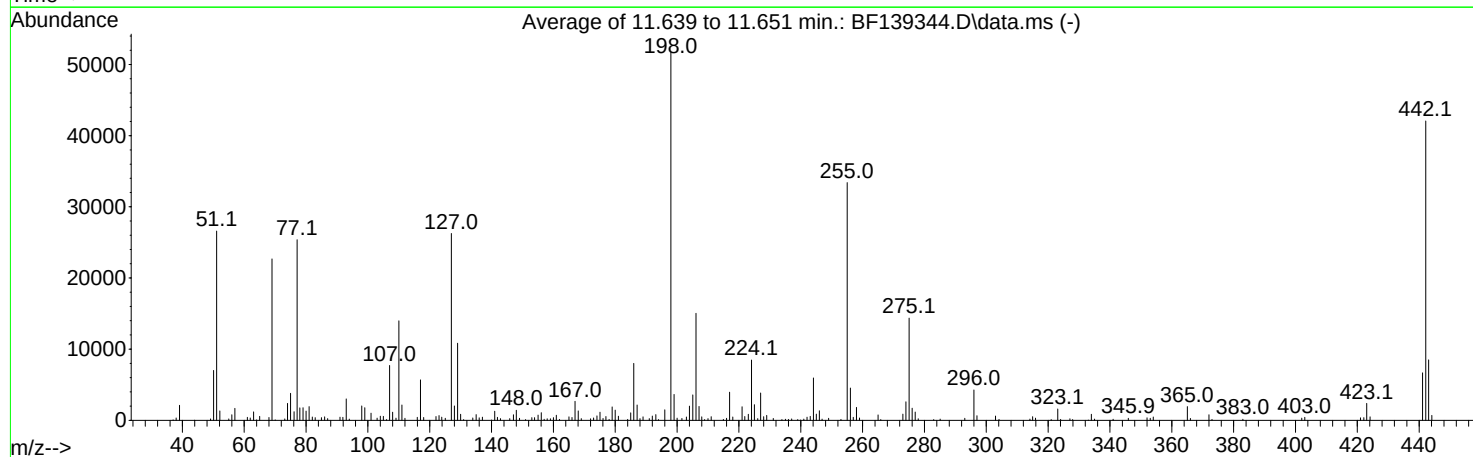


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091324\
Data File : BF139344.D
Acq On : 13 Sep 2024 14:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Sep 14 02:58:23 2024

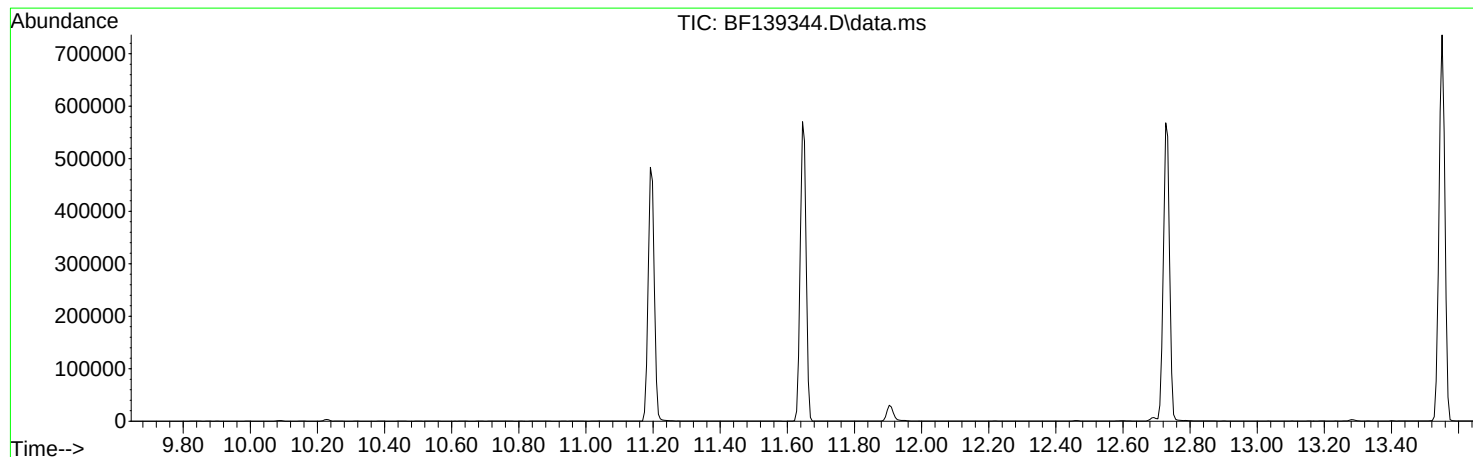

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	51.4	26587	PASS
68	69	0.00	2	1.8	408	PASS
69	198	0.00	100	43.9	22688	PASS
70	69	0.00	2	0.3	58	PASS
127	198	10	80	50.8	26253	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51680	PASS
199	198	5	9	7.0	3638	PASS
275	198	10	60	27.8	14373	PASS
365	198	1	100	3.7	1928	PASS
441	198	0.01	100	12.9	6681	PASS
442	442	50	100	100.0	42051	PASS
443	442	15	24	20.2	8504	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/13/2024	BNA_F	<u>BF139344.D</u>
Compound Name	Response	Retention Time
DDT	167916	13.551
DDD	1258	13.28
DDE	0	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1258	169174	0.74

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091324\
Data File : BF139344.D
Acq On : 13 Sep 2024 14:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 14 03:25:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

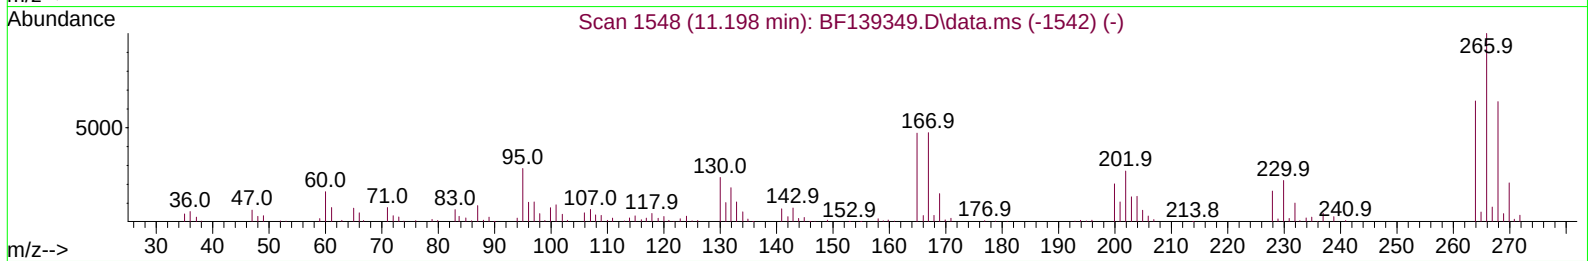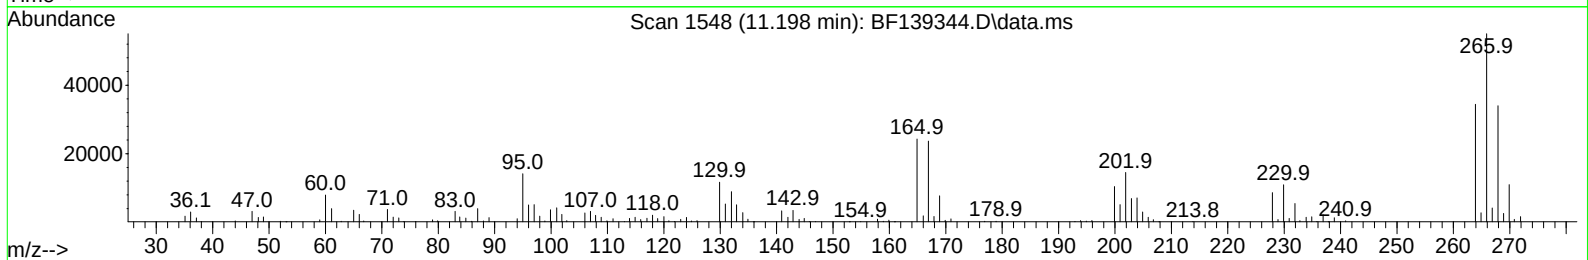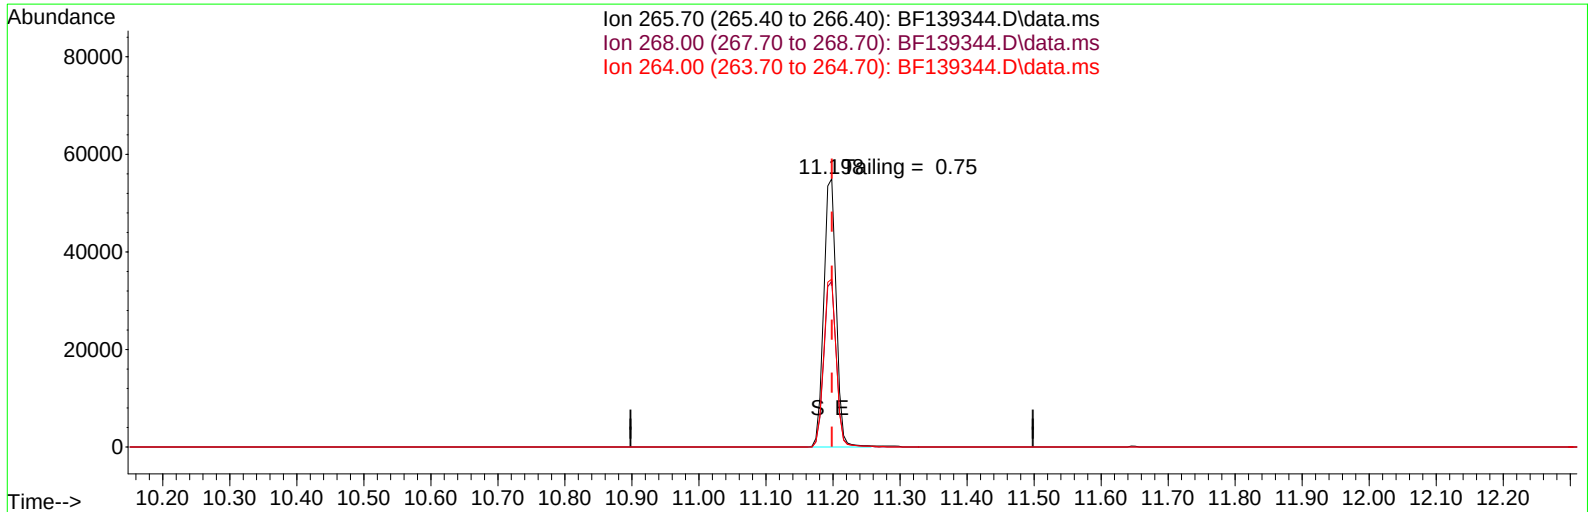

TIC: BF139344.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.000) 38365.64 ng




response 71487

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	61.78
264.00	64.20	62.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091324\
Data File : BF139344.D
Acq On : 13 Sep 2024 14:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 14 03:25:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

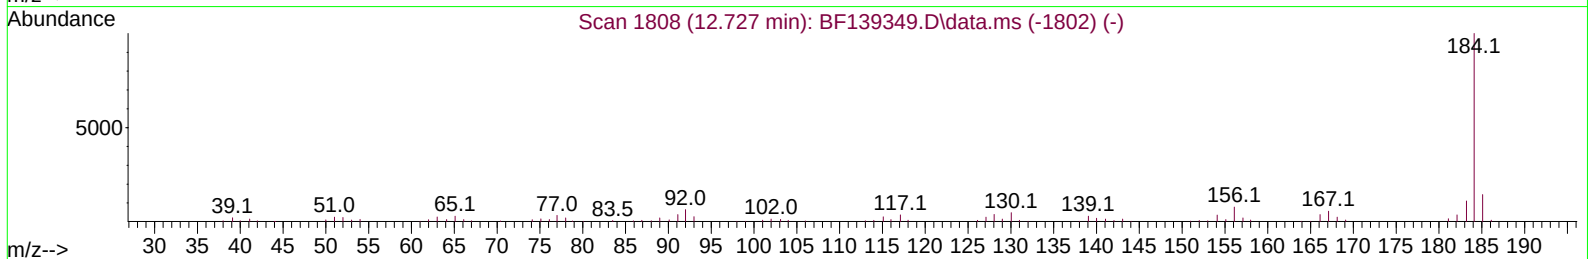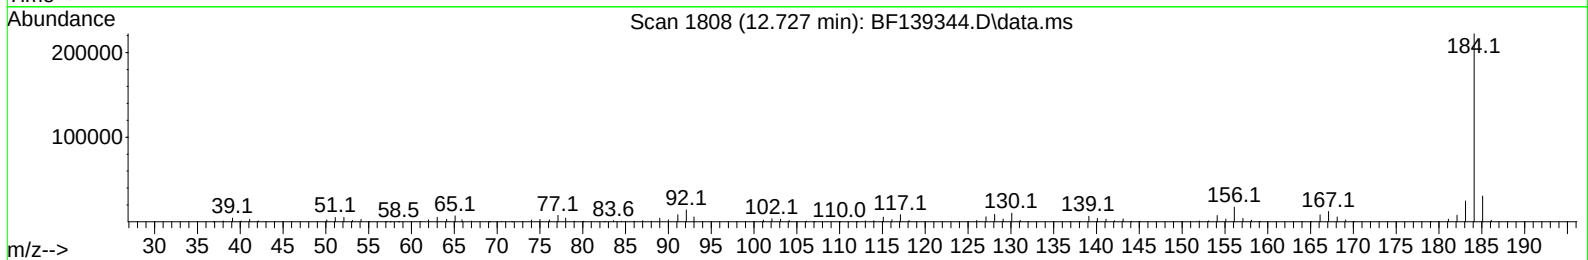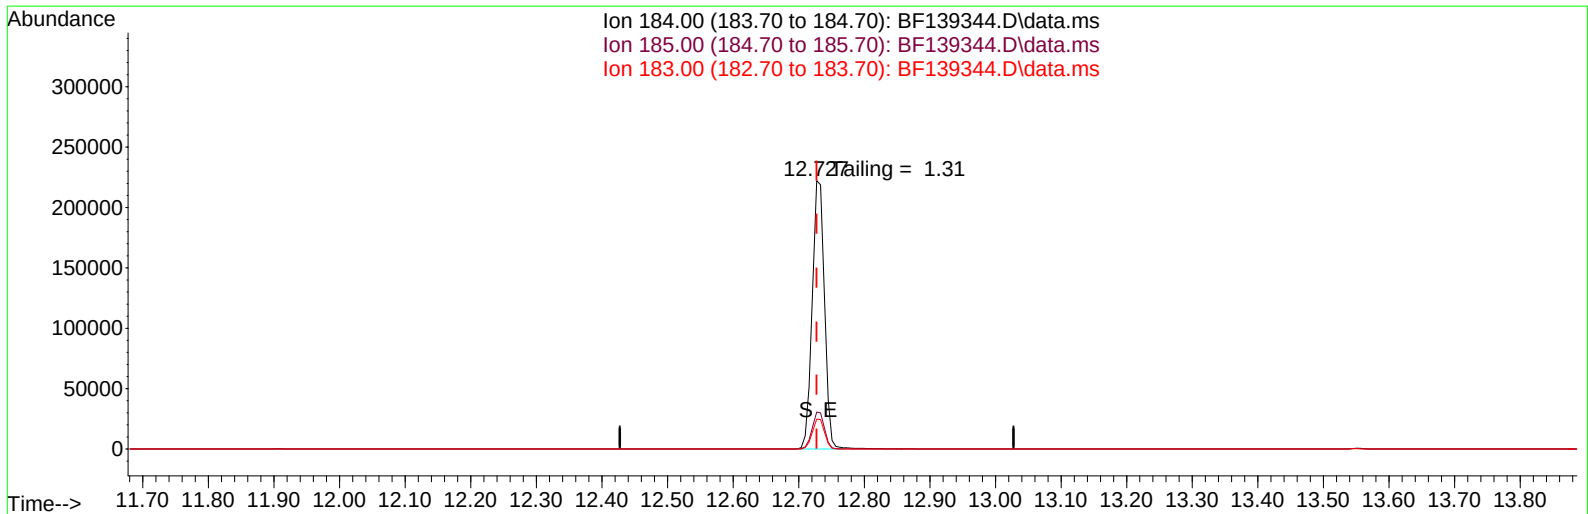

TIC: BF139344.D\data.ms

(77) Benzidine

12.727min (-0.000) 0.00 ng

response 292142

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.80
183.00	11.10	11.14
0.00	0.00	0.00