
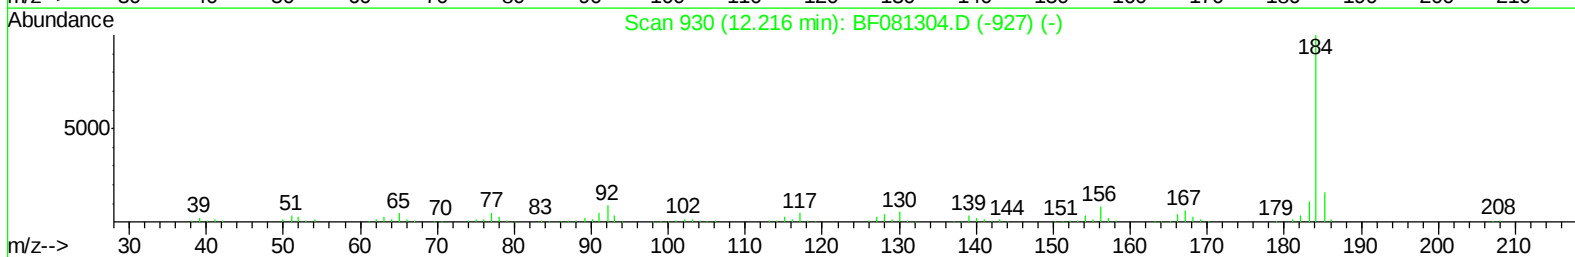
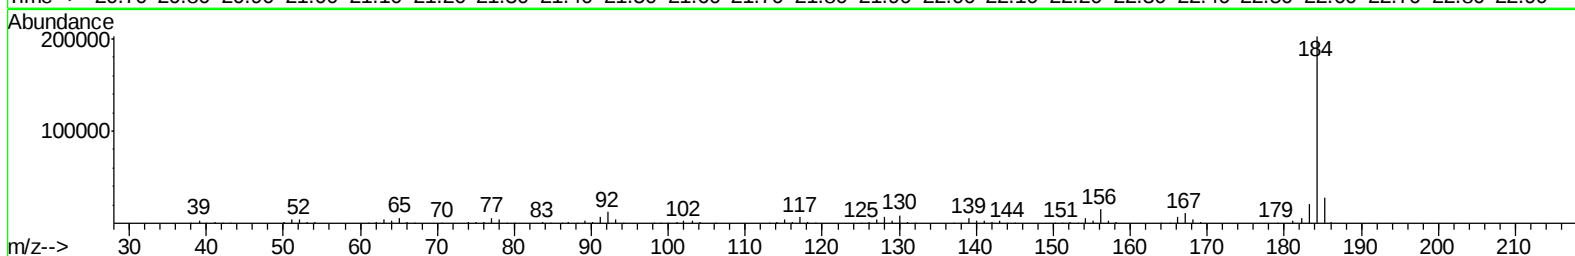


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091415\
Data File : BF081601.D
Acq On : 14 Sep 2015 10:30
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 18:44:22 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 14 13:51:56 2015
Response via : Initial Calibration

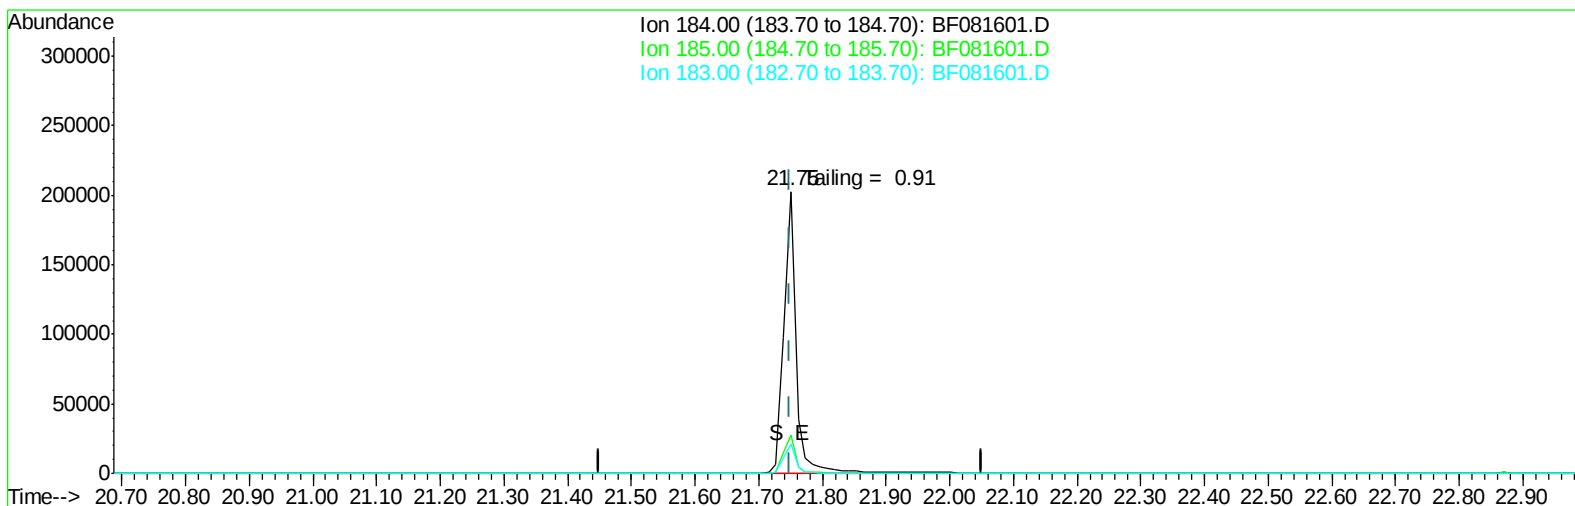

TIC: BF081601.D

(76) Benzidine




21.750min (+0.000) 0.00ng

response 268547

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.75
183.00	9.50	10.39
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091415\
Data File : BF081601.D
Acq On : 14 Sep 2015 10:30
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 18:44:22 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 14 13:51:56 2015
Response via : Initial Calibration

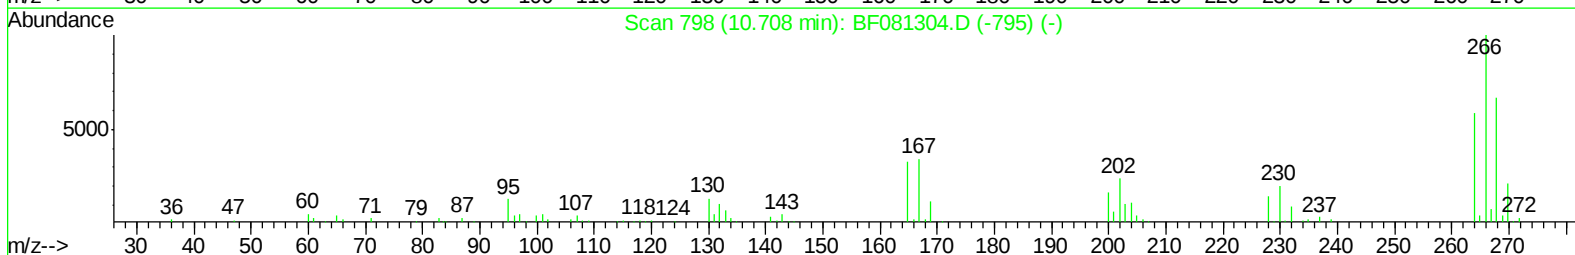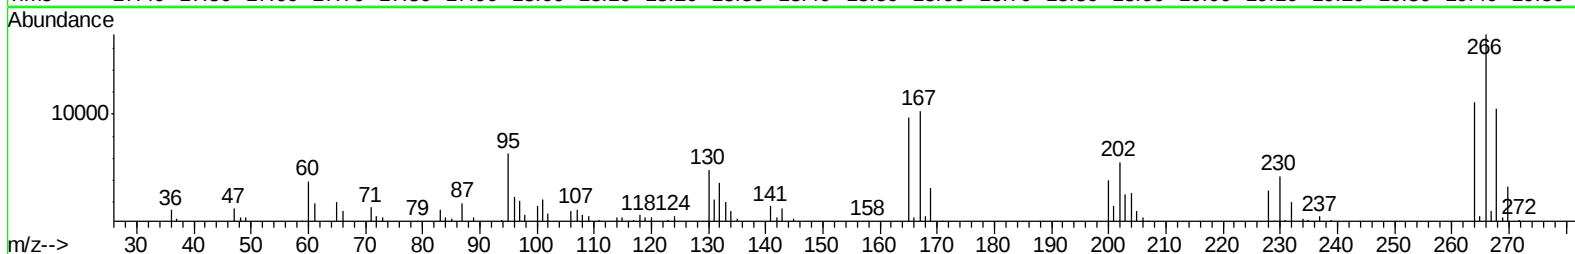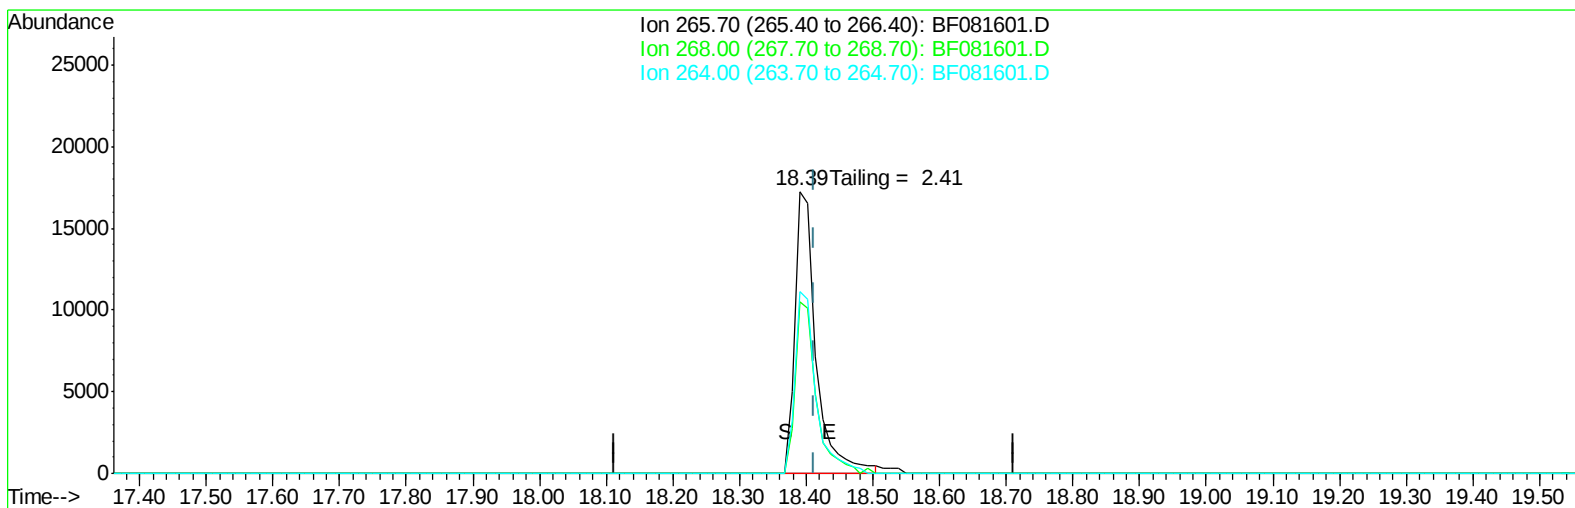

TIC: BF081601.D

(69) Pentachlorophenol (C)

18.390min (-0.023) 0.00ng

response 38439

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	61.00
264.00	62.70	64.35
0.00	0.00	0.00