


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF091415\  
 Data File : BF081620.D  
 Acq On : 15 Sep 2015 00:55  
 Operator : UM/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF090115.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Sep 14 13:51:56 2015

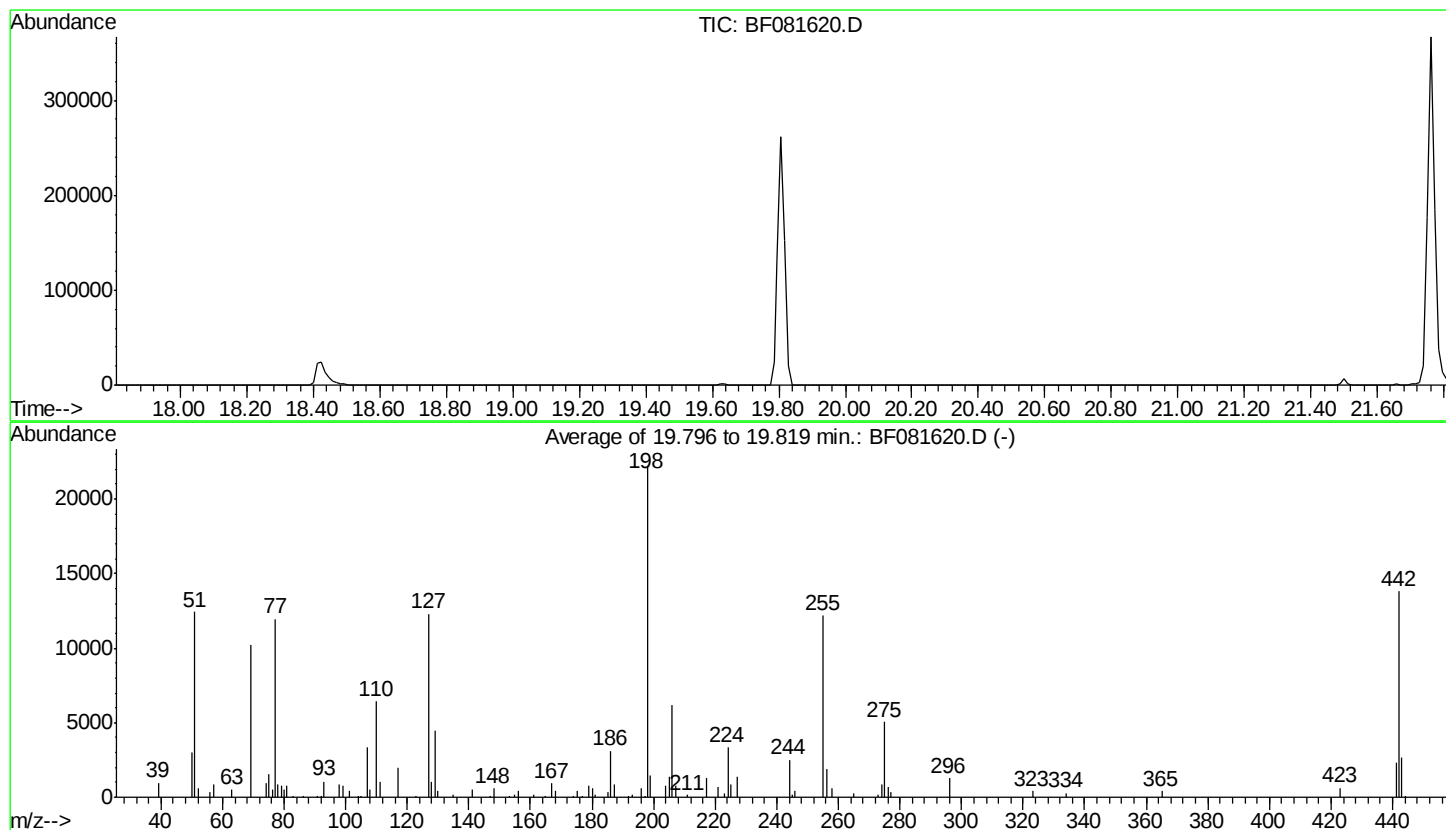

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1611

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 56.0      | 12449   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 45.9      | 10204   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 55.3      | 12297   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 105     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 22242   | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 1484    | PASS             |
| 275         | 198          | 10           | 60           | 22.7      | 5052    | PASS             |
| 365         | 198          | 1            | 100          | 1.9       | 424     | PASS             |
| 441         | 442          | 0.01         | 24           | 16.6      | 2288    | PASS             |
| 442         | 198          | 50           | 100          | 62.1      | 13823   | PASS             |
| 443         | 442          | 15           | 24           | 19.4      | 2676    | PASS             |