
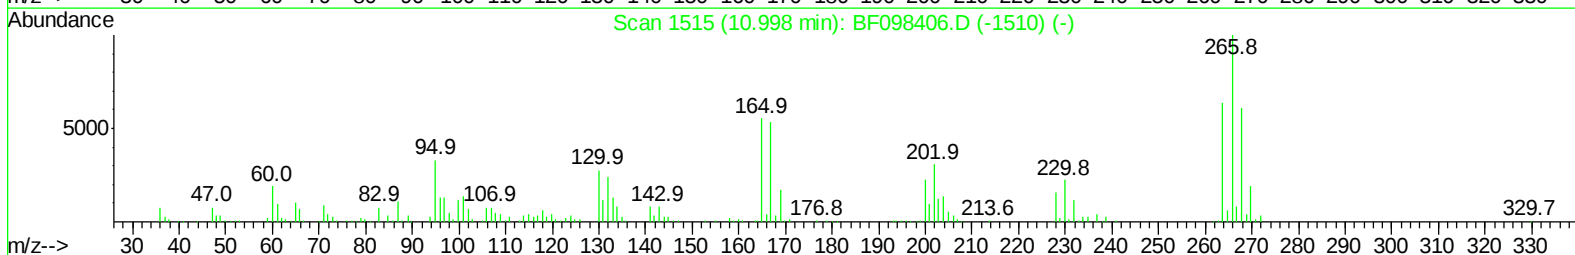
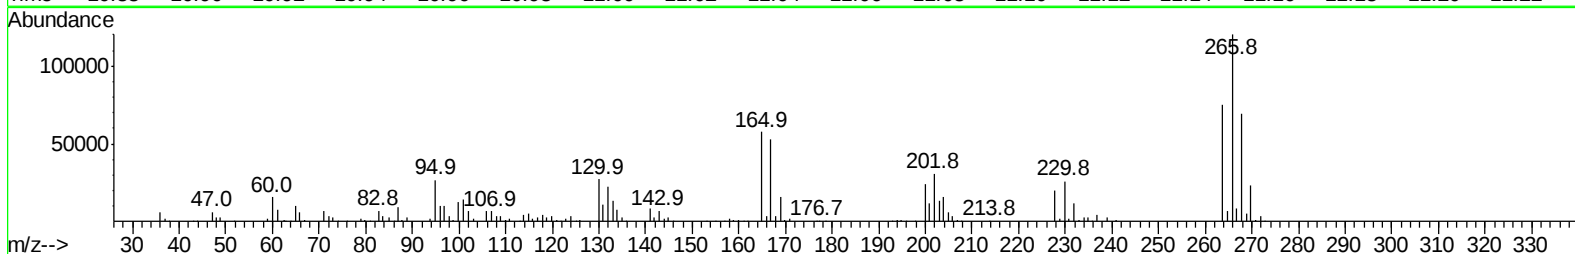


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF091417\
Data File : BF098518.D
Acq On : 14 Sep 2017 9:19
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 18:11:32 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 14 17:58:04 2017
Response via : Initial Calibration

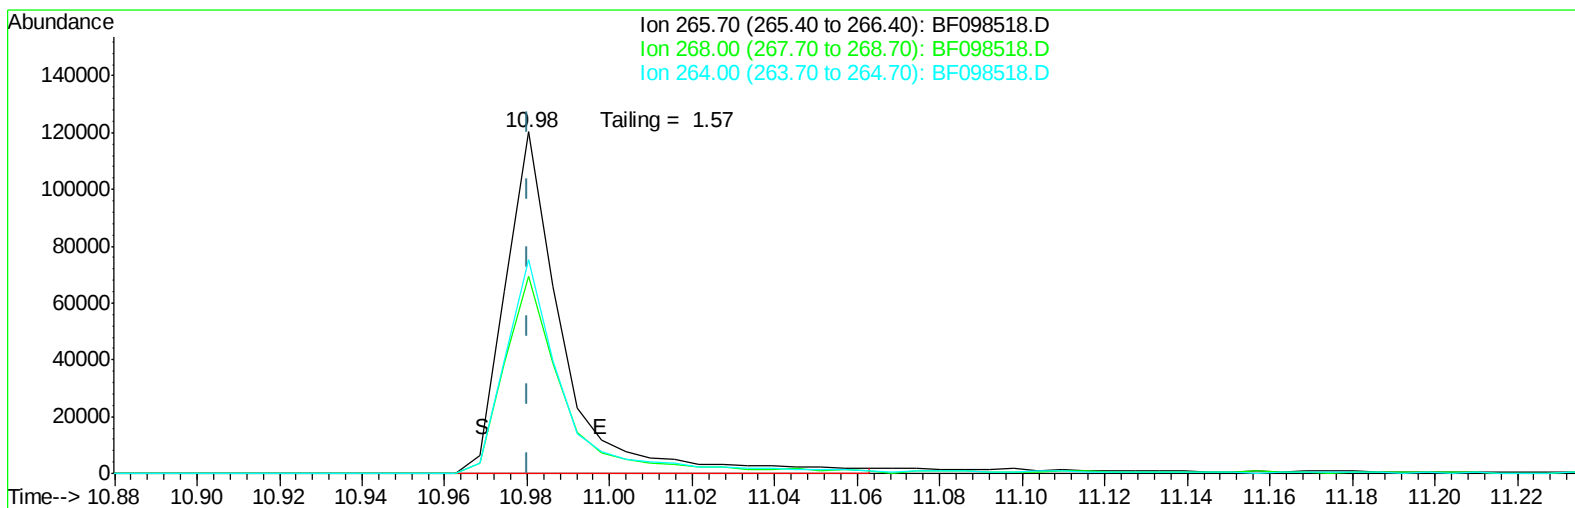

TIC: BF098518.D

(69) Pentachlorophenol (C)




10.980min (+0.000) 37755.64ng

response 118897

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	57.58
264.00	64.60	62.51
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF091417\
 Data File : BF098518.D
 Acq On : 14 Sep 2017 9:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 18:11:32 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 14 17:58:04 2017
 Response via : Initial Calibration

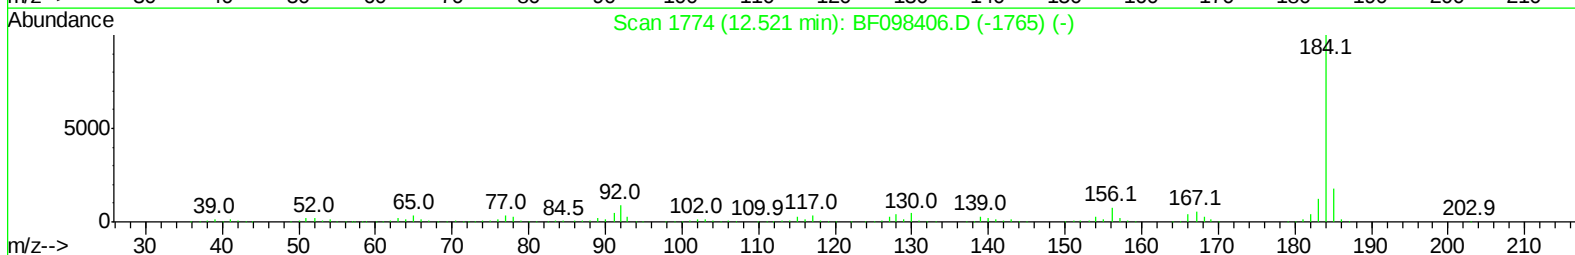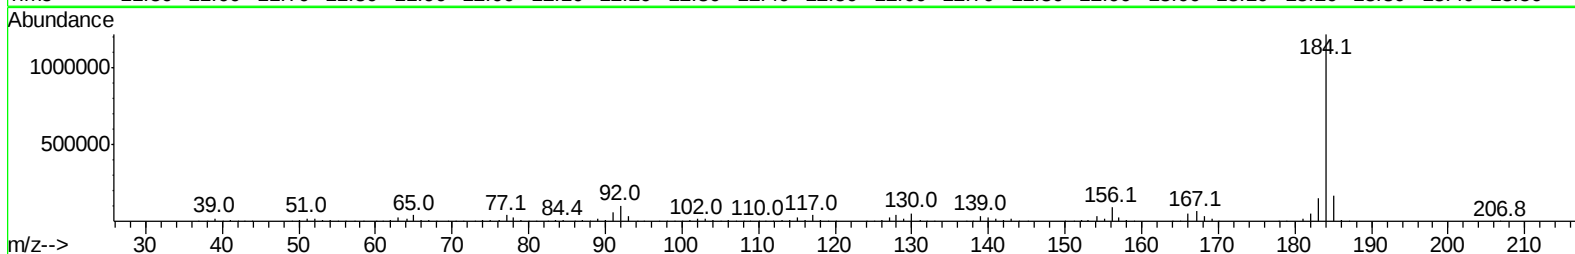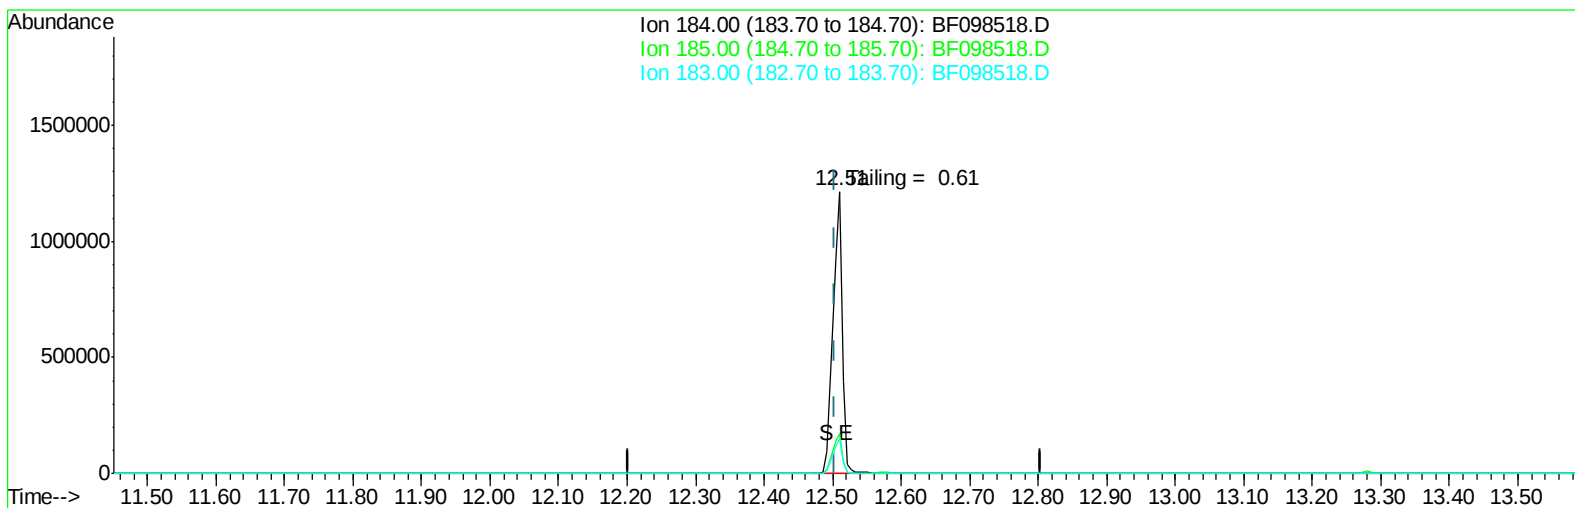

TIC: BF098518.D

(76) Benzidine

12.510min (+0.006) 0.00ng

response 1115000

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.03#
183.00	12.20	12.33
0.00	0.00	0.00