


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF091417\
 Data File : BF098518.D
 Acq On : 14 Sep 2017 9:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 02:14:50 2017

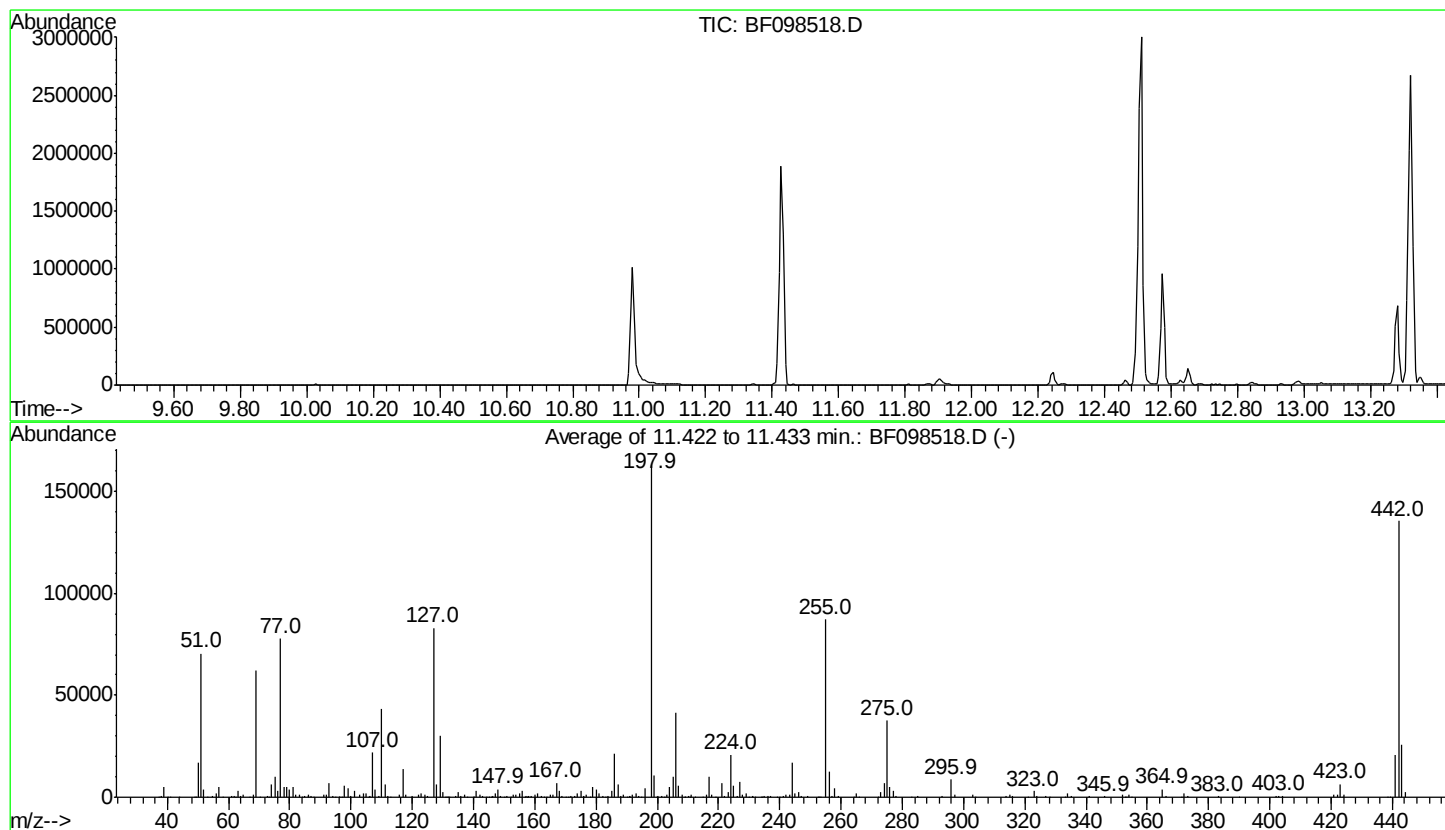

AutoFind: Scans 1587, 1588, 1589; Background Corrected with Scan 1581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.3	70493	PASS
68	69	0.00	2	2.0	1274	PASS
69	198	0.00	100	38.3	62256	PASS
70	69	0.00	2	0.3	196	PASS
127	198	10	80	51.0	82976	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	162645	PASS
199	198	5	9	6.7	10839	PASS
275	198	10	60	23.2	37661	PASS
365	198	1	100	2.4	3964	PASS
441	442	0.01	24	15.2	20583	PASS
442	198	50	100	83.3	135442	PASS
443	442	15	24	18.8	25467	PASS