


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF091417\
 Data File : BF098531.D
 Acq On : 14 Sep 2017 16:34
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 02:14:50 2017

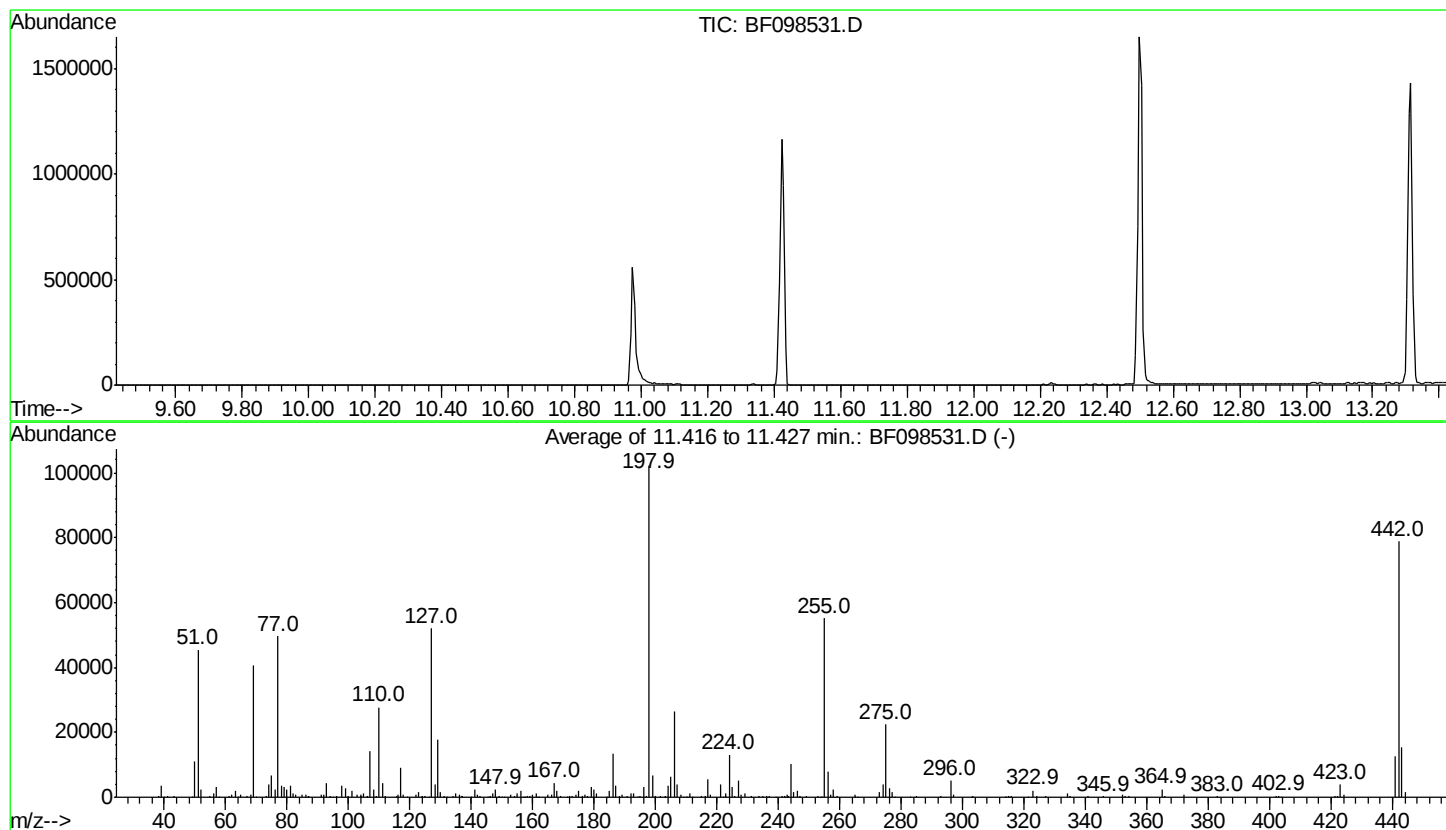

AutoFind: Scans 1586, 1587, 1588; Background Corrected with Scan 1581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	45458	PASS
68	69	0.00	2	2.0	822	PASS
69	198	0.00	100	39.8	40725	PASS
70	69	0.00	2	0.5	205	PASS
127	198	10	80	50.8	51952	PASS
197	198	0.00	2	0.2	226	PASS
198	198	100	100	100.0	102218	PASS
199	198	5	9	6.4	6573	PASS
275	198	10	60	21.9	22404	PASS
365	198	1	100	2.4	2467	PASS
441	442	0.01	24	16.3	12821	PASS
442	198	50	100	77.1	78778	PASS
443	442	15	24	19.4	15300	PASS