
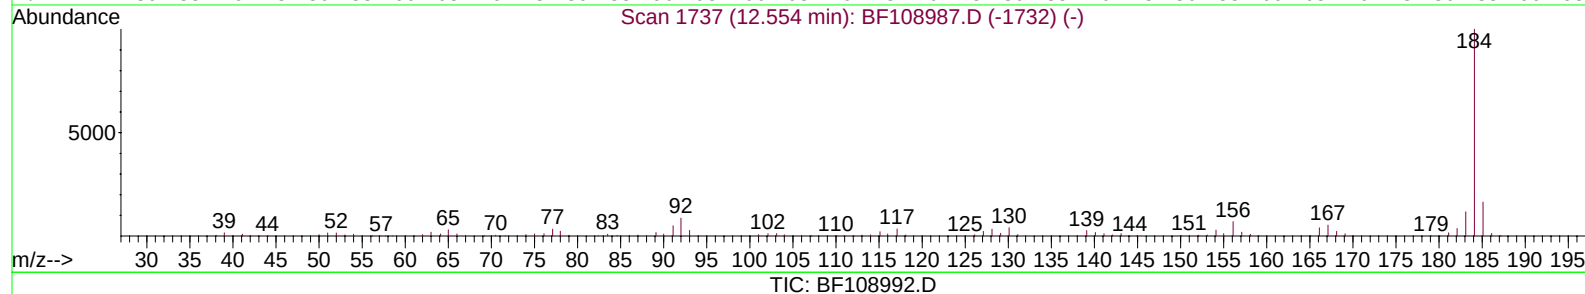
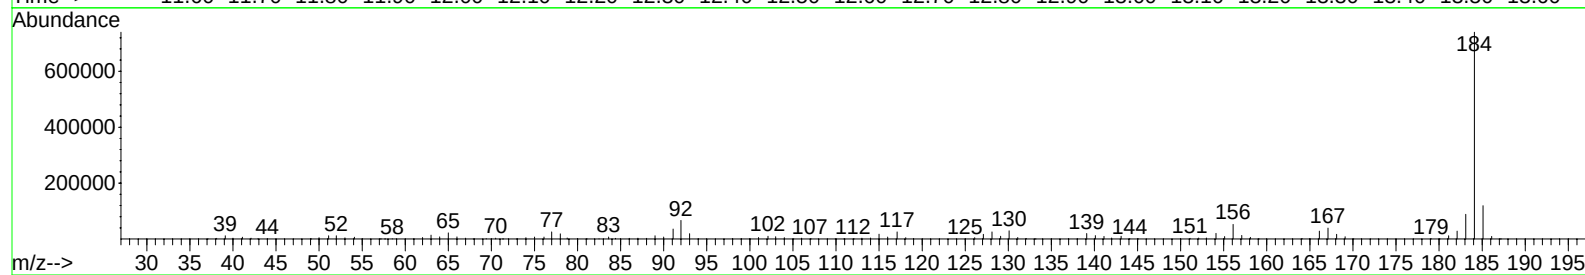


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF091418\
 Data File : BF108992.D
 Acq On : 14 Sep 2018 14:06
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 17:29:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 14 13:26:52 2018
 Response via : Initial Calibration

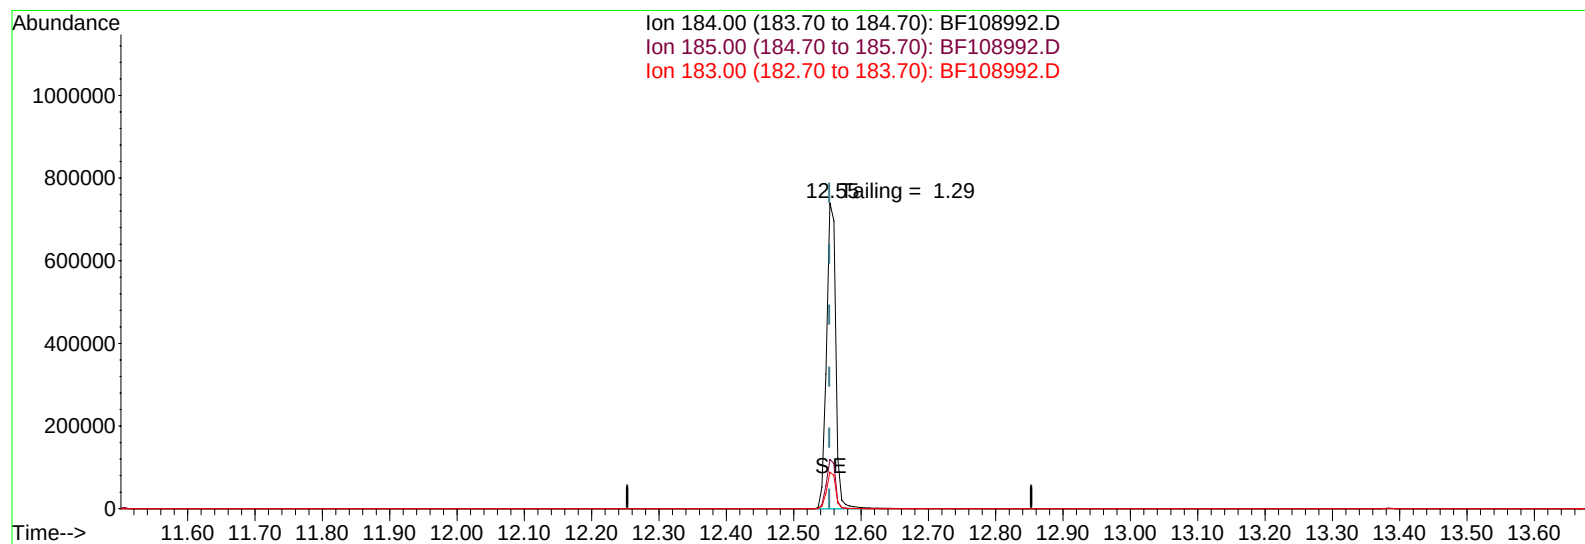

(76) Benzidine




12.554min (+0.001) 0.00ng

response 706936

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.10
183.00	11.60	11.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF091418\
 Data File : BF108992.D
 Acq On : 14 Sep 2018 14:06
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 17:29:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 14 13:26:52 2018
 Response via : Initial Calibration

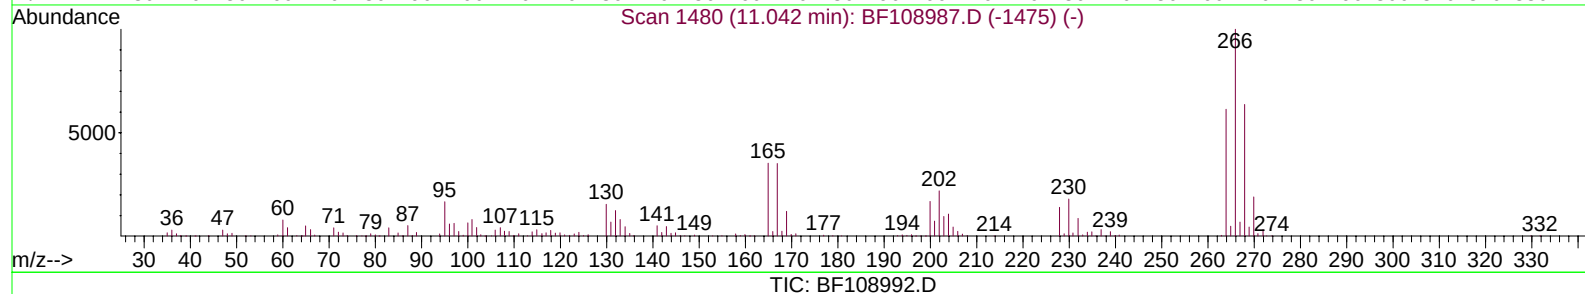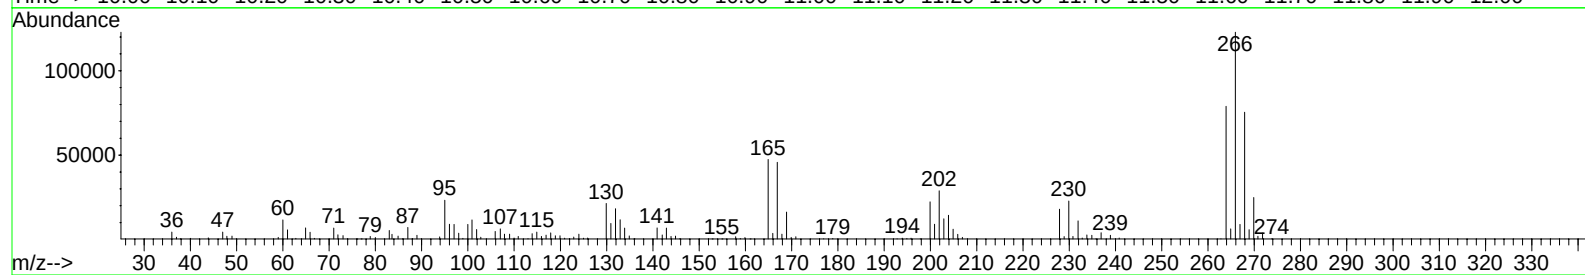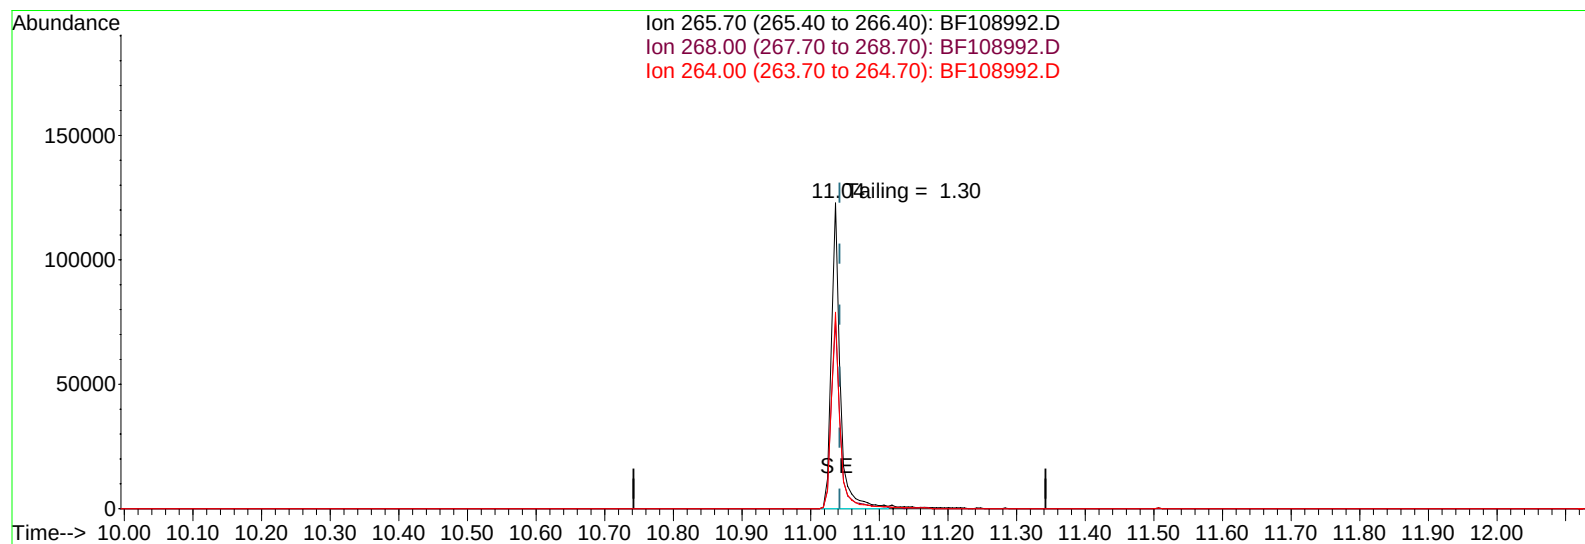

(69) Pentachlorophenol (C)

11.036min (-0.006) 38031.79ng

response 111793

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.37
264.00	61.90	64.27
0.00	0.00	0.00