

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091418\
 Data File : BF109022.D
 Acq On : 15 Sep 2018 4:08
 Operator : JU/SJ
 Sample : J4901-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 091218-DBRI-F-D-B

Quant Time: Sep 15 07:06:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 14 13:26:52 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.72	152	147262	20.00	ng	0.00
21) Naphthalene-d8	8.00	136	561767	20.00	ng	0.00
38) Acenaphthene-d10	9.75	164	268678	20.00	ng	0.00
63) Phenanthrene-d10	11.22	188	507864	20.00	ng	0.00
75) Chrysene-d12	13.85	240	360059	20.00	ng	-0.01
86) Perylene-d12	15.25	264	375893	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	348807	39.34	ng	0.00
7) Phenol-d6	6.34	99	285724	24.99	ng	-0.02
23) Nitrobenzene-d5	7.28	82	902164	90.07	ng	-0.01
41) 2,4,6-Tribromophenol	10.53	330	256916	88.11	ng	-0.01
44) 2-Fluorobiphenyl	9.08	172	1511050	88.11	ng	0.00
78) Terphenyl-d14	12.81	244	1538881	101.30	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.47	163	130173	6.779	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091418\
Data File : BF109022.D
Acq On : 15 Sep 2018 4:08
Operator : JU/SJ
Sample : J4901-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
091218-DBRI-F-D-B

Quant Time: Sep 15 07:06:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 14 13:26:52 2018
Response via : Initial Calibration

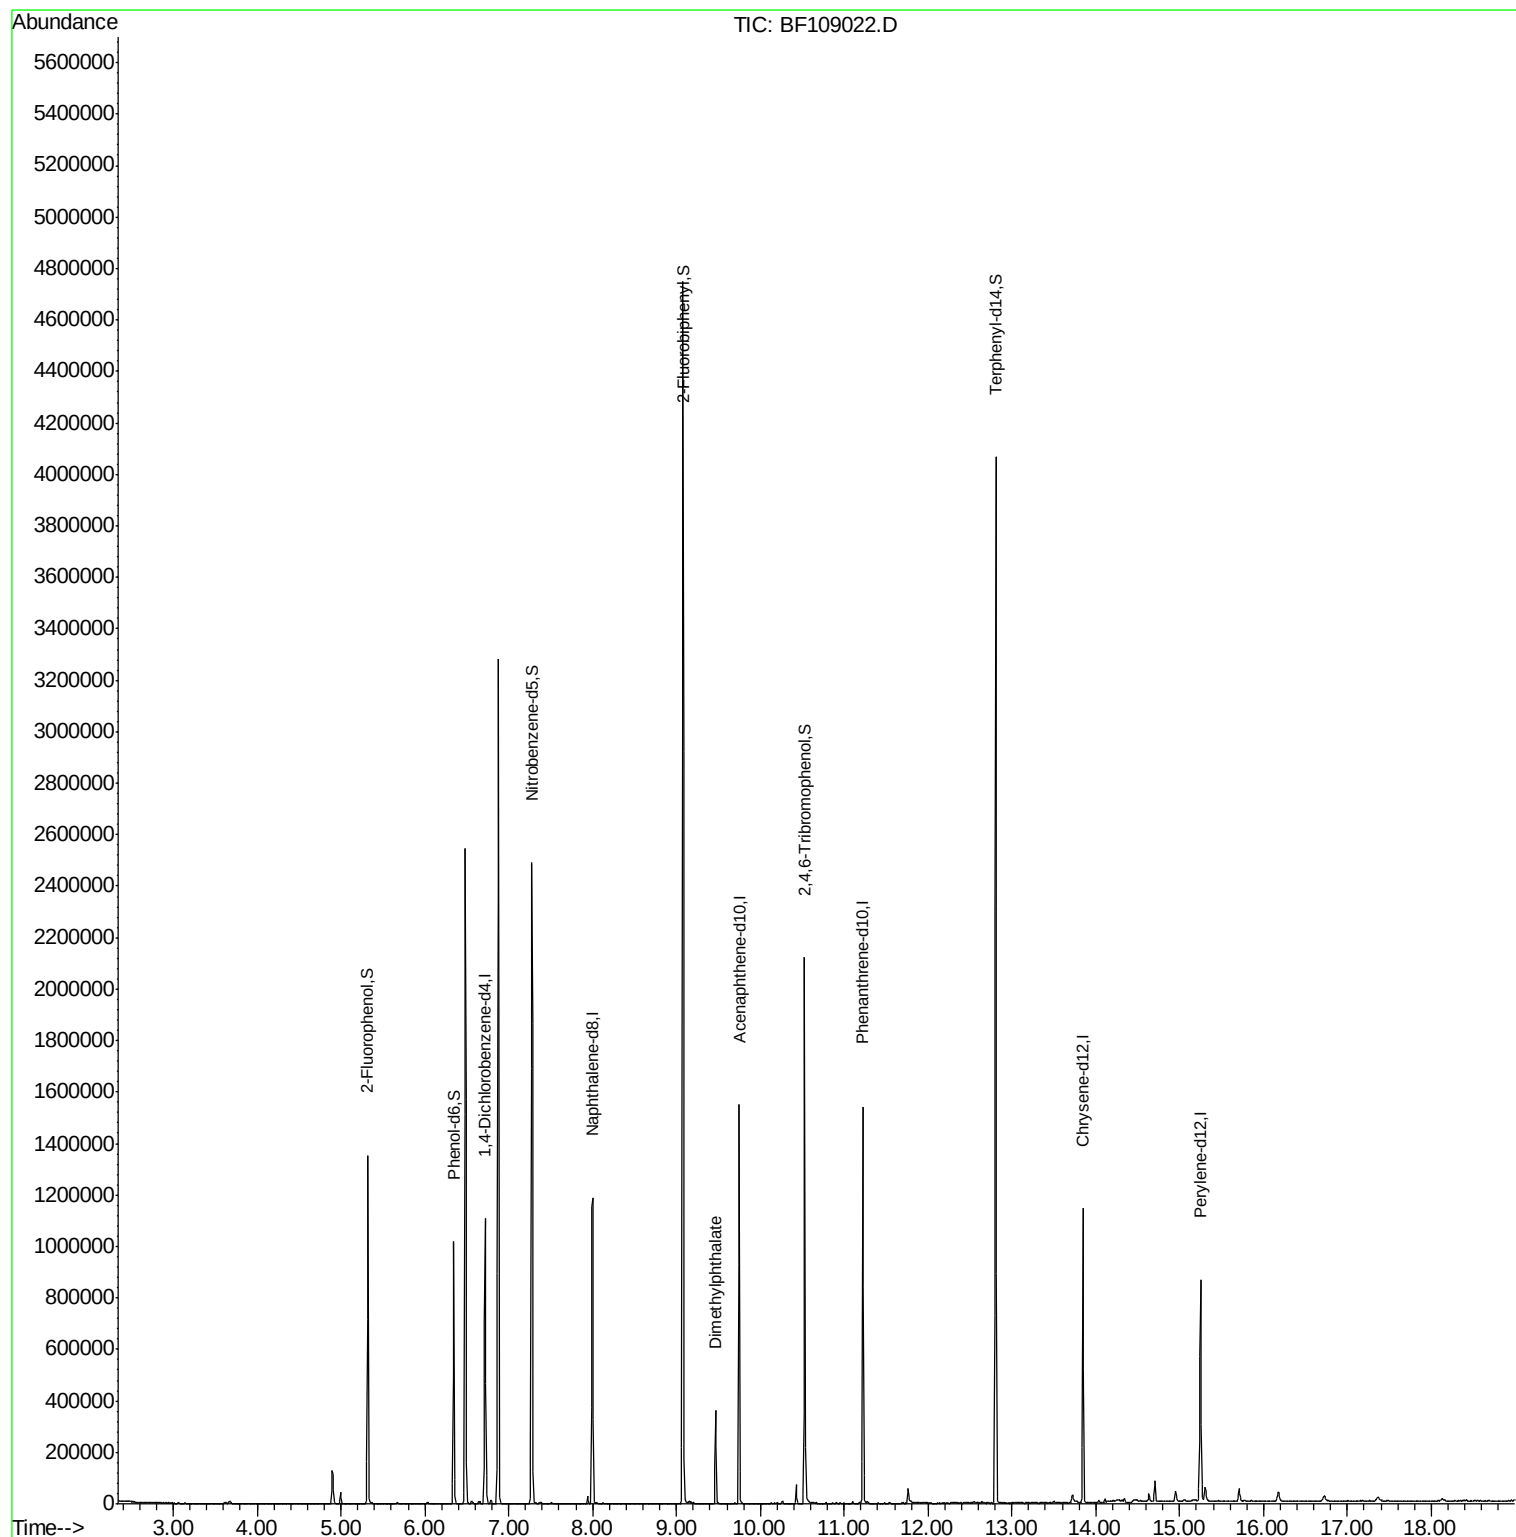

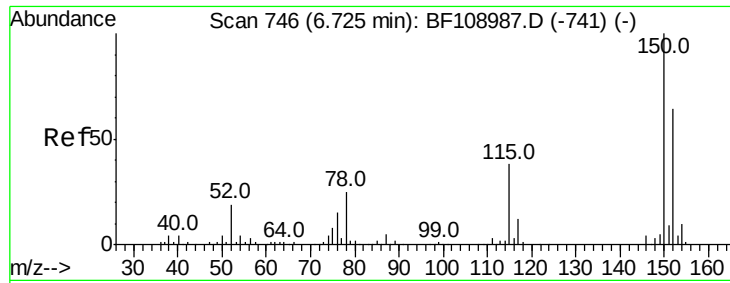


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.72 min Scan# 745
 Delta R.T. -0.01 min
 Lab File: BF109022.D
 Acq: 15 Sep 2018 4:08

Instrument :
 BNA_F
 ClientSampleId :
 091218-DBRI-F-D-B

Tot Ion	Ratio	Lower	Upper
152	100		
150	154.0	124.6	186.8
115	60.7	50.1	75.1

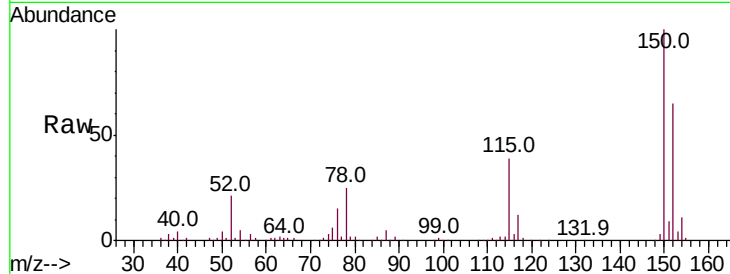


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

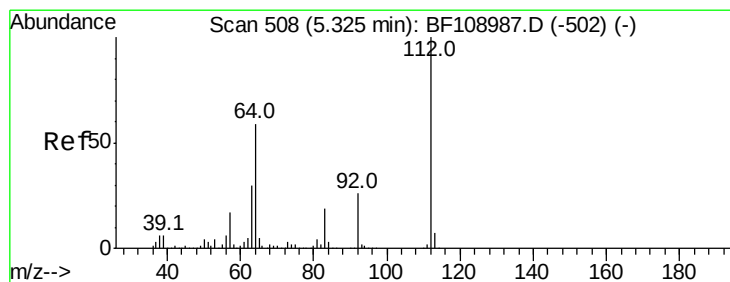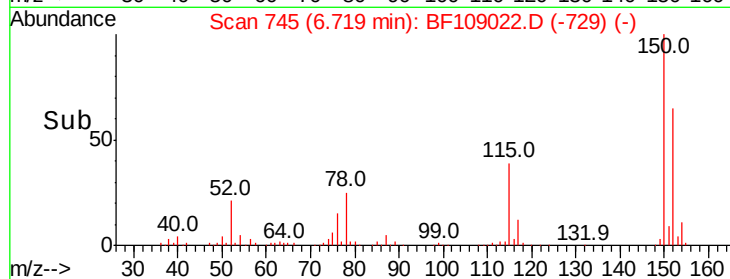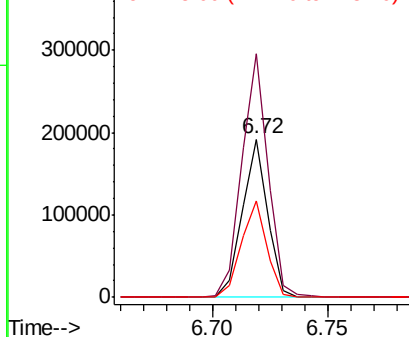



#5


2-Fluorophenol
 Concen: 39.340 ng
 RT: 5.32 min Scan# 507
 Delta R.T. -0.00 min
 Lab File: BF109022.D
 Acq: 15 Sep 2018 4:08

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.4	47.9	71.9
63	30.6	23.7	35.5

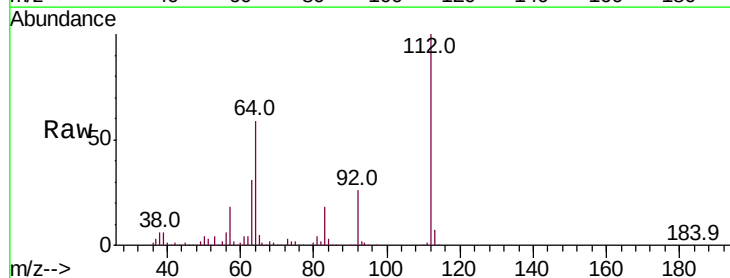

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

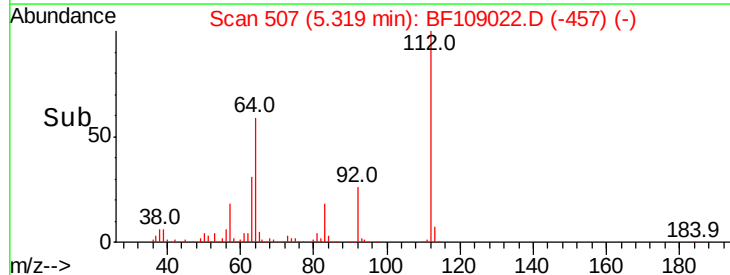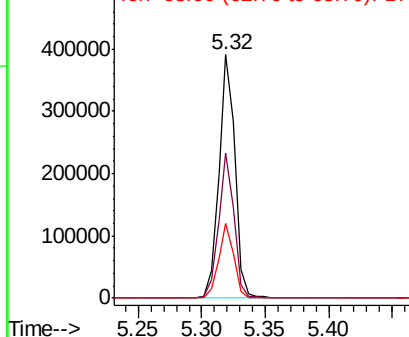

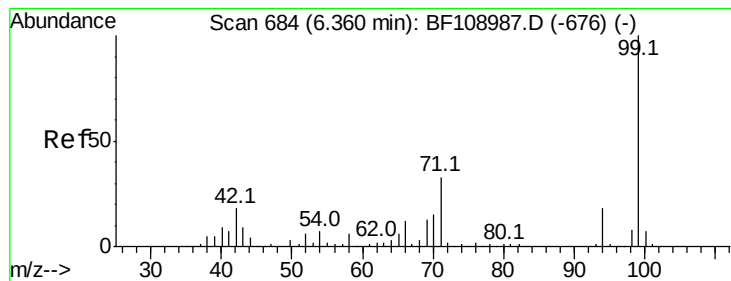

#7

Phenol-d6

Concen: 24.991 ng

RT: 6.34 min Scan# 681

Delta R.T. -0.02 min

Lab File: BF109022.D

Acq: 15 Sep 2018 4:08

Instrument :

BNA_F

ClientSampleId :

091218-DBRI-F-D-B





Tot Ion: 99 Resp: 285724

Ion Ratio Lower Upper

99 100

42 18.0 14.5 21.7

71 32.4 25.4 38.0

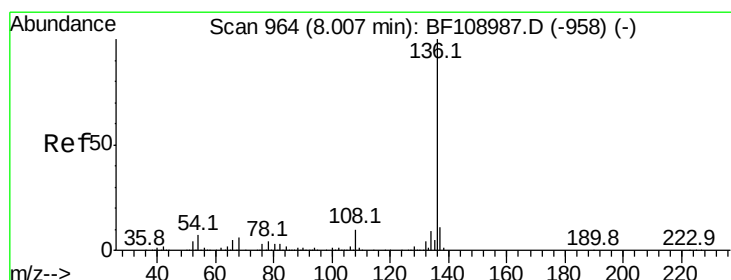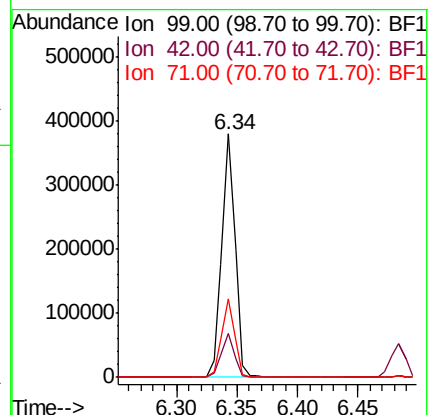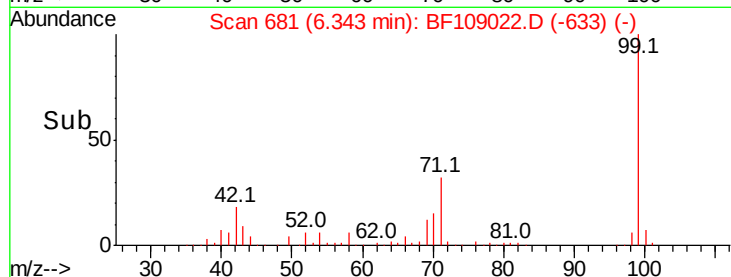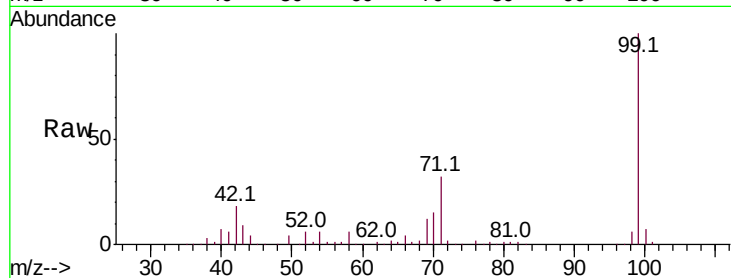

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.00 min Scan# 963

Delta R.T. -0.01 min

Lab File: BF109022.D

Acq: 15 Sep 2018 4:08

Tgt Ion: 136 Resp: 561767




Ion Ratio Lower Upper


136 100

137 10.9 8.9 13.3

54 6.8 6.6 9.8

68 5.8 5.0 7.4

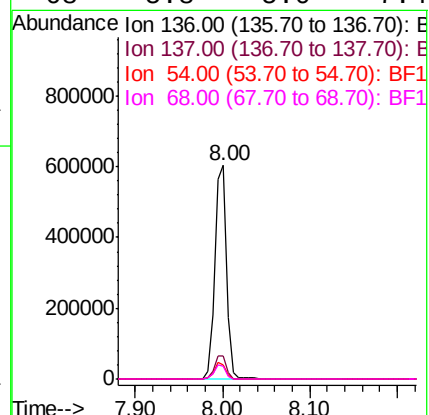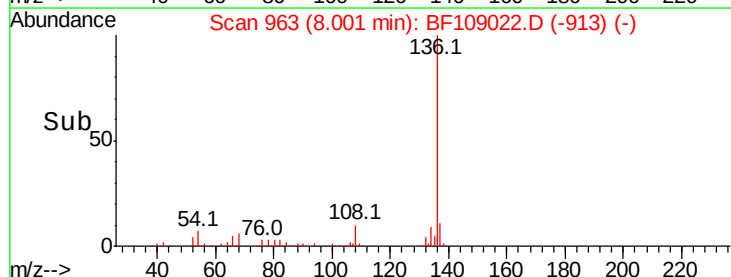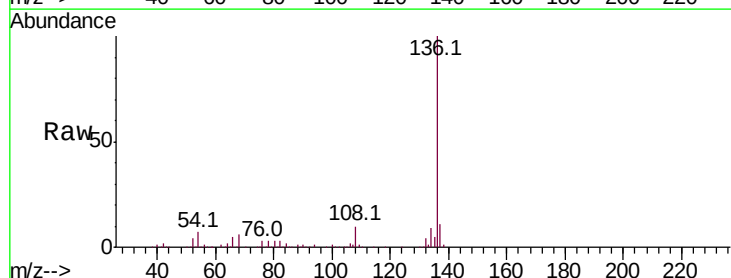


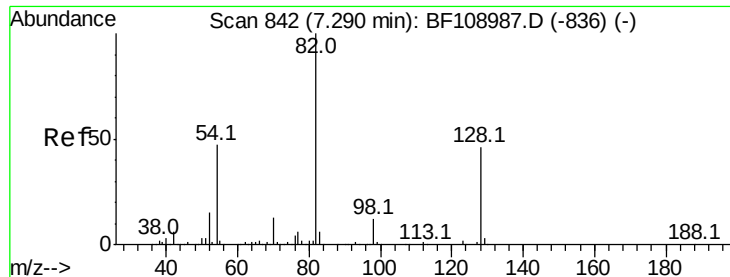




#23
Nitrobenzene-d5
Concen: 90.074 ng
RT: 7.28 min Scan# 840
Delta R.T. -0.01 min
Lab File: BF109022.D
Acq: 15 Sep 2018 4:08

Instrument :
BNA_F
ClientSampleId :
091218-DBRI-F-D-B

Tot Ion	82	Resp	902164
Ion Ratio	100	Lower	Upper
128	42.5	36.1	54.1
54	48.1	41.4	62.2

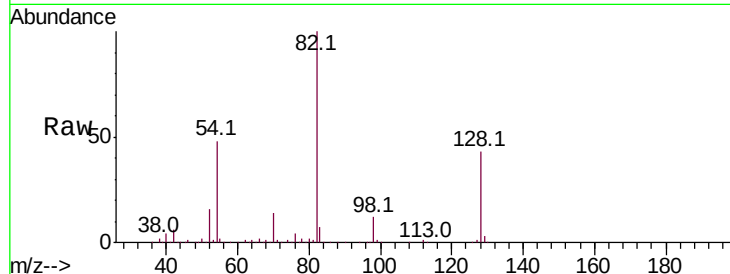


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

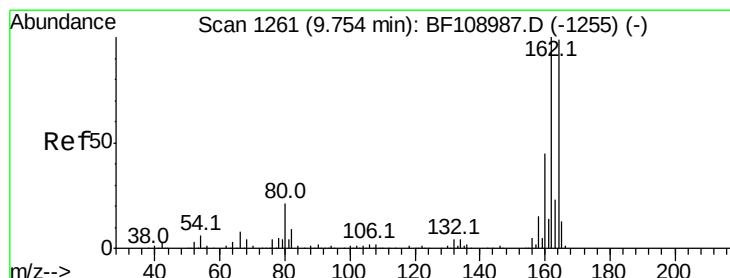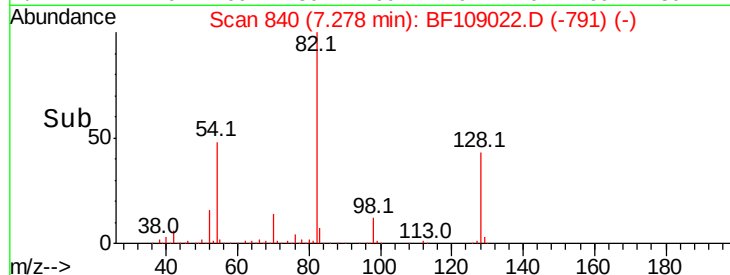
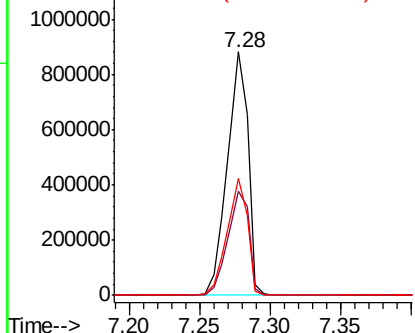



#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.75 min Scan# 1260
Delta R.T. -0.01 min
Lab File: BF109022.D
Acq: 15 Sep 2018 4:08

Tgt Ion	164	Resp	268678
Ion Ratio	100	Lower	Upper
162	102.8	86.1	129.1
160	46.1	38.3	57.5

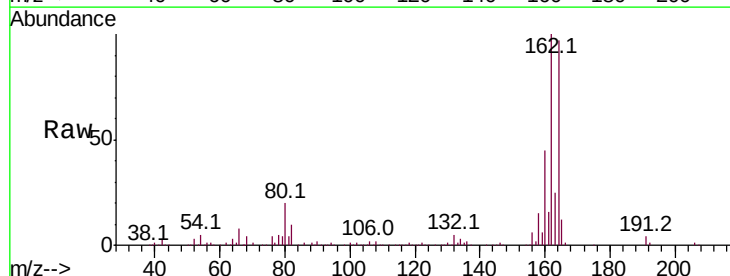

Abundance Ion 164.00 (163.70 to 164.70): BF1
Ion 162.00 (161.70 to 162.70): BF1
Ion 160.00 (159.70 to 160.70): BF1

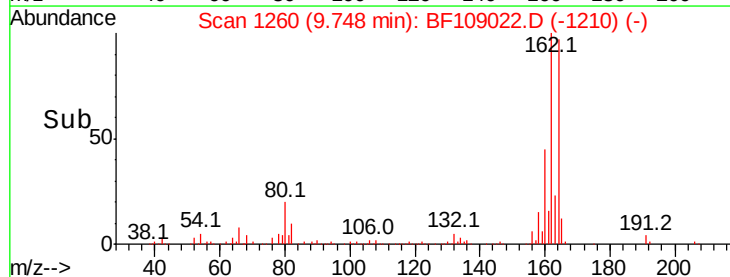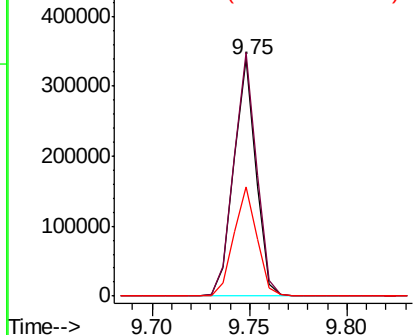


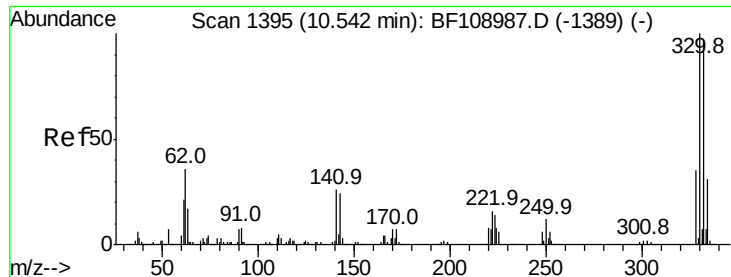




#41
 2,4,6-Tribromophenol
 Concen: 88.109 ng
 RT: 10.53 min Scan# 1393
 Delta R.T. -0.01 min
 Lab File: BF109022.D
 Acq: 15 Sep 2018 4:08

Instrument :
 BNA_F
 ClientSampleId :
 091218-DBRI-F-D-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.0	77.0	115.6
141	32.0	29.9	44.9

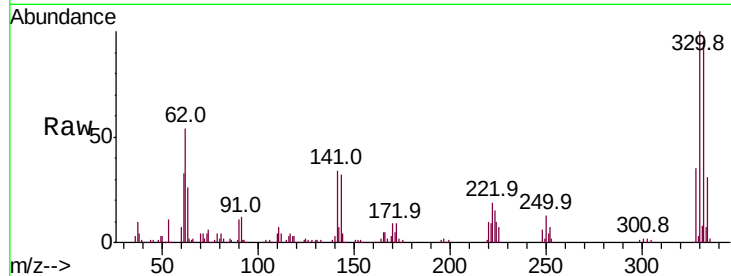


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

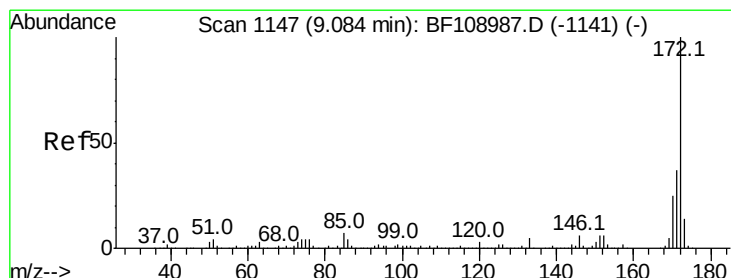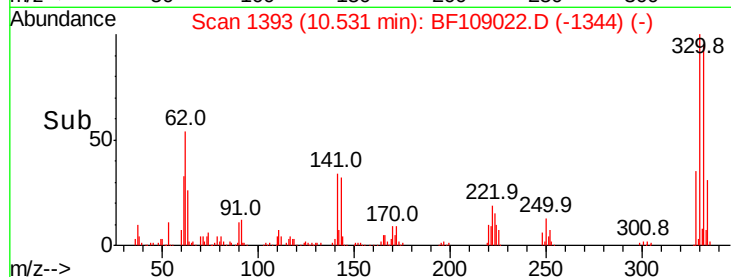
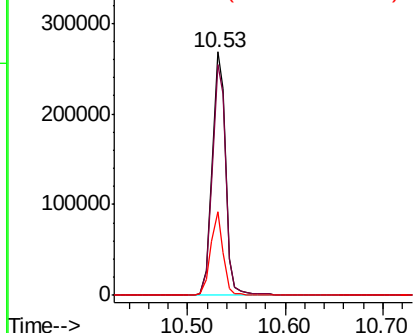



#44
 2-Fluorobiphenyl
 Concen: 88.113 ng
 RT: 9.08 min Scan# 1146
 Delta R.T. -0.01 min
 Lab File: BF109022.D
 Acq: 15 Sep 2018 4:08

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.3	29.7	44.5
170	24.6	19.6	29.4

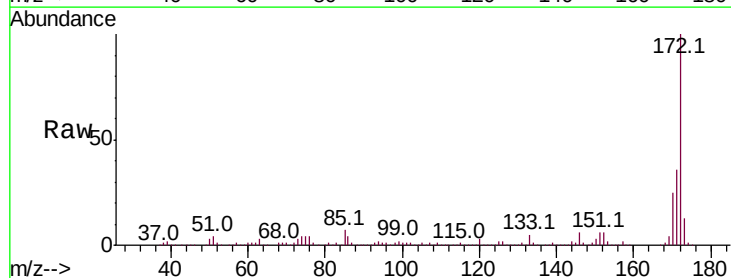

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

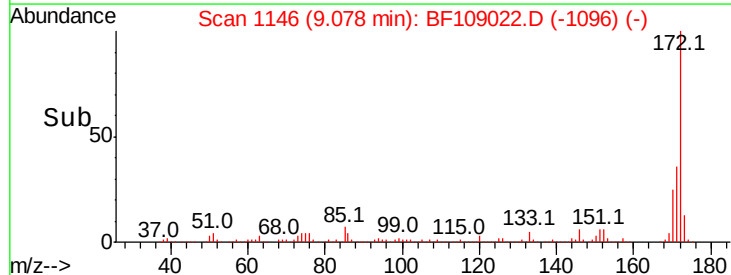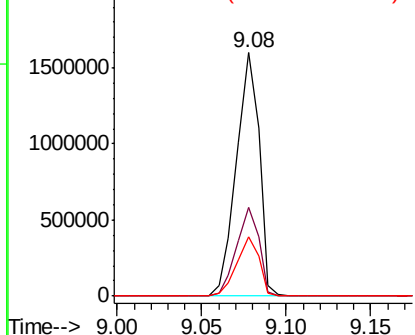

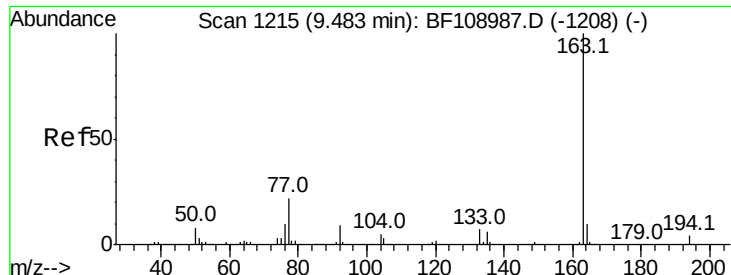

#49

Dimethylphthalate

Concen: 6.779 ng

RT: 9.47 min Scan# 1212

Delta R.T. -0.02 min

Lab File: BF109022.D

Acq: 15 Sep 2018 4:08

Instrument :

BNA_F

ClientSampleId :

091218-DBRI-F-D-B


Tot Ion:163 Resp: 130173

Ion Ratio Lower Upper




163 100

194 3.9 2.7 4.1

164 10.2 8.2 12.2

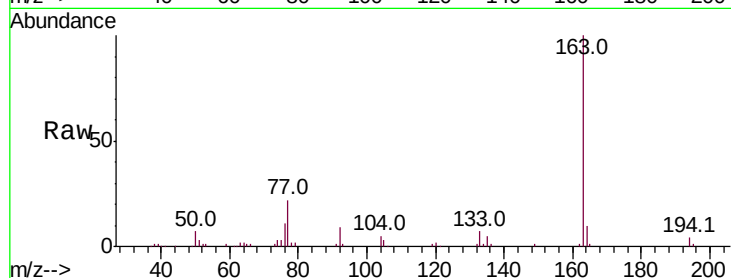

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

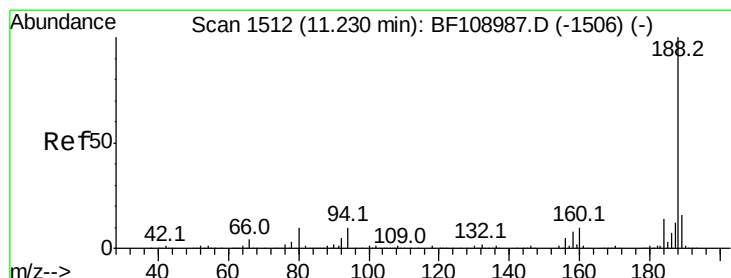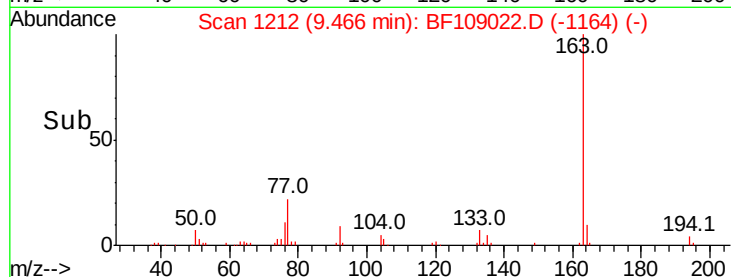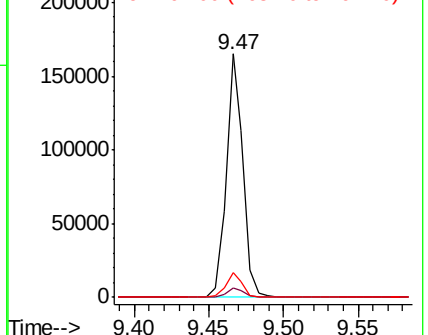

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.22 min Scan# 1511

Delta R.T. -0.01 min

Lab File: BF109022.D

Acq: 15 Sep 2018 4:08


Tgt Ion:188 Resp: 507864

Ion Ratio Lower Upper



188 100


94 10.0 8.5 12.7

80 10.8 9.2 13.8

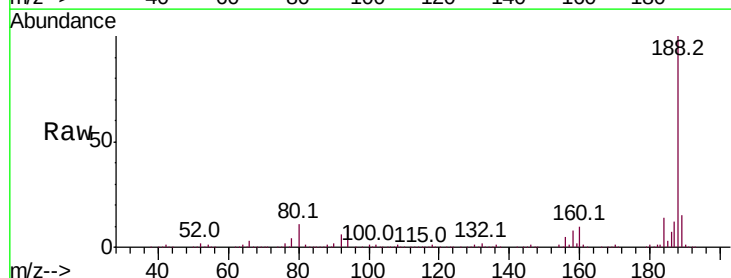

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

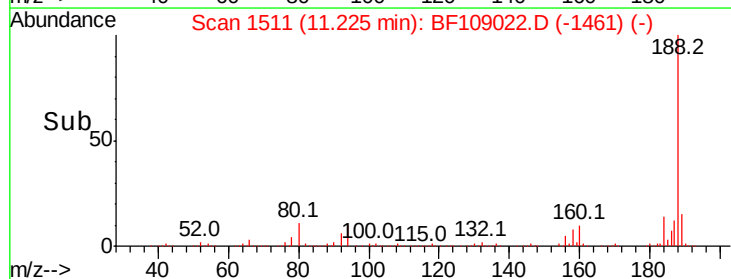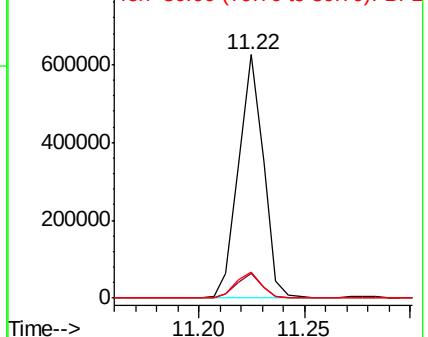

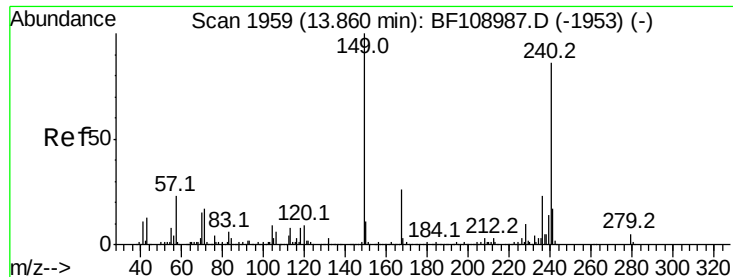

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.85 min Scan# 1957

Delta R.T. -0.01 min

Lab File: BF109022.D

Acq: 15 Sep 2018 4:08

Instrument :

BNA_F

ClientSampleId :

091218-DBRI-F-D-B


Tot Ion:240 Resp: 360059

Ion Ratio Lower Upper

240 100

120 12.0 9.5 14.3




236 26.2 20.7 31.1

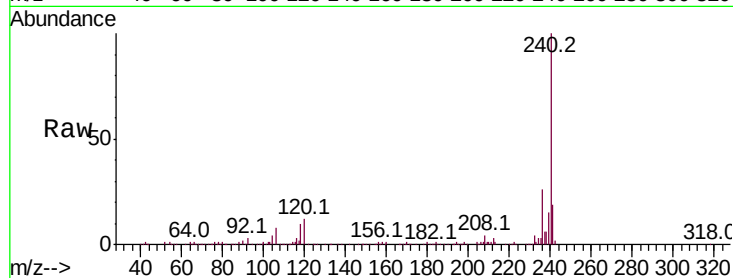

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

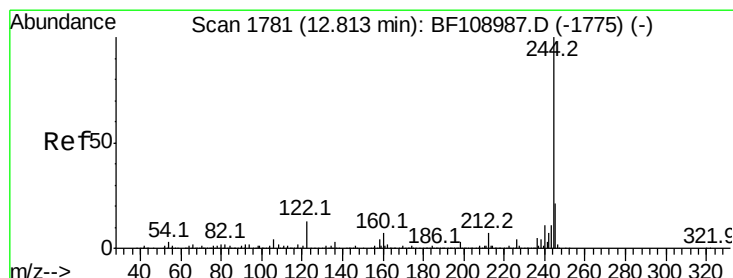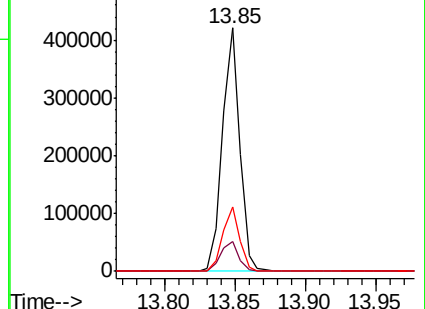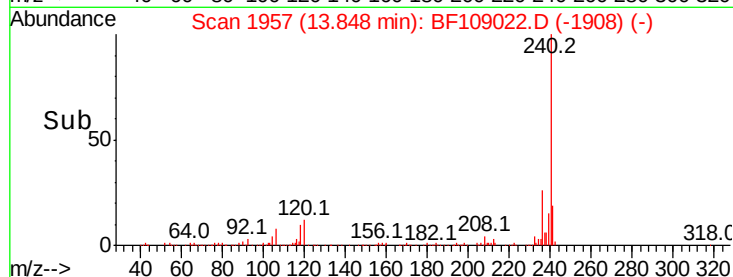

#78

Terphenyl-d14

Concen: 101.304 ng

RT: 12.81 min Scan# 1781

Delta R.T. 0.00 min

Lab File: BF109022.D

Acq: 15 Sep 2018 4:08


Tgt Ion:244 Resp: 1538881

Ion Ratio Lower Upper

244 100

212 6.9 5.4 8.0



122 11.0 11.0 16.4#

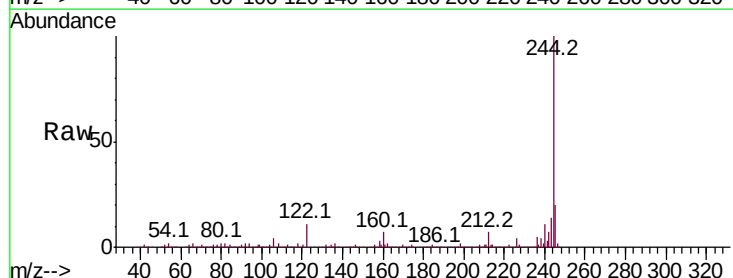


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

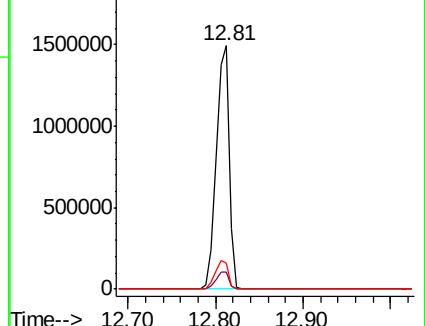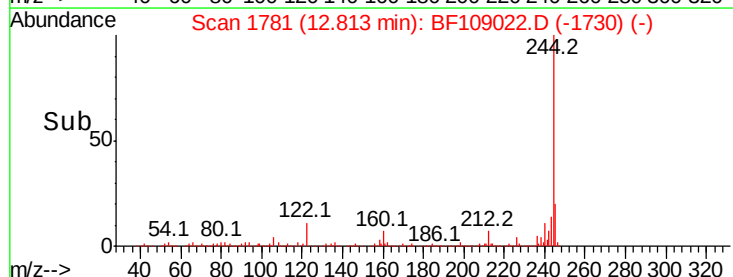

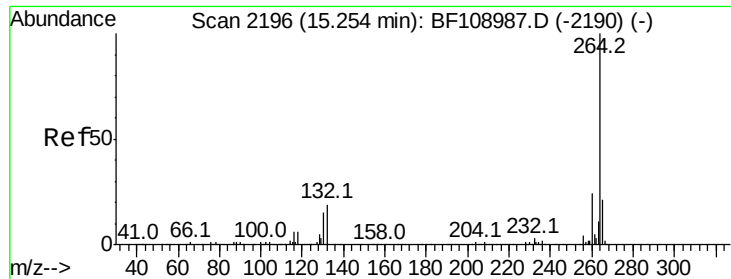

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.25 min Scan# 2195
Delta R.T. -0.01 min
Lab File: BF109022.D
Acq: 15 Sep 2018 4:08

Instrument :
BNA_F
ClientSampleId :
091218-DBRI-F-D-B

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.4	19.2	28.8
265	22.2	17.5	26.3

