

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091418\
 Data File : BF108999.D
 Acq On : 14 Sep 2018 17:16
 Operator : JU/SJ
 Sample : J4898-01DL 50X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ROLLOFF01-COMP-FILLDL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.295	499	503	504	rBV	103986	99784	3.40%	0.250%
2	5.313	504	506	511	rVB2	84831	76801	2.62%	0.193%
3	6.548	713	716	719	rBV2	160841	143827	4.90%	0.361%
4	6.719	741	745	749	rBV	1112141	870596	29.67%	2.183%
5	6.978	786	789	793	rBV	371152	310519	10.58%	0.779%
6	7.425	861	865	868	rBV	86986	88542	3.02%	0.222%
7	7.754	914	921	924	rBV3	128177	141422	4.82%	0.355%
8	7.784	924	926	935	rVB	100990	127393	4.34%	0.320%
9	8.001	959	963	965	rBV	1344624	1443437	49.19%	3.620%
10	8.025	965	967	970	rVV	3708667	2934461	100.00%	7.360%
11	8.072	970	975	979	rVV	202159	181575	6.19%	0.455%
12	8.713	1080	1084	1087	rBV	1703568	1314697	44.80%	3.297%
13	8.813	1095	1101	1104	rVB	933941	783624	26.70%	1.965%
14	9.172	1159	1162	1166	rBV	348536	301362	10.27%	0.756%
15	9.272	1176	1179	1184	rVB	82497	92490	3.15%	0.232%
16	9.336	1184	1190	1195	rVV	329883	458126	15.61%	1.149%
17	9.413	1198	1203	1205	rBV	485673	460501	15.69%	1.155%
18	9.436	1205	1207	1211	rVV	363742	281844	9.60%	0.707%
19	9.472	1211	1213	1216	rVV	91155	77149	2.63%	0.193%
20	9.525	1220	1222	1232	rVV	228492	262967	8.96%	0.660%
21	9.607	1232	1236	1242	rVB	471157	380610	12.97%	0.955%
22	9.748	1255	1260	1263	rBV2	1456860	1452337	49.49%	3.642%
23	9.783	1263	1266	1269	rVV	1313194	1043093	35.55%	2.616%
24	9.954	1291	1295	1298	rVB	1052075	848880	28.93%	2.129%
25	9.995	1298	1302	1305	rVB	123017	100932	3.44%	0.253%
26	10.066	1309	1314	1317	rBV2	109881	152555	5.20%	0.383%
27	10.095	1317	1319	1325	rVB2	134674	110477	3.76%	0.277%
28	10.160	1325	1330	1331	rBV2	98509	119651	4.08%	0.300%
29	10.201	1334	1337	1340	rVB	136837	113158	3.86%	0.284%
30	10.266	1345	1348	1350	rVV2	100790	102767	3.50%	0.258%
31	10.295	1350	1353	1358	rVB	1421633	1175580	40.06%	2.948%
32	10.401	1369	1371	1377	rVB2	84811	104948	3.58%	0.263%
33	10.454	1377	1380	1382	rBV	281414	233217	7.95%	0.585%
34	10.513	1387	1390	1391	rVV	238915	182860	6.23%	0.459%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091418\
 Data File : BF108999.D
 Acq On : 14 Sep 2018 17:16
 Operator : JU/SJ
 Sample : J4898-01DL 50X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ROLLOFF01-COMP-FILLDL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.530	1391	1393	1397	rVV	357193	392273	13.37%	0.984%
36	10.842	1441	1446	1448	rBV	200125	232186	7.91%	0.582%
37	10.866	1448	1450	1453	rVB	107650	91047	3.10%	0.228%
38	10.925	1457	1460	1463	rBV2	115936	106747	3.64%	0.268%
39	10.972	1463	1468	1470	rBV	107184	119975	4.09%	0.301%
40	10.989	1470	1471	1473	rVV	96432	77989	2.66%	0.196%
41	11.036	1477	1479	1483	rVB2	108306	98152	3.34%	0.246%
42	11.077	1483	1486	1490	rBV	127258	137133	4.67%	0.344%
43	11.119	1490	1493	1500	rVB	306931	345676	11.78%	0.867%
44	11.230	1507	1512	1513	rBV	1324819	1298458	44.25%	3.257%
45	11.254	1513	1516	1519	rVV	3395300	2934346	100.00%	7.359%
46	11.301	1519	1524	1527	rVB	1473638	1223483	41.69%	3.068%
47	11.336	1527	1530	1534	rBV2	115042	116846	3.98%	0.293%
48	11.454	1544	1550	1552	rBV	335157	338759	11.54%	0.850%
49	11.724	1593	1596	1598	rBV	342443	279446	9.52%	0.701%
50	11.754	1598	1601	1605	rVB	579934	482575	16.45%	1.210%
51	11.801	1605	1609	1612	rBV	342947	281643	9.60%	0.706%
52	11.836	1612	1615	1618	rBV	648085	690583	23.53%	1.732%
53	11.860	1618	1619	1622	rVB	270634	141024	4.81%	0.354%
54	12.019	1643	1646	1652	rVB	235196	218686	7.45%	0.548%
55	12.271	1684	1689	1692	rBV	165780	204197	6.96%	0.512%
56	12.313	1692	1696	1698	rVV3	152467	193624	6.60%	0.486%
57	12.371	1701	1706	1709	rVB4	71704	119503	4.07%	0.300%
58	12.436	1713	1717	1720	rBV	1879700	1696919	57.83%	4.256%
59	12.524	1729	1732	1735	rVB	294934	229898	7.83%	0.577%
60	12.583	1735	1742	1746	rBV3	74689	129683	4.42%	0.325%
61	12.660	1749	1755	1758	rVV2	1516965	1594100	54.32%	3.998%
62	12.707	1761	1763	1770	rVB2	124811	145627	4.96%	0.365%
63	12.777	1772	1775	1777	rVV	148352	114017	3.89%	0.286%
64	12.807	1777	1780	1786	rVB2	86805	119371	4.07%	0.299%
65	12.877	1786	1792	1795	rBV2	130143	224984	7.67%	0.564%
66	12.966	1804	1807	1808	rVV2	119790	135587	4.62%	0.340%
67	12.983	1808	1810	1814	rVB	381364	356187	12.14%	0.893%
68	13.054	1818	1822	1825	rVV	426371	397627	13.55%	0.997%
69	13.089	1825	1828	1832	rVV	234583	245495	8.37%	0.616%
70	13.154	1836	1839	1841	rVV2	118588	131618	4.49%	0.330%
71	13.177	1841	1843	1846	rVV	109137	119202	4.06%	0.299%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091418\
 Data File : BF108999.D
 Acq On : 14 Sep 2018 17:16
 Operator : JU/SJ
 Sample : J4898-01DL 50X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ROLLOFF01-COMP-FILLDL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	13.213	1846	1849	1858	rVB2	117917	174602	5.95%	0.438%
73	13.466	1889	1892	1896	rBV3	63855	91370	3.11%	0.229%
74	13.601	1909	1915	1918	rBV	103476	132540	4.52%	0.332%
75	13.630	1918	1920	1922	rVV	116051	93531	3.19%	0.235%
76	13.848	1952	1957	1960	rBV2	1319079	1735096	59.13%	4.352%
77	13.877	1960	1962	1964	rVB	473101	364762	12.43%	0.915%
78	14.036	1986	1989	1992	rVB	91116	75586	2.58%	0.190%
79	14.071	1992	1995	1999	rBV2	67967	73907	2.52%	0.185%
80	14.201	2014	2017	2019	rVV	64647	79367	2.70%	0.199%
81	14.236	2019	2023	2026	rVV	171186	204195	6.96%	0.512%
82	14.265	2026	2028	2032	rVV	81845	91537	3.12%	0.230%
83	14.330	2036	2039	2041	rVV2	102453	130367	4.44%	0.327%
84	14.377	2045	2047	2051	rVV4	103133	124723	4.25%	0.313%
85	14.430	2051	2056	2060	rVB4	43588	74993	2.56%	0.188%
86	14.560	2072	2078	2084	rVB7	35545	83575	2.85%	0.210%
87	14.636	2088	2091	2096	rVB3	76690	99395	3.39%	0.249%
88	14.860	2124	2129	2131	rBV	364914	513609	17.50%	1.288%
89	14.954	2142	2145	2150	rVB	181067	203871	6.95%	0.511%
90	15.136	2172	2176	2182	rVB	200114	240980	8.21%	0.604%
91	15.195	2182	2186	2191	rVB	389767	449294	15.31%	1.127%
92	15.254	2191	2196	2199	rBV	937340	1071860	36.53%	2.688%
93	15.277	2199	2200	2203	rVV	93183	95466	3.25%	0.239%
94	15.307	2203	2205	2211	rVB2	115022	141008	4.81%	0.354%
95	15.442	2220	2228	2229	rBV2	47020	85044	2.90%	0.213%
96	15.712	2268	2274	2281	rBV2	145297	252805	8.62%	0.634%
97	16.183	2347	2354	2362	rBV	115072	213954	7.29%	0.537%
98	16.595	2418	2424	2432	rVB2	163414	312253	10.64%	0.783%
99	16.995	2486	2492	2503	rBV	103836	222376	7.58%	0.558%
100	17.212	2524	2529	2535	rVB2	54518	103457	3.53%	0.259%


Sum of corrected areas: 39872371

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091418\
Data File : BF108999.D
Acq On : 14 Sep 2018 17:16
Operator : JU/SJ
Sample : J4898-01DL 50X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ROLLOFF01-COMP-FILLDL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

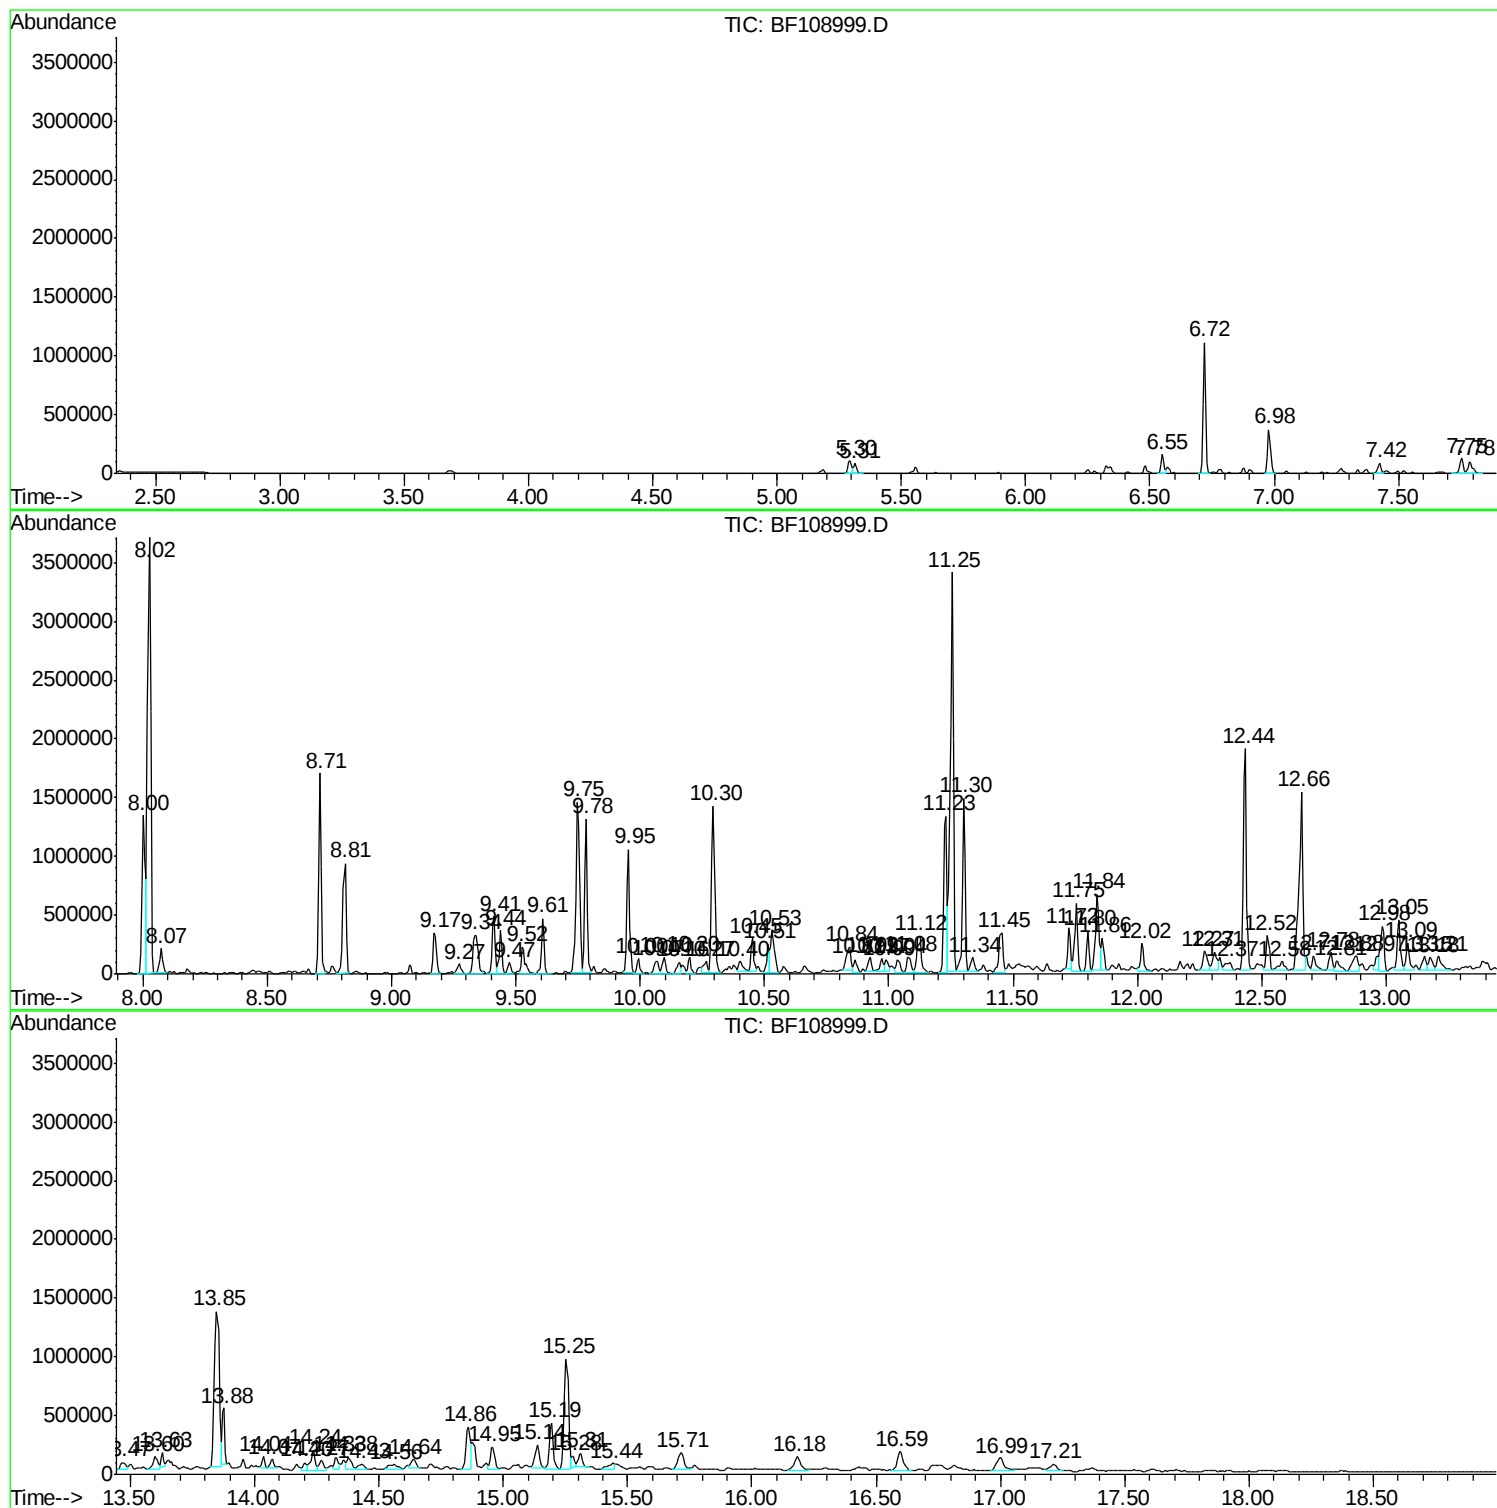

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091418\
Data_File : BF108999.D
Acq_On : 14 Sep 2018 17:166
Operator : JU/SJJ
Sample : J4898-01DL_50XX
Misc :
ALS_Vial : 8 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
ROLLOFF01-COMP-FILLDL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
