


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091418\
 Data File : BF108983.D
 Acq On : 14 Sep 2018 9:07
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 14 13:26:52 2018

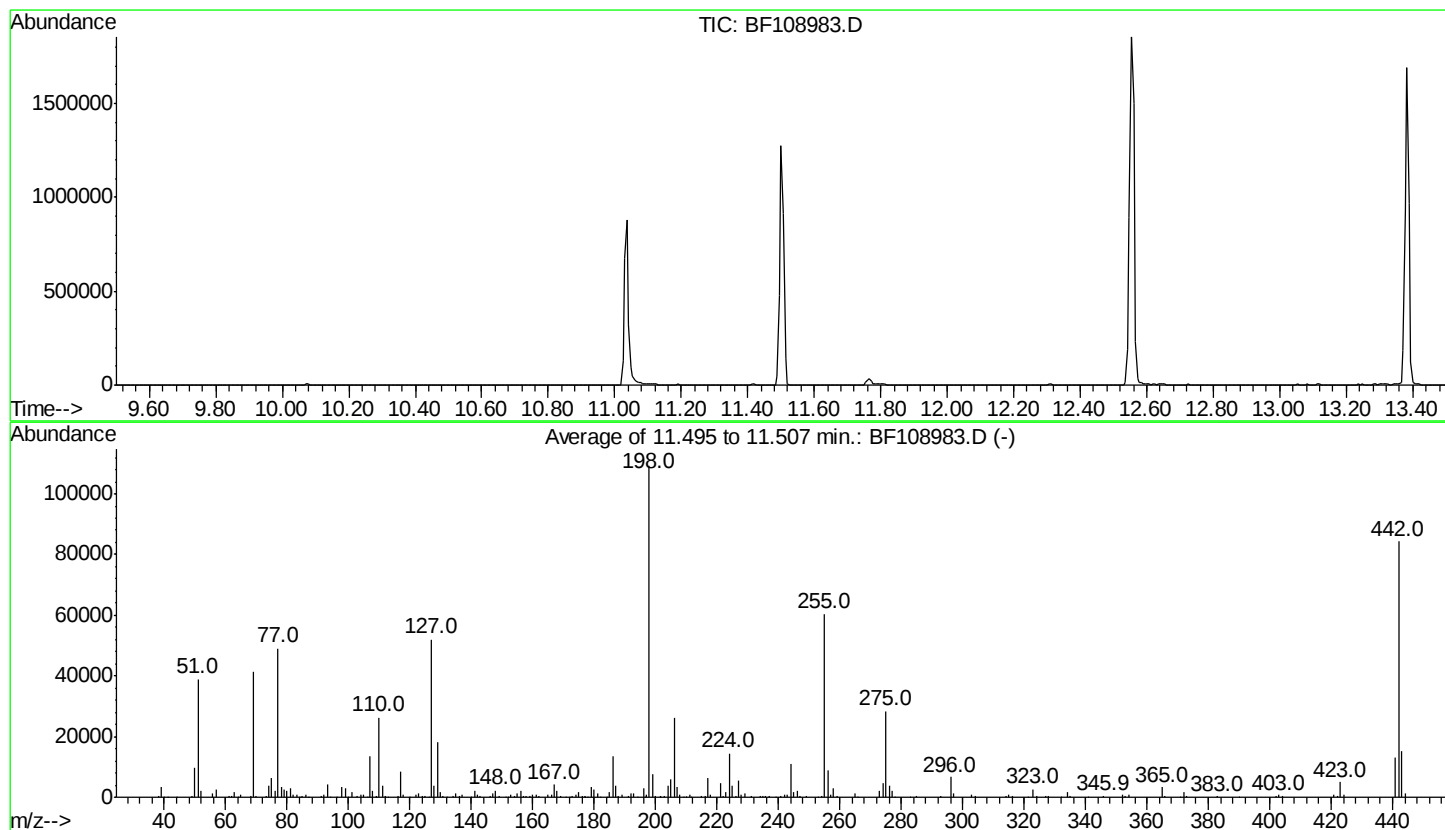

AutoFind: Scans 1557, 1558, 1559; Background Corrected with Scan 1553

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	38821	PASS
68	69	0.00	2	1.4	590	PASS
69	198	0.00	100	37.7	41157	PASS
70	69	0.00	2	0.6	240	PASS
127	198	10	80	47.5	51909	PASS
197	198	0.00	2	0.7	714	PASS
198	198	100	100	100.0	109301	PASS
199	198	5	9	7.0	7613	PASS
275	198	10	60	26.0	28455	PASS
365	198	1	100	3.0	3228	PASS
441	198	0.01	100	12.2	13282	PASS
442	198	50	100	77.2	84376	PASS
443	442	15	24	18.0	15164	PASS