
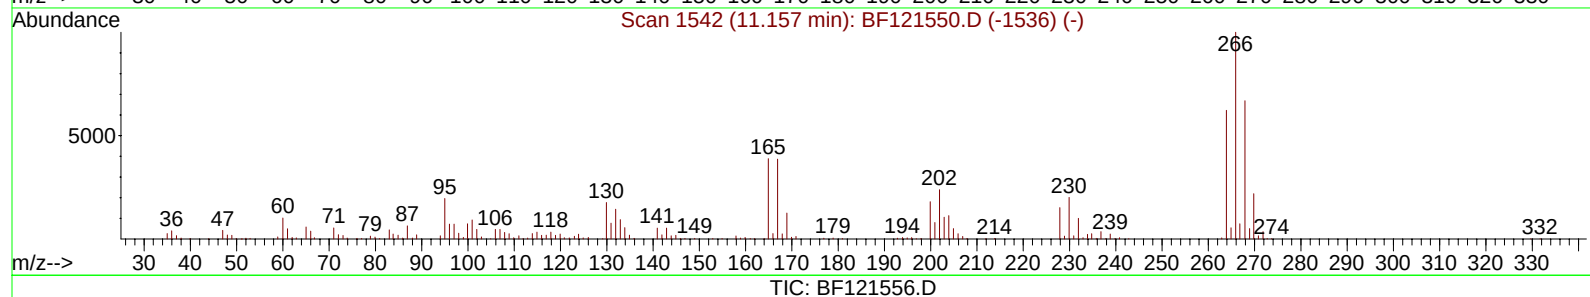
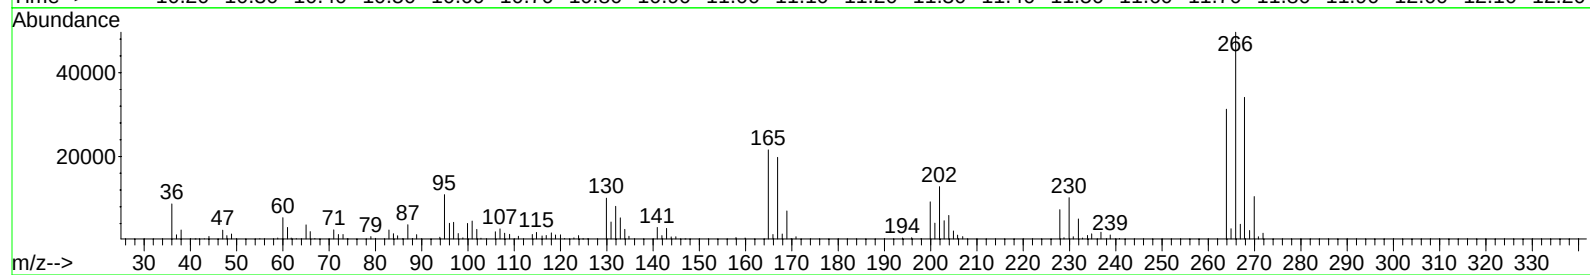


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091420\
 Data File : BF121556.D
 Acq On : 14 Sep 2020 12:03
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 18:10:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 10 16:47:54 2020
 Response via : Initial Calibration

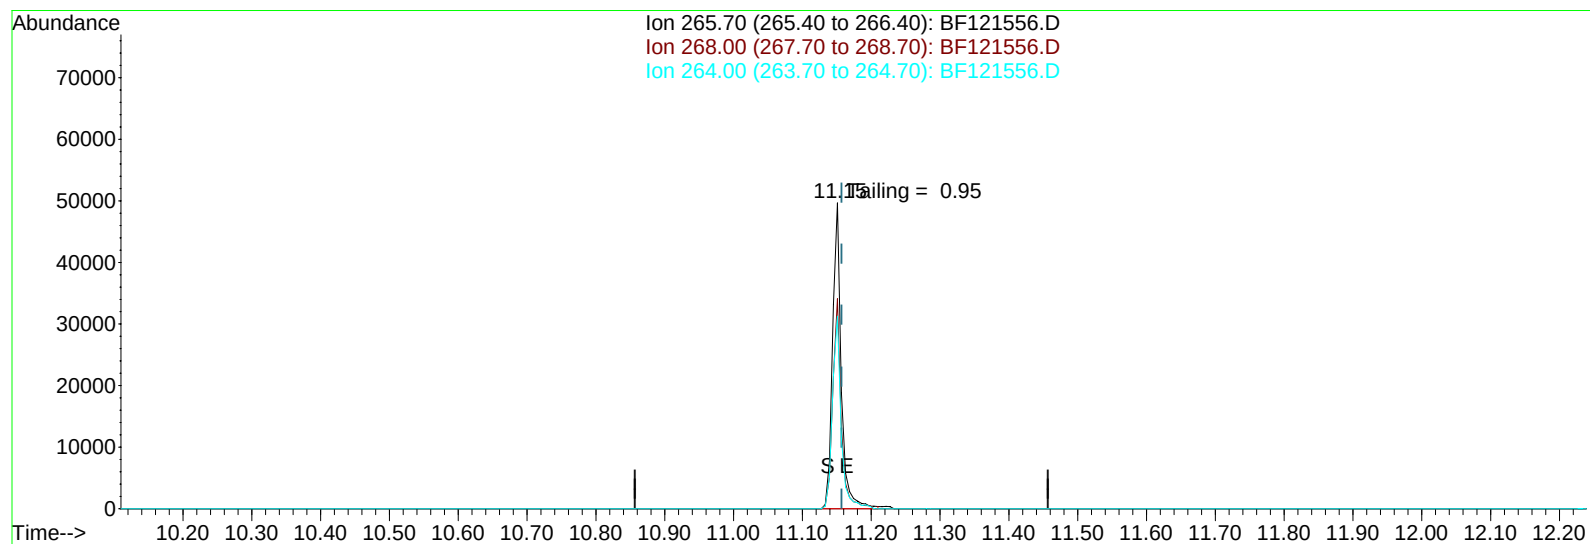

(70) Pentachlorophenol (C)




11.151min (-0.006) 17453.88ng

response 44215

Ion	Exp%	Act%
265.70	100	100
268.00	66.90	68.68
264.00	62.30	62.98
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091420\
 Data File : BF121556.D
 Acq On : 14 Sep 2020 12:03
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 18:10:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 10 16:47:54 2020
 Response via : Initial Calibration

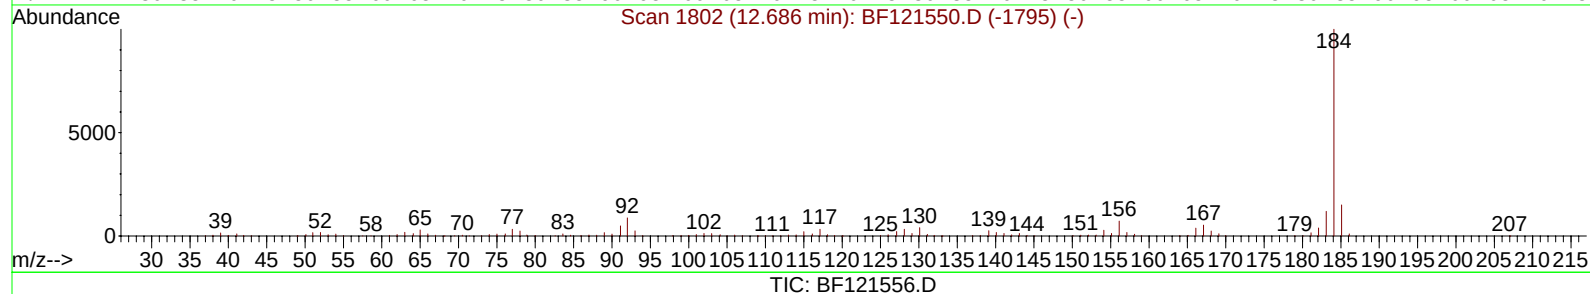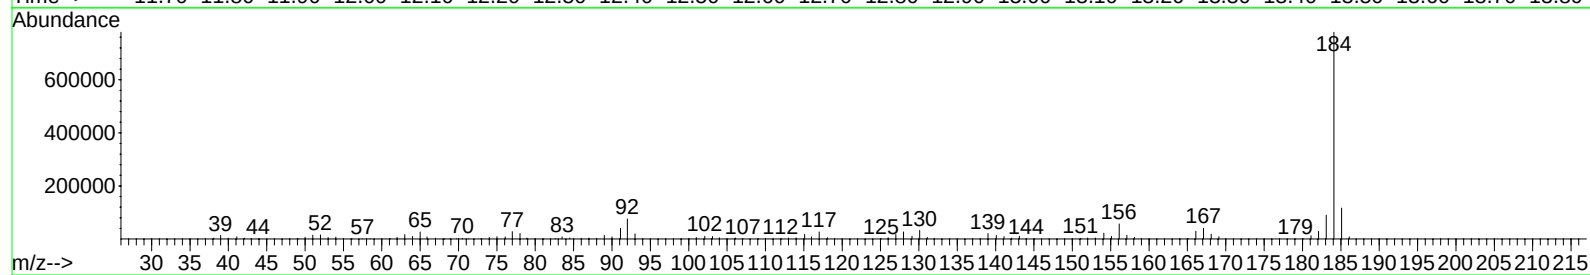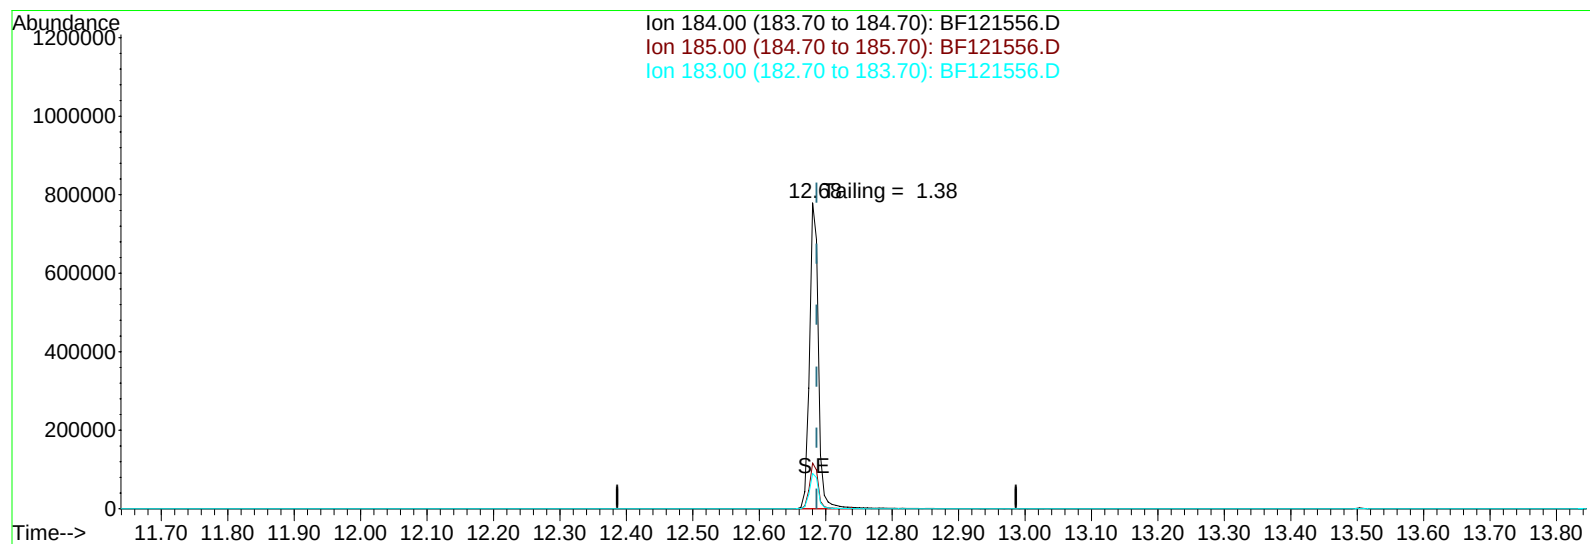

(77) Benzidine

12.680min (-0.006) 0.00ng

response 730745

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.99
183.00	11.90	11.57
0.00	0.00	0.00