

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091420\
 Data File : BF121563.D
 Acq On : 14 Sep 2020 16:32
 Operator : JU/CG
 Sample : L3993-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PAV-B38-091120-0-10

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.204	15	20	30	rVB	695537	1217613	18.62%	2.736%
2	2.775	112	117	126	rVB	838289	1237217	18.92%	2.780%
3	3.675	265	270	275	rBV	85906	121043	1.85%	0.272%
4	4.363	383	387	393	rVB	64810	75554	1.16%	0.170%
5	4.440	395	400	406	rVB	216796	235316	3.60%	0.529%
6	4.634	429	433	440	rVB	375153	364590	5.58%	0.819%
7	5.057	500	505	507	rBV	910490	1139270	17.43%	2.560%
8	5.075	507	508	512	rVB	544129	347900	5.32%	0.782%
9	5.469	571	575	578	rBV	4076531	4000001	61.18%	8.989%
10	5.722	615	618	620	rBV	75123	67187	1.03%	0.151%
11	6.481	743	747	764	rVB	3671488	3767173	57.62%	8.466%
12	6.669	776	779	790	rVB	223709	195048	2.98%	0.438%
13	6.834	803	807	810	rBV	1536829	1202074	18.39%	2.701%
14	7.398	897	903	906	rBV	3380256	3483461	53.28%	7.828%
15	8.116	1020	1025	1028	rBV	1909008	1586363	24.27%	3.565%
16	9.192	1202	1208	1211	rBV	5883941	5838770	89.31%	13.121%
17	9.580	1270	1274	1278	rBV	830922	756132	11.57%	1.699%
18	9.869	1317	1323	1327	rBV	2156611	1803527	27.59%	4.053%
19	10.663	1452	1458	1461	rBV	4051760	3862876	59.09%	8.681%
20	10.927	1495	1503	1514	rBV2	41236	146703	2.24%	0.330%
21	11.351	1571	1575	1579	rBV	2062151	1880176	28.76%	4.225%
22	11.886	1661	1666	1669	rBV	1000617	904573	13.84%	2.033%
23	12.586	1779	1785	1794	rBV6	47874	123118	1.88%	0.277%
24	12.668	1795	1799	1810	rVV	395795	417995	6.39%	0.939%
25	12.945	1840	1846	1849	rBV	6200355	6537568	100.00%	14.691%
26	13.845	1995	1999	2010	rBV	214503	432879	6.62%	0.973%
27	13.986	2019	2023	2027	rBV	1649714	1523920	23.31%	3.425%
28	15.445	2266	2271	2275	rBV	1043829	1231306	18.83%	2.767%


Sum of corrected areas: 44499353

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091420\
Data File : BF121563.D
Acq On : 14 Sep 2020 16:32
Operator : JU/CG
Sample : L3993-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PAV-B38-091120-0-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

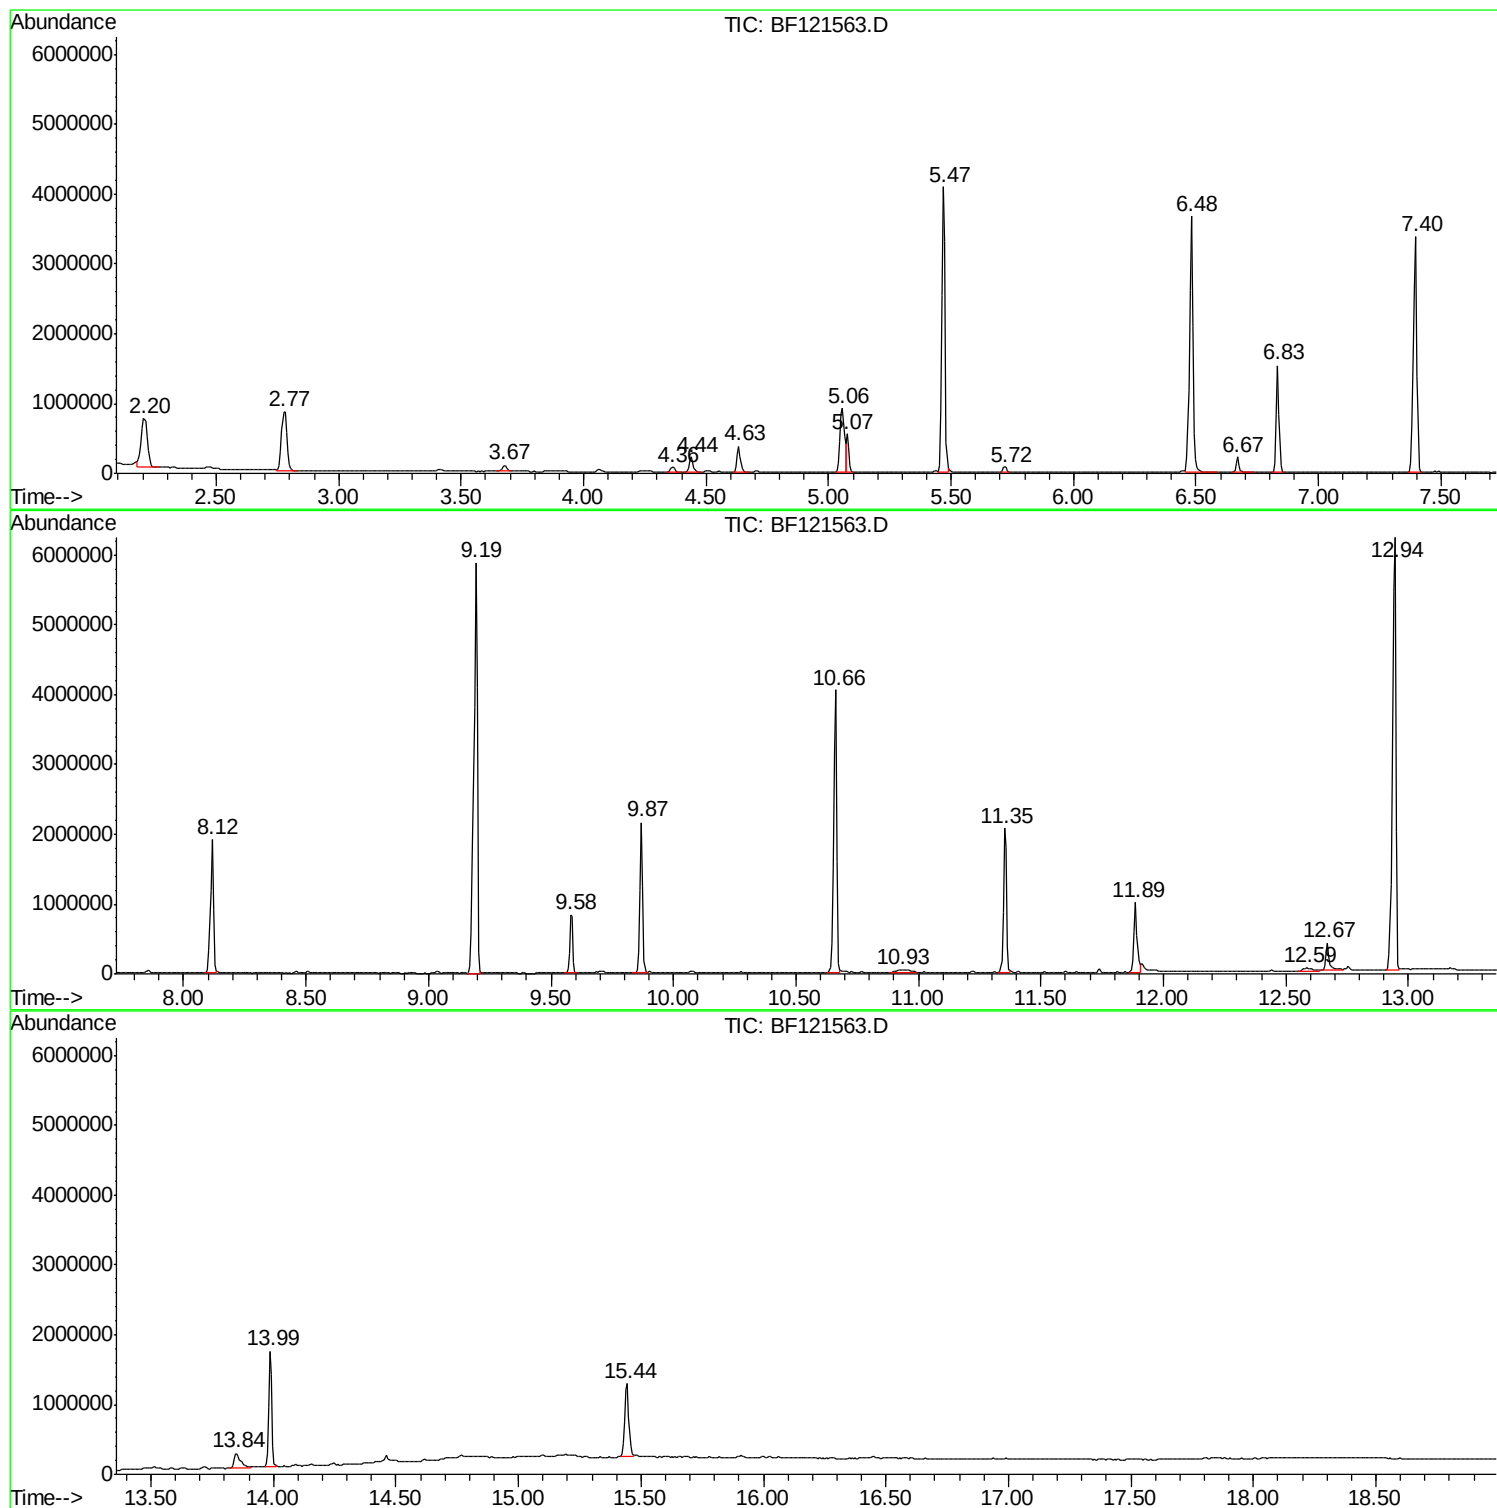

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091420\
Data File : BF121563.D
Acq On : 14 Sep 2020 16:32
Operator : JU/CG
Sample : L3993-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PAV-B38-091120-0-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091420\
Data File : BF121563.D
Acq On : 14 Sep 2020 16:32
Operator : JU/CG
Sample : L3993-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PAV-B38-091120-0-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc