


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091420\
 Data File : BF121556.D
 Acq On : 14 Sep 2020 12:03
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 10 16:47:54 2020

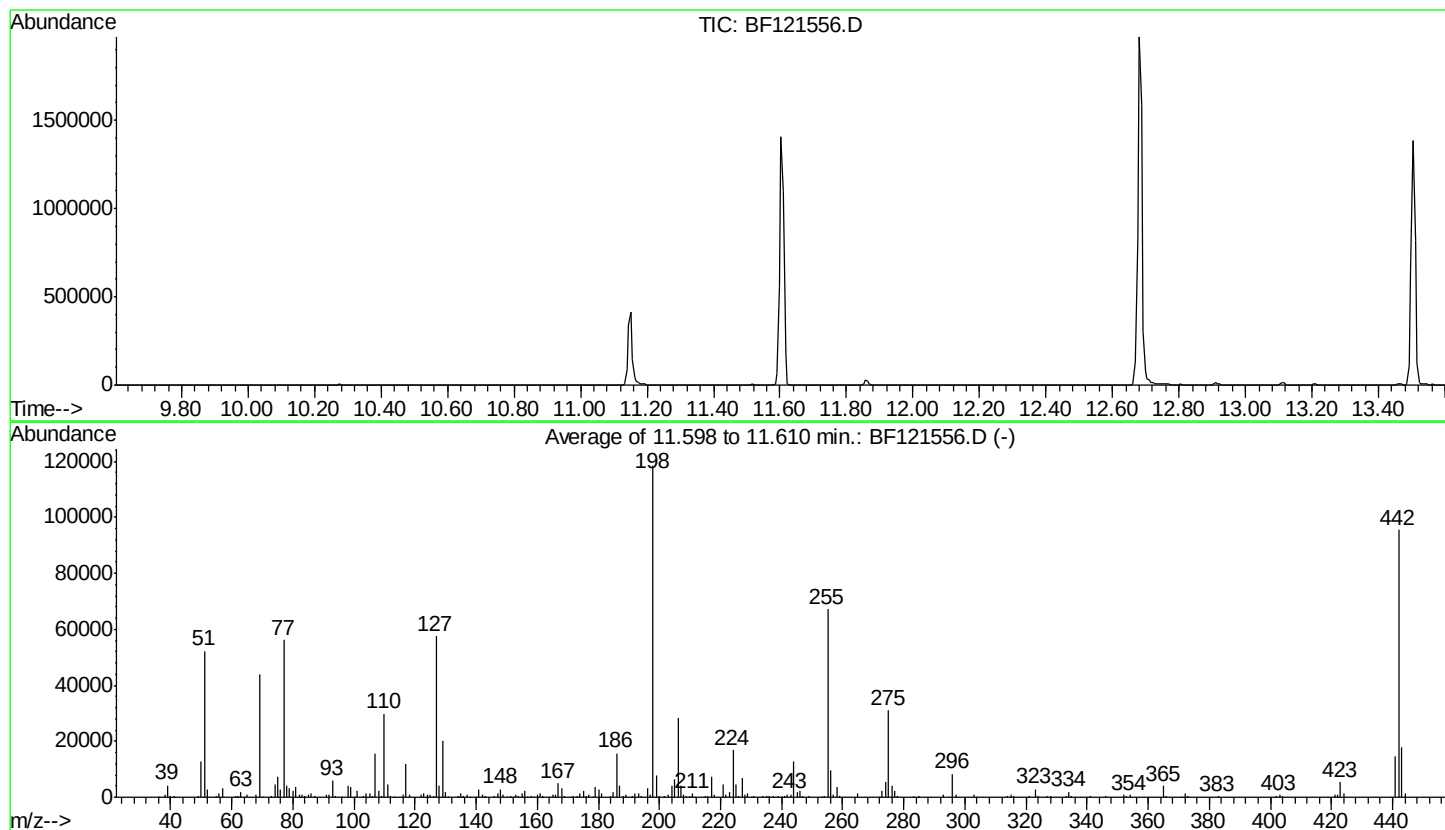

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.2	52354	PASS
68	69	0.00	2	1.7	736	PASS
69	198	0.00	100	37.0	43850	PASS
70	69	0.00	2	0.3	118	PASS
127	198	10	80	48.5	57456	PASS
197	198	0.00	2	0.7	880	PASS
198	198	100	100	100.0	118480	PASS
199	198	5	9	6.5	7645	PASS
275	198	10	60	26.2	31010	PASS
365	198	1	100	3.4	4065	PASS
441	198	0.01	100	12.5	14777	PASS
442	198	50	100	80.6	95544	PASS
443	442	15	24	18.7	17882	PASS