

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091421\
 Data File : BF125468.D
 Acq On : 14 Sep 2021 11:17
 Operator : JU/CG
 Sample : PB139040BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB139040BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.240	17	26	34	rVB	133500	173831	2.74%	0.463%
2	5.516	577	583	586	rBV	4542223	4766851	75.12%	12.705%
3	6.516	747	753	756	rBV	3732468	4771864	75.20%	12.718%
4	6.875	810	814	818	rBV	1349084	1085512	17.11%	2.893%
5	7.445	904	911	914	rBV	2702540	3203577	50.48%	8.538%
6	8.157	1027	1032	1036	rBV	1542846	1468201	23.14%	3.913%
7	9.239	1209	1216	1219	rBV	5558897	5527387	87.10%	14.732%
8	9.916	1325	1331	1335	rBV	1832231	1690711	26.64%	4.506%
9	10.716	1460	1467	1470	rBV	3603065	3750633	59.11%	9.996%
10	11.410	1580	1585	1588	rBV	2025413	1788724	28.19%	4.767%
11	12.998	1850	1855	1858	rBV	5953595	6345676	100.00%	16.913%
12	13.915	2007	2011	2017	rVB	68654	88622	1.40%	0.236%
13	14.057	2030	2035	2038	rBV	1531918	1514254	23.86%	4.036%
14	15.545	2282	2288	2299	rBV	1003437	1344355	21.19%	3.583%

Sum of corrected areas: 37520198

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091421\
Data File : BF125468.D
Acq On : 14 Sep 2021 11:17
Operator : JU/CG
Sample : PB139040BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139040BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.240	3.20 ng	173831	1,4-Dichlorobenzene-d4	6.875

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	37
4			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	25
5			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	23

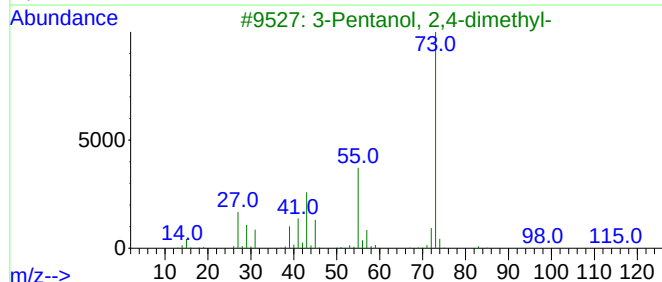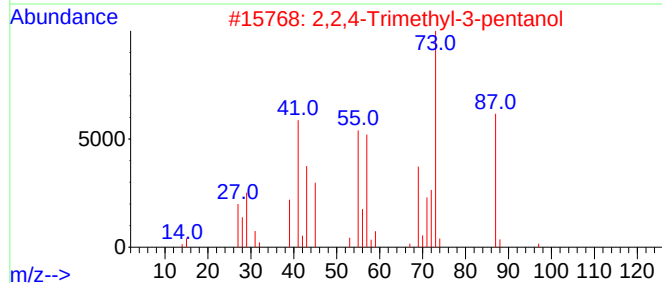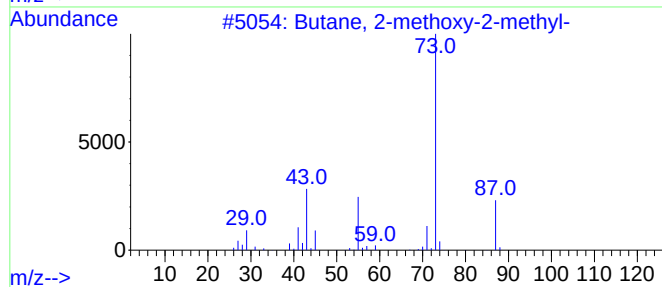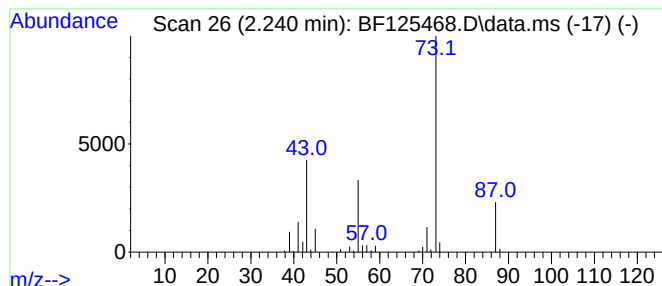

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091421\
Data File : BF125468.D
Acq On : 14 Sep 2021 11:17
Operator : JU/CG
Sample : PB139040BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139040BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.240	3.2	ng	173831	1	6.875	1085510	20.0