

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091421\
 Data File : BF125469.D
 Acq On : 14 Sep 2021 11:49
 Operator : JU/CG
 Sample : PB139016BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB139016BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125469.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.240	18	26	33	rVB	126790	172032	2.74%	0.460%
2	5.516	577	583	586	rBV	4573161	4764723	75.76%	12.744%
3	6.516	747	753	756	rBV	3804730	4752007	75.56%	12.710%
4	6.875	810	814	817	rBV	1406560	1101145	17.51%	2.945%
5	7.445	904	911	914	rBV	2757830	3230532	51.37%	8.640%
6	8.157	1027	1032	1036	rBV	1545633	1472236	23.41%	3.938%
7	9.239	1209	1216	1219	rBV	5443451	5547556	88.21%	14.837%
8	9.916	1326	1331	1335	rBV	1907698	1702921	27.08%	4.555%
9	10.710	1460	1466	1470	rBV	3570923	3747294	59.59%	10.022%
10	11.410	1580	1585	1588	rBV	1900177	1783441	28.36%	4.770%
11	12.998	1850	1855	1859	rBV	5571960	6288952	100.00%	16.820%
12	14.057	2030	2035	2038	rBV	1490888	1501882	23.88%	4.017%
13	15.545	2283	2288	2296	rBV2	982773	1324301	21.06%	3.542%




Sum of corrected areas: 37389022

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091421\
Data File : BF125469.D
Acq On : 14 Sep 2021 11:49
Operator : JU/CG
Sample : PB139016BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139016BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

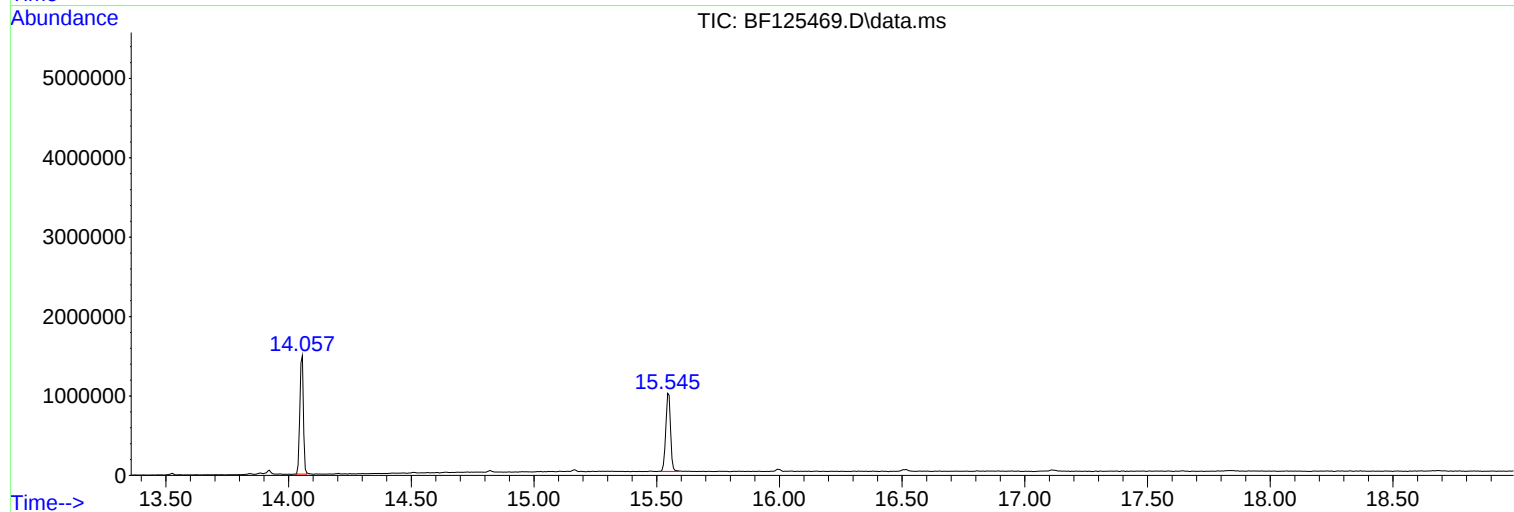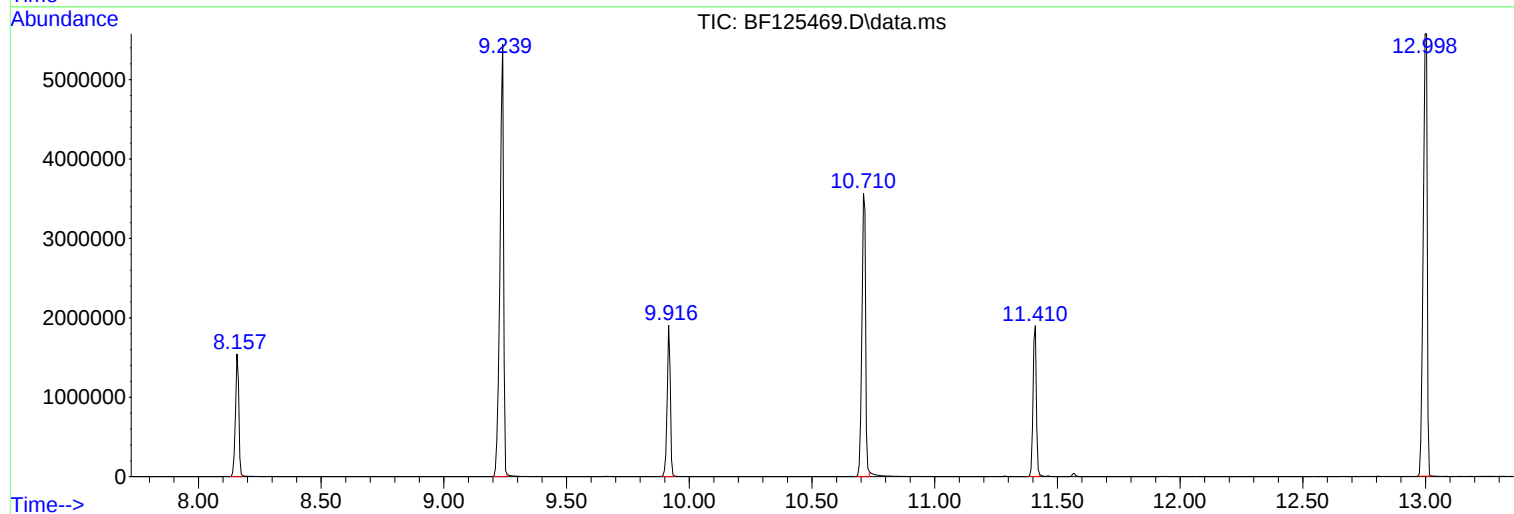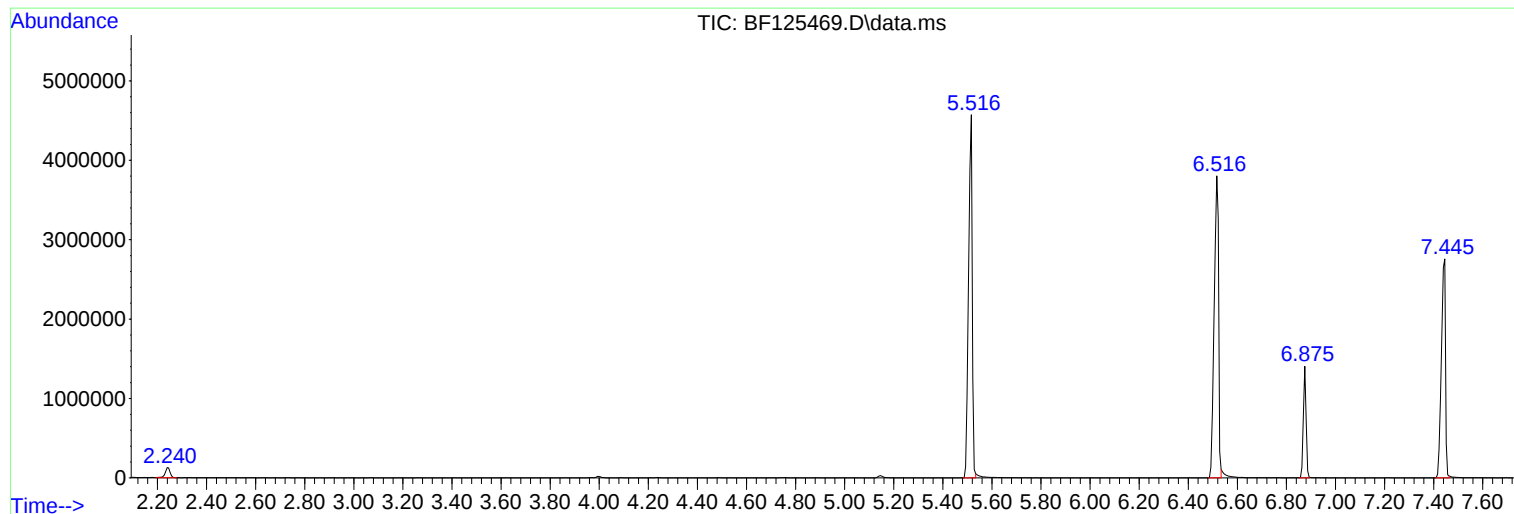

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091421\
Data File : BF125469.D
Acq On : 14 Sep 2021 11:49
Operator : JU/CG
Sample : PB139016BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139016BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.240	3.12 ng	172032	1,4-Dichlorobenzene-d4	6.875

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	50
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	32
5			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	25

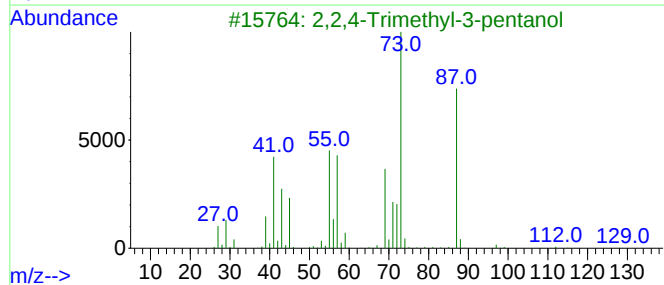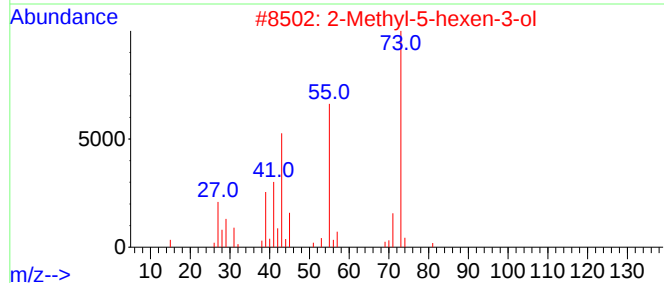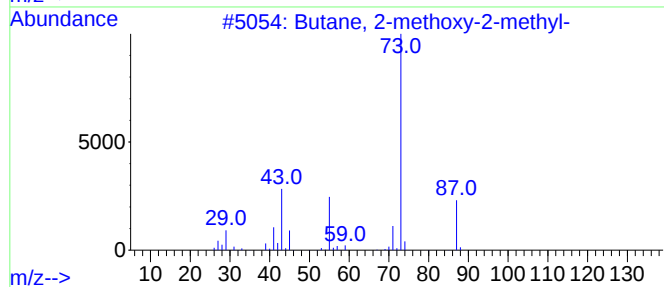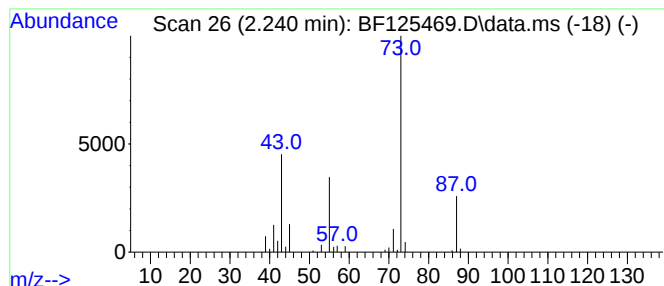

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091421\
Data File : BF125469.D
Acq On : 14 Sep 2021 11:49
Operator : JU/CG
Sample : PB139016BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139016BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.240	3.1	ng	172032	1	6.875	1101150	20.0