
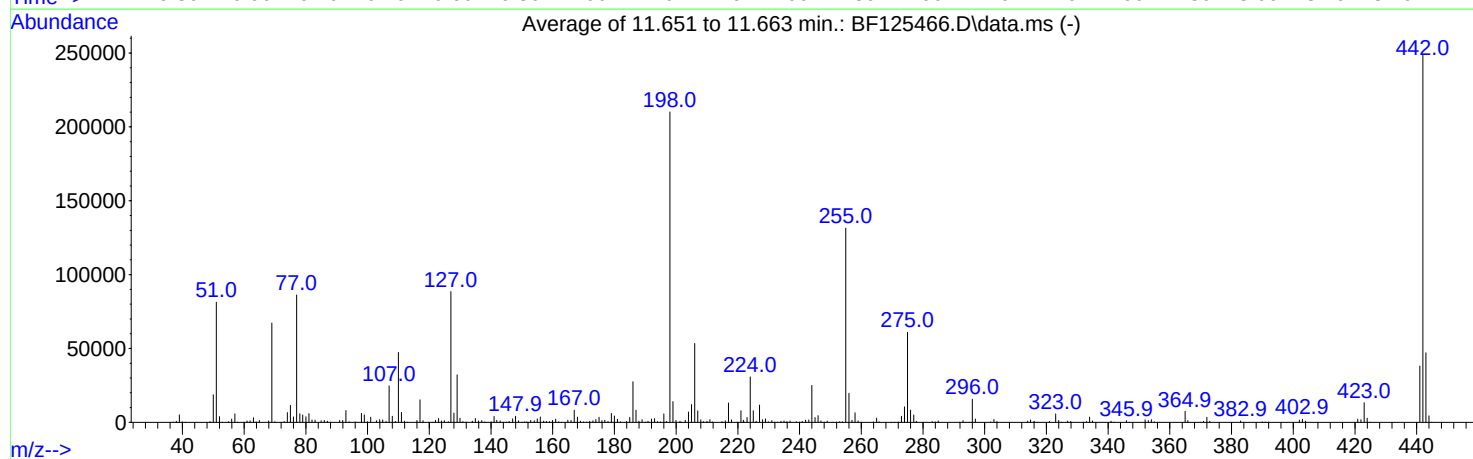


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091421\
 Data File : BF125466.D
 Acq On : 14 Sep 2021 10:14
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 14 17:17:24 2021

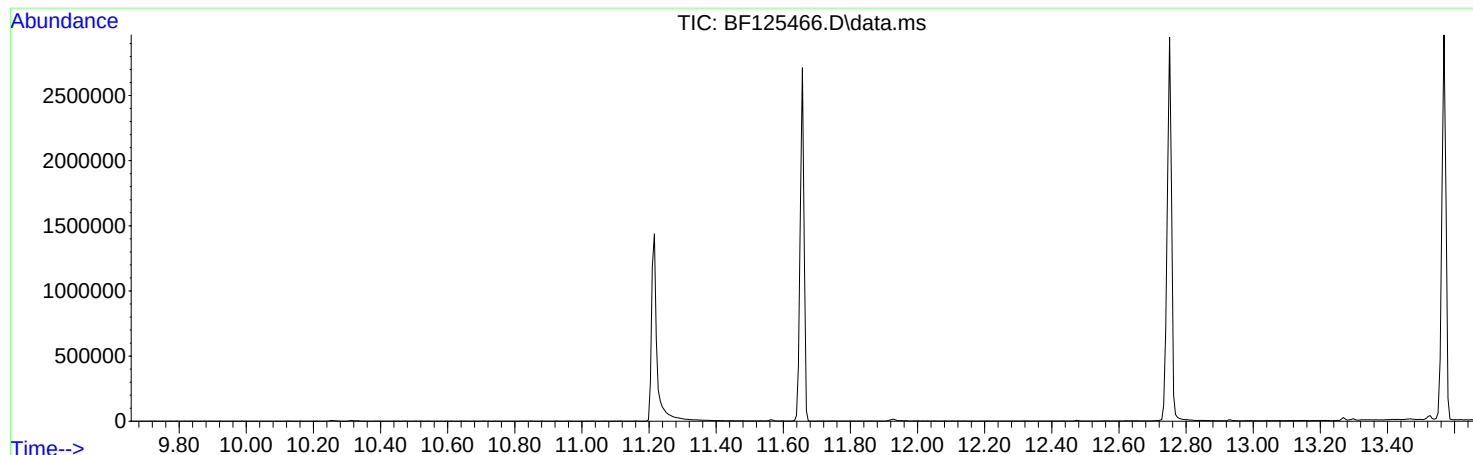




AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	81285	PASS
68	69	0.00	2	1.5	1015	PASS
69	198	0.00	100	32.0	67288	PASS
70	69	0.00	2	0.6	397	PASS
127	198	10	80	42.1	88437	PASS
197	198	0.00	2	0.3	636	PASS
198	198	100	100	100.0	210093	PASS
199	198	5	9	6.7	14072	PASS
275	198	10	60	29.0	61003	PASS
365	198	1	100	3.5	7450	PASS
441	198	0.01	100	18.2	38171	PASS
442	442	50	100	100.0	248981	PASS
443	442	15	24	18.9	47091	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091421\
Data File : BF125466.D
Acq On : 14 Sep 2021 10:14
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 14 11:41:29 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 13 12:03:46 2021
Response via : Initial Calibration

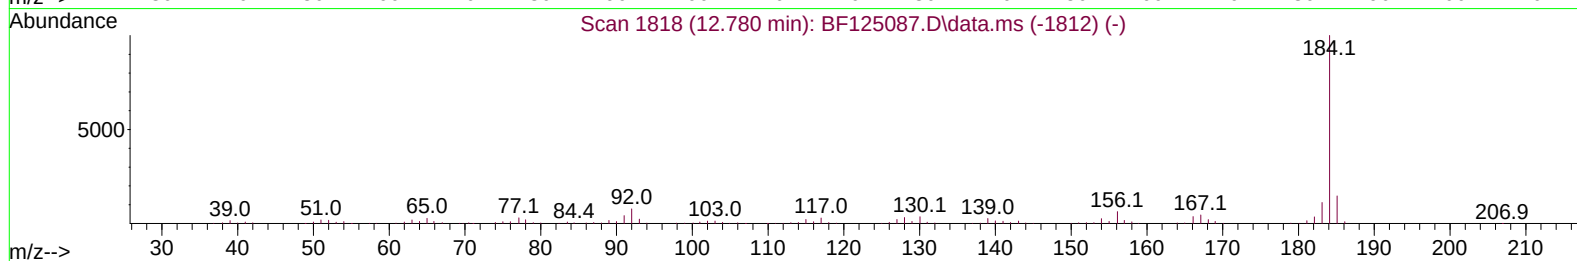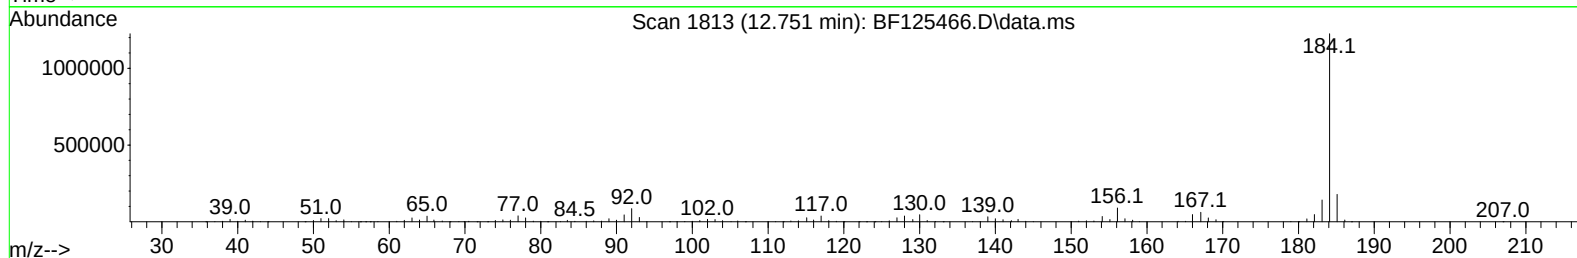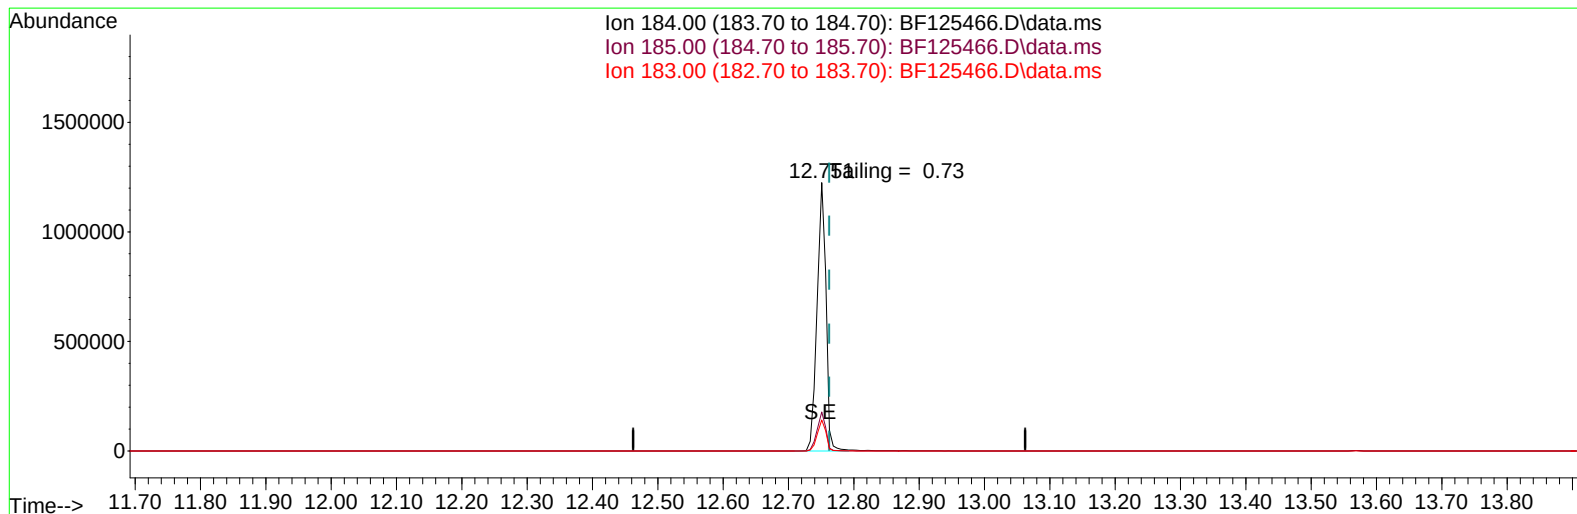

TIC: BF125466.D\data.ms

(77) Benzidine

12.751min (-0.012) 0.00 ng




response 1176949

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.59
183.00	10.10	11.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091421\
 Data File : BF125466.D
 Acq On : 14 Sep 2021 10:14
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 14 11:41:29 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 13 12:03:46 2021
 Response via : Initial Calibration

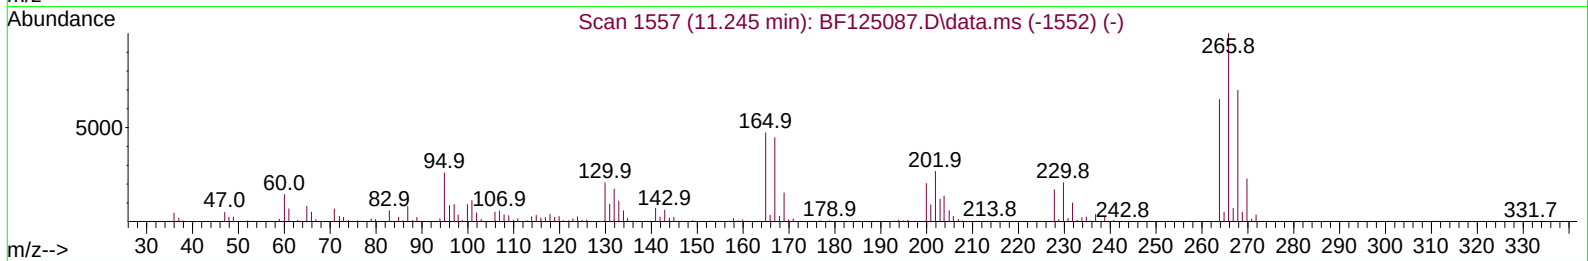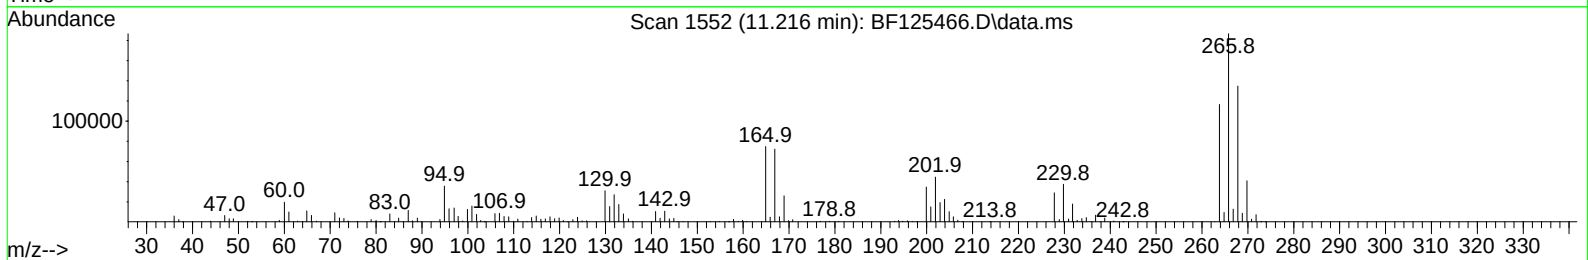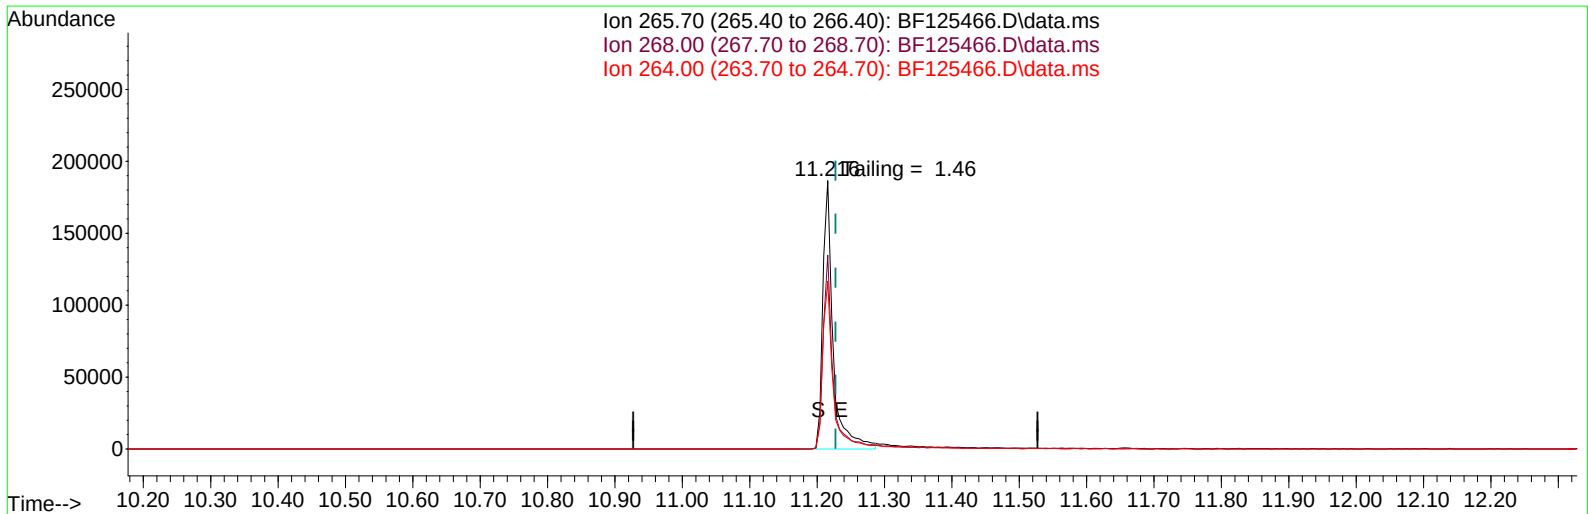

TIC: BF125466.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.012) 30918.01 ng

response 205172

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	72.22
264.00	69.90	62.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/14/2021	BNA_F	<u>BF125466.D</u>
Compound Name	Response	Retention Time
DDT	518911	13.56
DDD	5372	13.26
DDE	1603	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6975	525886	1.33

Instrument :
BNA_F
ClientSampleId :
DFTPP