


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091421\
 Data File : BF125475.D
 Acq On : 14 Sep 2021 15:38
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 14 17:17:24 2021

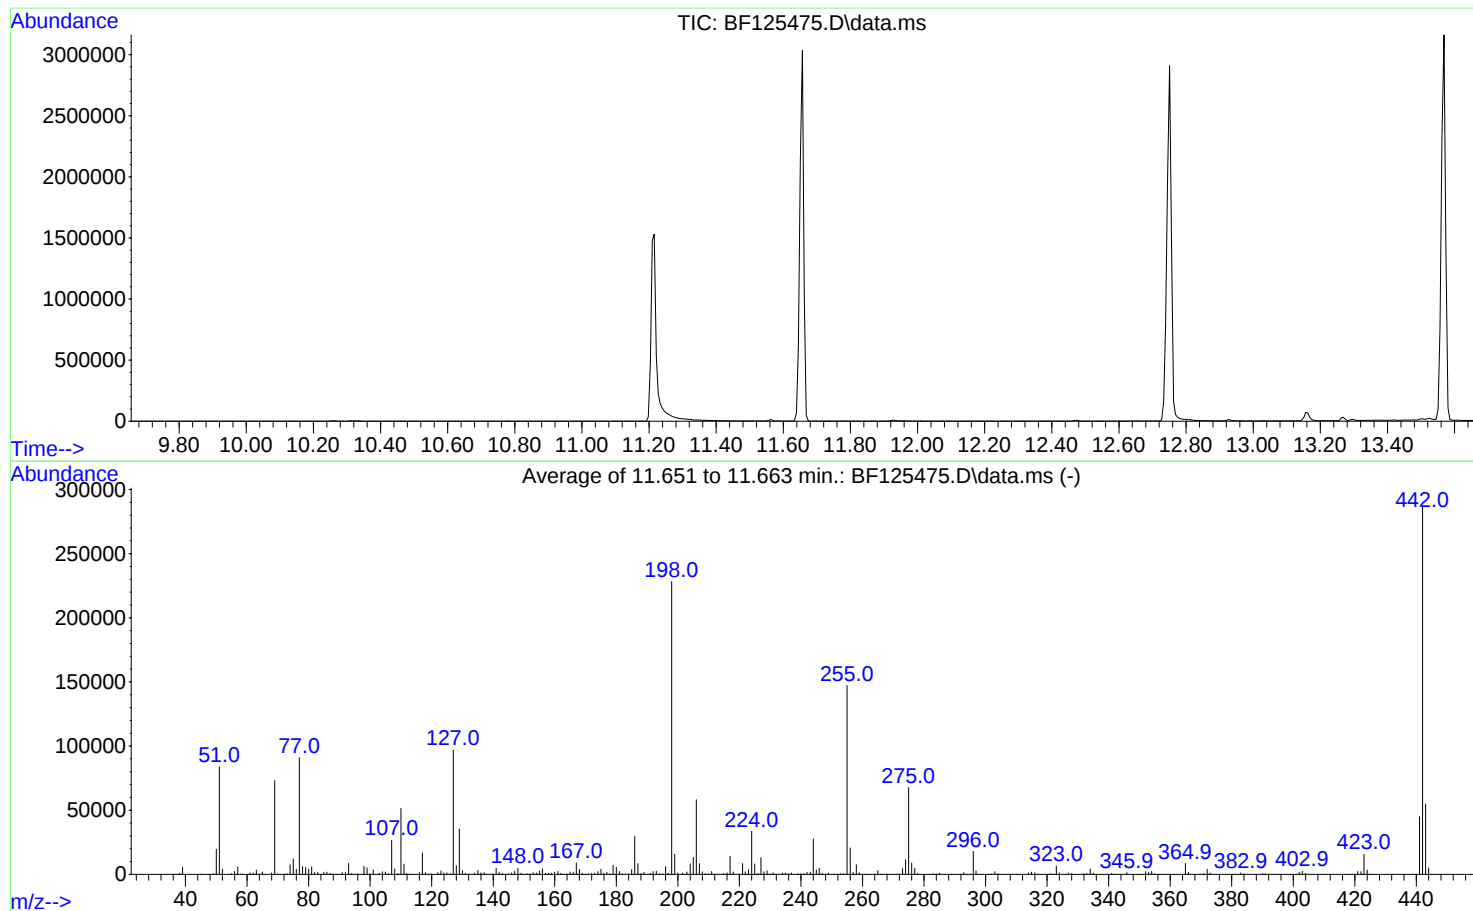




AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	83864	PASS
68	69	0.00	2	1.4	1033	PASS
69	198	0.00	100	32.0	73045	PASS
70	69	0.00	2	0.4	319	PASS
127	198	10	80	42.4	96781	PASS
197	198	0.00	2	0.3	688	PASS
198	198	100	100	100.0	228285	PASS
199	198	5	9	6.9	15715	PASS
275	198	10	60	29.6	67584	PASS
365	198	1	100	3.8	8561	PASS
441	198	0.01	100	19.7	44957	PASS
442	442	50	100	100.0	286763	PASS
443	442	15	24	19.2	54923	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091421\
 Data File : BF125475.D
 Acq On : 14 Sep 2021 15:38
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 14 16:09:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 14 11:45:52 2021
 Response via : Initial Calibration

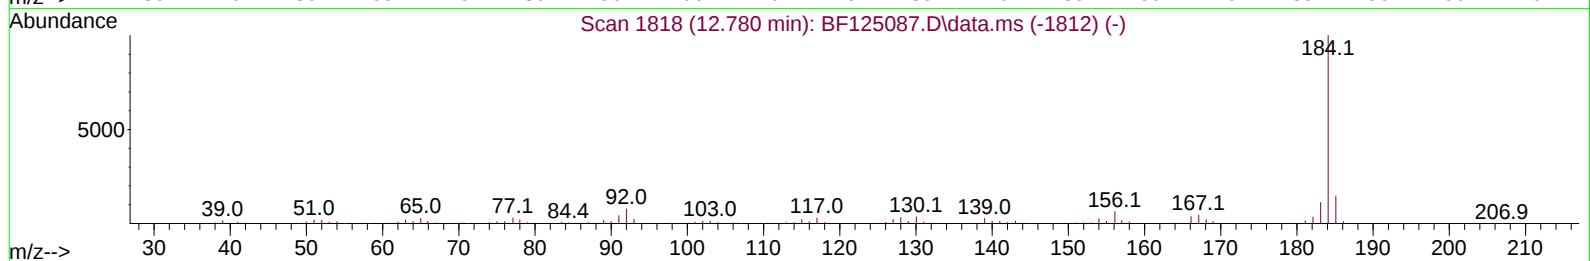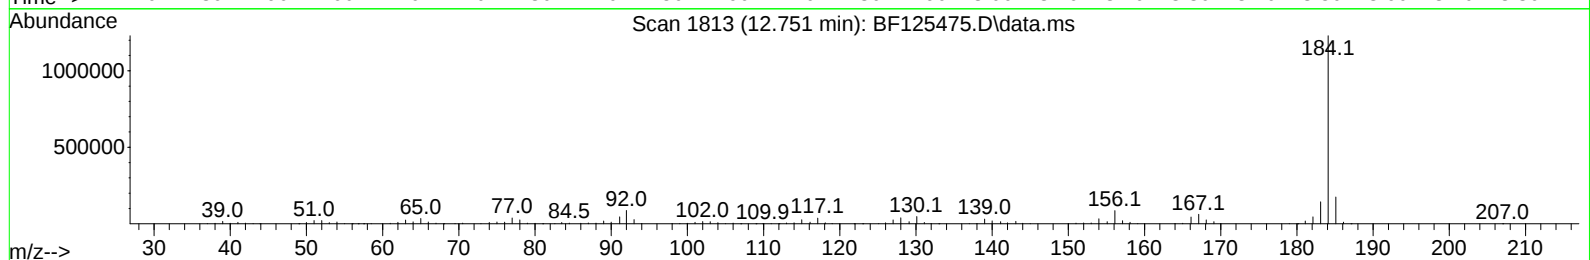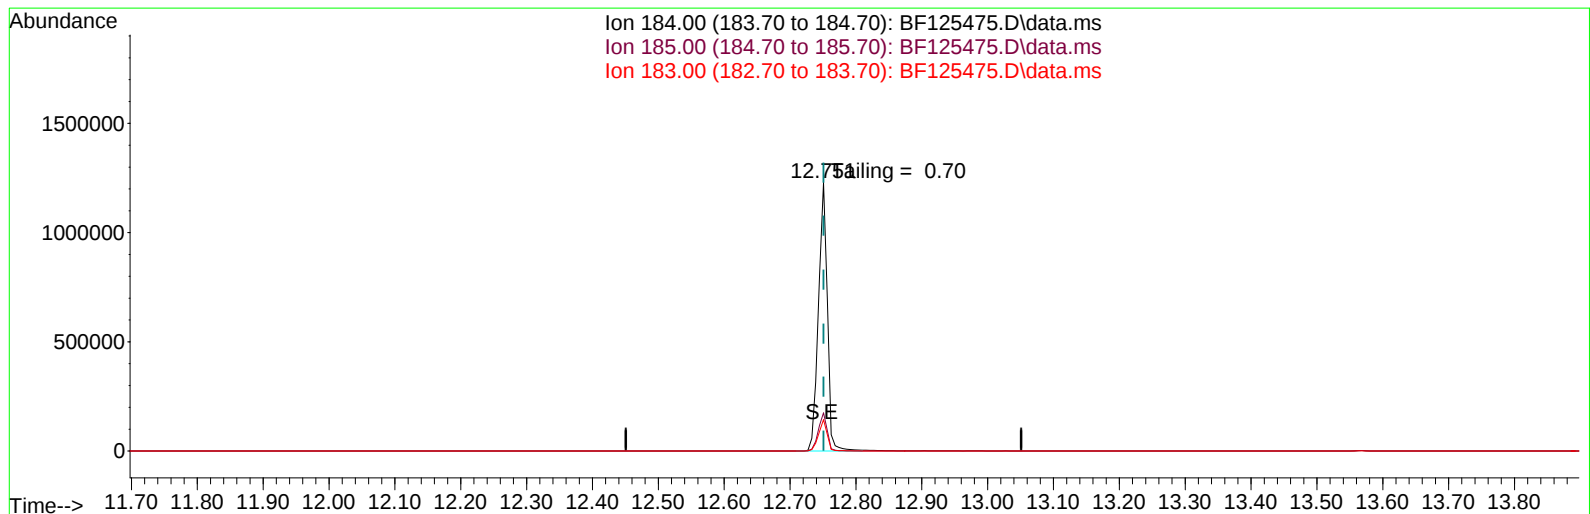

TIC: BF125475.D\data.ms

(77) Benzidine

12.751min (-0.000) 0.00 ng




response 1158623

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.26
183.00	10.10	11.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091421\
 Data File : BF125475.D
 Acq On : 14 Sep 2021 15:38
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 14 16:09:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 14 11:45:52 2021
 Response via : Initial Calibration

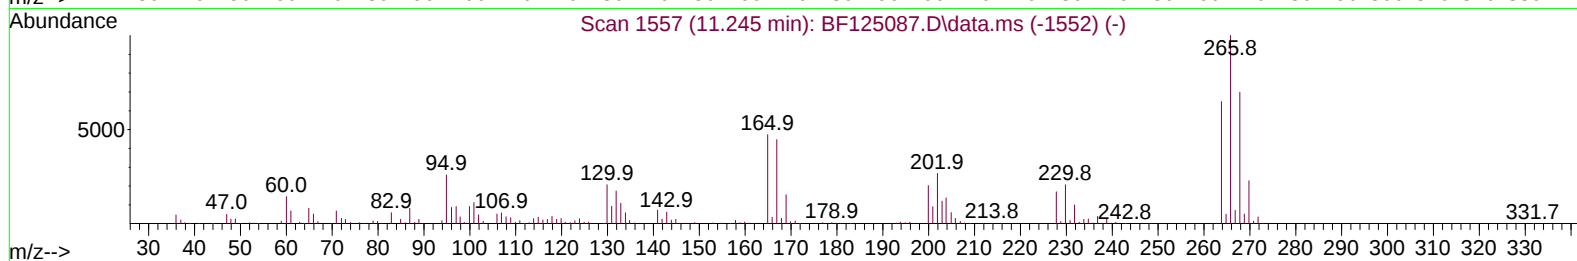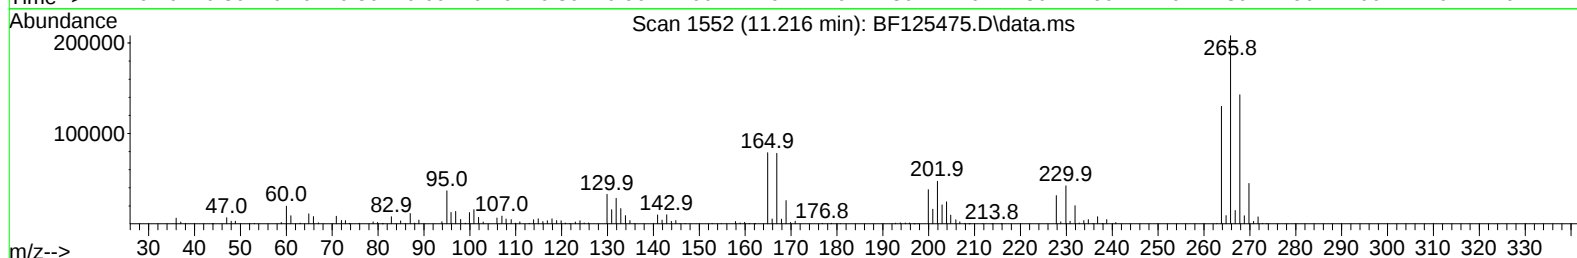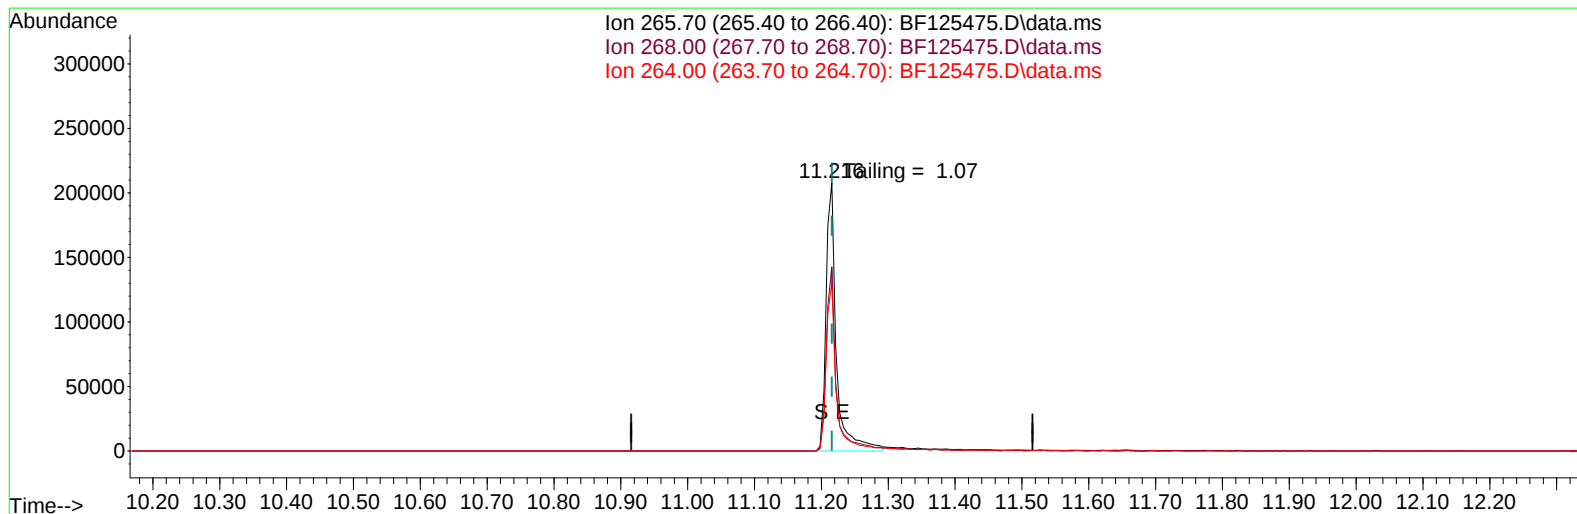

TIC: BF125475.D\data.ms

(70) Pentachlorophenol (C)

11.216min (-0.000) 33593.66 ng

response 230197

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	68.62
264.00	69.90	62.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/14/2021	BNA_F	<u>BF125475.D</u>
Compound Name	Response	Retention Time
DDT	569352	13.56
DDD	6394	13.26
DDE	2341	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8735	578087	1.51

Instrument :
BNA_F
ClientSampleId :
DFTPP