

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091515\
 Data File : BF081626.D
 Acq On : 15 Sep 2015 12:59
 Operator : UM/IZ
 Sample : G3597-03DL 50X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 GP-3(0-5)DL

Quant Time: Sep 15 13:59:03 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 14 13:51:56 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.21	152	50402	20.00	ng	-0.02
21) Naphthalene-d8	11.11	136	206711	20.00	ng	-0.02
38) Acenaphthene-d10	15.24	164	96987	20.00	ng	-0.03
63) Phenanthrene-d10	18.74	188	185719	20.00	ng	-0.02
75) Chrysene-d12	23.38	240	126077	20.00	ng	-0.01
86) Perylene-d12	24.81	264	91370	20.00	ng	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.41	112	3146	0.97	ng	0.03
7) Phenol-d6	7.66	99	5469	1.27	ng	0.00
23) Nitrobenzene-d5	9.51	82	3791	0.88	ng	-0.03
41) 2,4,6-Tribromophenol	17.14	330	976	1.13	ng	-0.03
44) 2-Fluorobiphenyl	13.75	172	8946	1.18	ng	-0.03
78) Terphenyl-d14	22.09	244	7546	1.39	ng	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	1.54	88	49438	33.89	ng	# 14
31) Naphthalene	11.15	128	50922	4.62	ng	99
37) 2-Methylnaphthalene	12.81	142	19857	2.77	ng	# 92
51) Acenaphthene	15.32	154	23560	3.62	ng	# 80
54) Dibenzofuran	15.74	168	32213	3.39	ng	# 83
55) 4-Nitrophenol	15.74	139	13864	11.33	ng	# 25
57) Fluorene	16.55	166	40192	5.58	ng	94
70) Phenanthrene	18.81	178	455705	44.14	ng	97
71) Anthracene	18.93	178	109337	10.31	ng	98
72) Carbazole	19.40	167	27750	2.79	ng	# 94
74) Fluoranthene	21.43	202	396543	35.48	ng	88
77) Pyrene	21.77	202	350876	37.57	ng	96
80) Benzo(a)anthracene	23.37	228	134860	16.80	ng	96
82) Chrysene	23.41	228	119063	16.54	ng	94
85) Indeno(1,2,3-cd)pyrene	25.86	276	45711	8.66	ng	# 82
87) Benzo(b)fluoranthene	24.47	252	127415	19.53	ng	# 88
88) Benzo(k)fluoranthene	24.47	252	127097	23.48	ng	# 88
89) Benzo(a)pyrene	24.77	252	75458	13.65	ng	# 82
90) Dibenzo(a,h)anthracene	25.86	278	10162	2.38	ng	# 75
91) Benzo(g,h,i)perylene	26.16	276	40154	9.85	ng	# 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091515\
Data File : BF081626.D
Acq On : 15 Sep 2015 12:59
Operator : UM/IZ
Sample : G3597-03DL 50X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleID :
GP-3(0-5)DL

Quant Time: Sep 15 13:59:03 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 14 13:51:56 2015
Response via : Initial Calibration

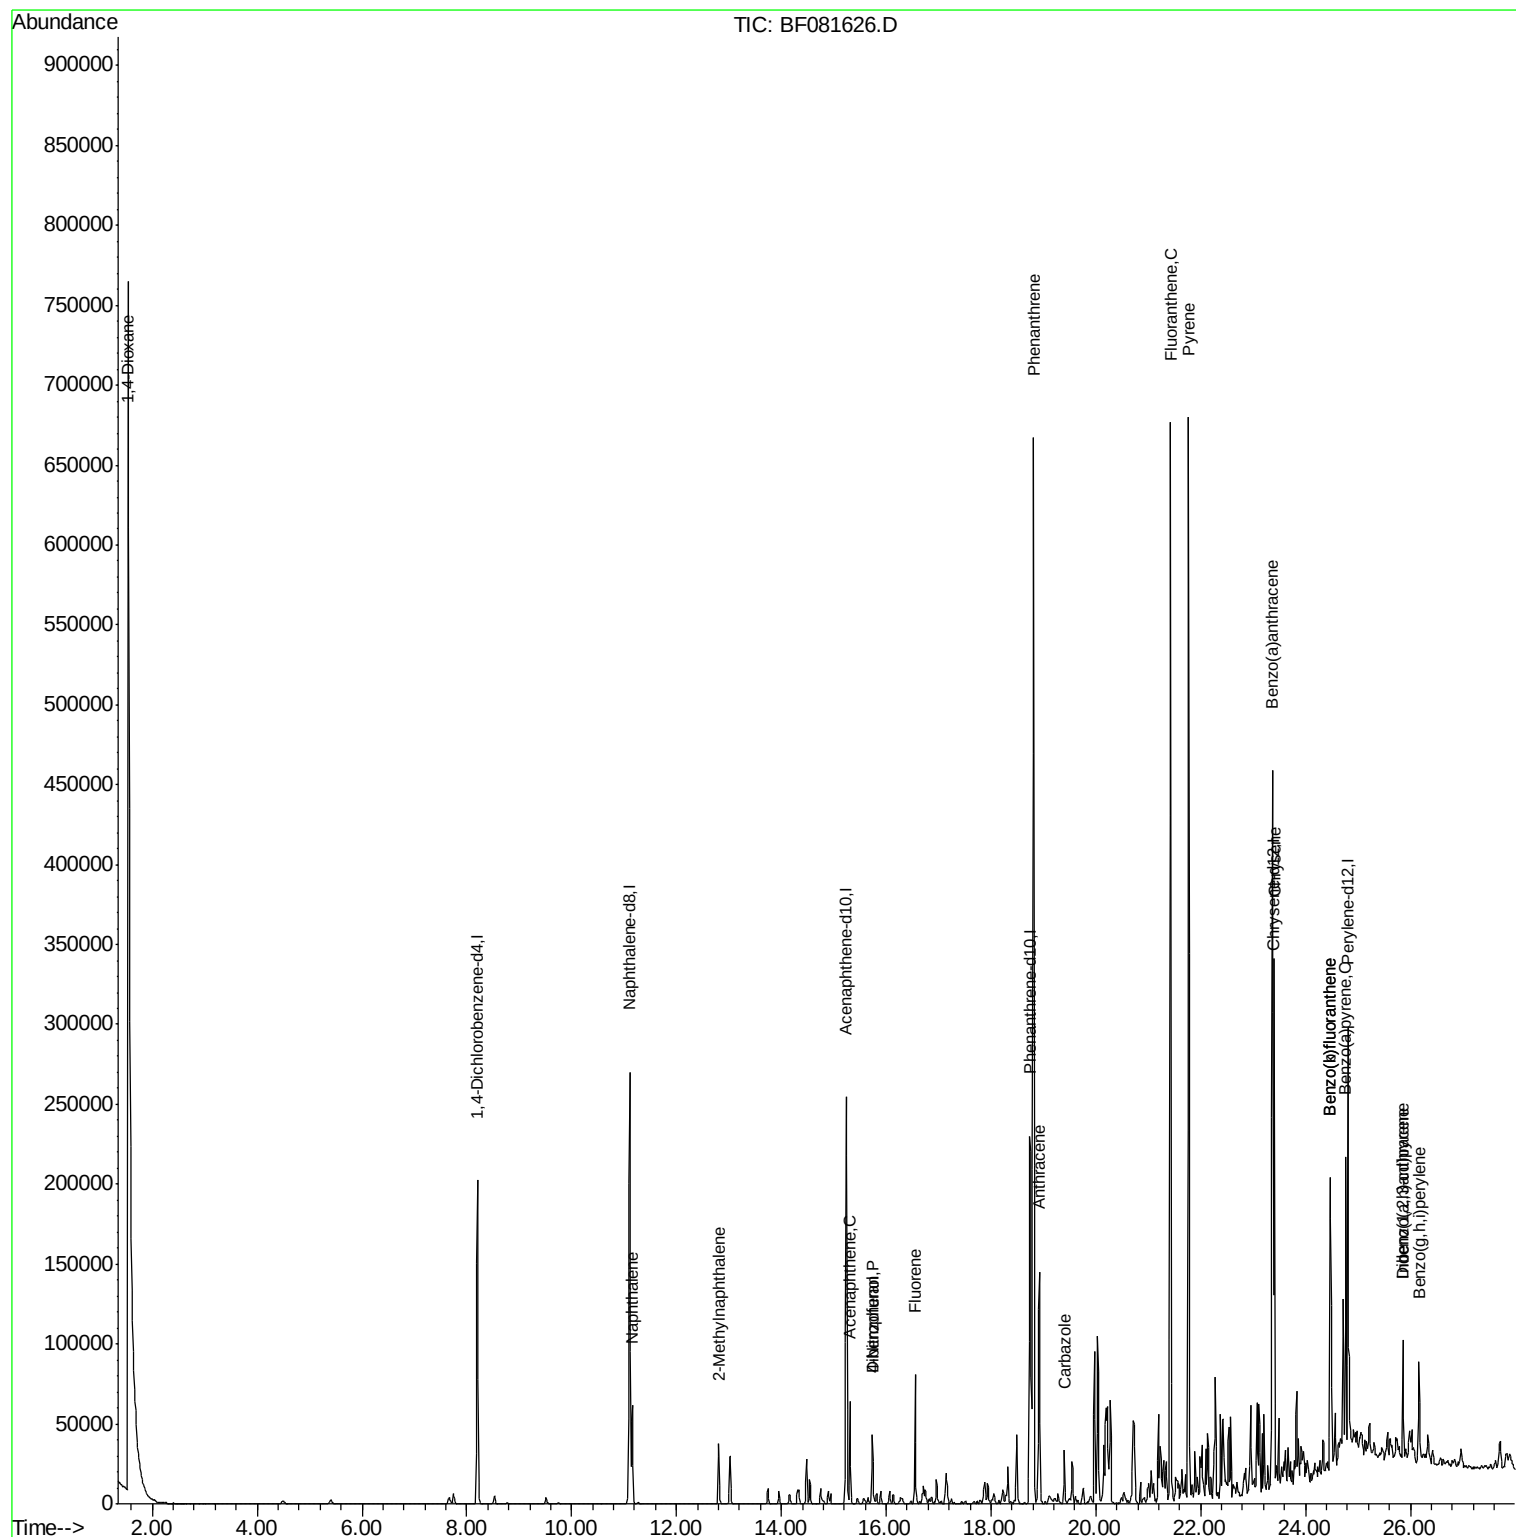



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.21 min Scan# 601

Delta R.T. -0.02 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59

Instrument :

BNA_F

ClientSampleId :

GP-3(0-5)DL


Tgt Ion:152 Resp: 50402

Ion Ratio Lower Upper

152 100

150 157.5 124.7 187.1




115 62.7 39.0 58.4#

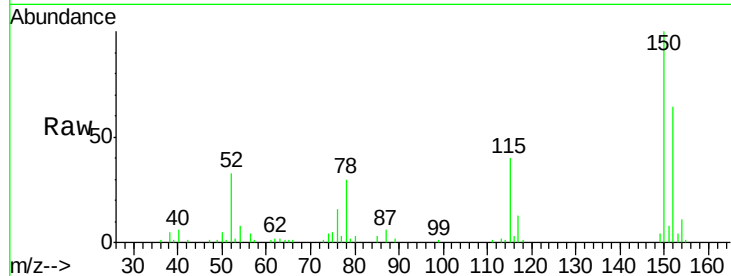

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

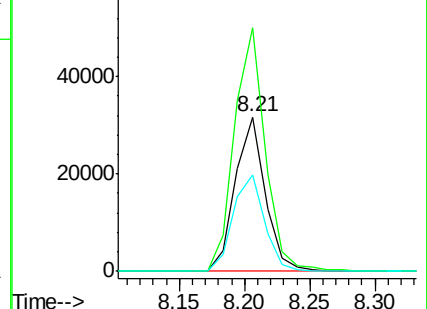

#2

1,4-Dioxane

Concen: 33.89 ng

RT: 1.54 min Scan# 18

Delta R.T. -0.02 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59


Tgt Ion: 88 Resp: 49438

Ion Ratio Lower Upper

88 100

58 0.0 77.7 116.5#



43 5.5 26.6 40.0#




Abundance Ion 88.00 (87.70 to 88.70): BF0

Ion 58.00 (57.70 to 58.70): BF0

Ion 43.00 (42.70 to 43.70): BF0

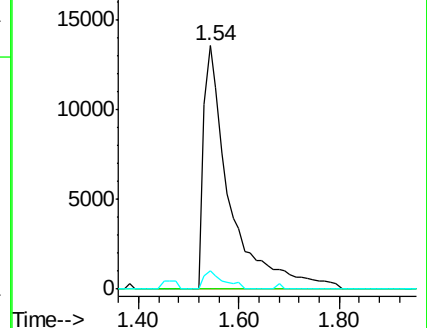



#5

2-Fluorophenol

Concen: 0.97 ng

RT: 5.41 min Scan# 356

Delta R.T. 0.03 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59


Instrument :

BNA_F

ClientSampleId :

GP-3(0-5)DL




Tgt Ion:	112	Resp:	3146
Ion	Ratio	Lower	Upper
112	100		
64	55.3	39.7	59.5
63	38.4	17.4	26.0#



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

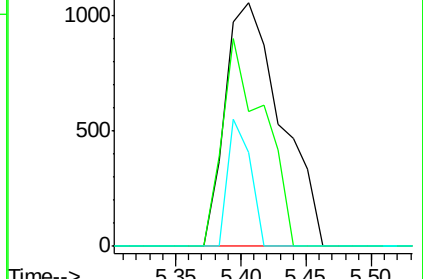

#7

Phenol-d6

Concen: 1.27 ng


RT: 7.66 min Scan# 553

Delta R.T. -0.00 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59



Tgt Ion:	99	Resp:	5469
Ion	Ratio	Lower	Upper
99	100		
42	28.1	13.7	20.5#
71	39.0	14.2	21.2#




Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

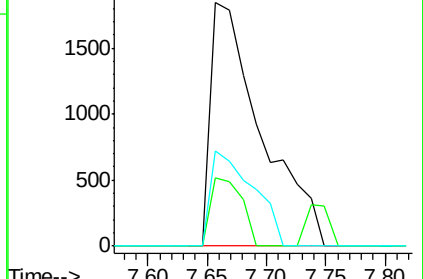







#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.11 min Scan# 855
Delta R.T. -0.02 min
Lab File: BF081626.D
Acq: 15 Sep 2015 12:59

Instrument :
BNA_F
ClientSampleId :
GP-3(0-5)DL

Tgt Ion:	136	Resp:	206711
Ion	Ratio	Lower	Upper
136	100		
137	10.6	9.0	13.6
54	10.9	8.2	12.2
68	5.1	5.8	8.6#

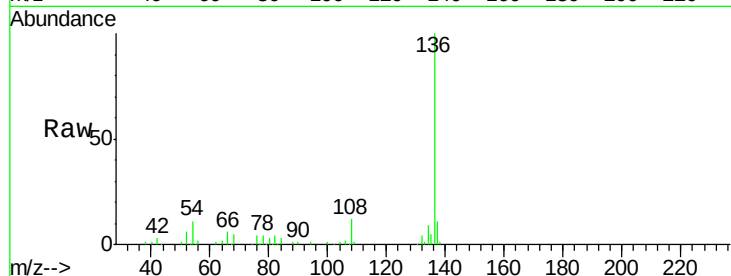


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0


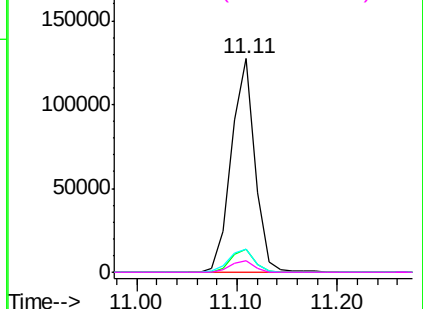



#23
Nitrobenzene-d5
Concen: 0.88 ng
RT: 9.51 min Scan# 715
Delta R.T. -0.03 min
Lab File: BF081626.D
Acq: 15 Sep 2015 12:59

Tgt Ion:	82	Resp:	3791
Ion	Ratio	Lower	Upper
82	100		
128	41.9	51.0	76.6#
54	71.0	47.5	71.3

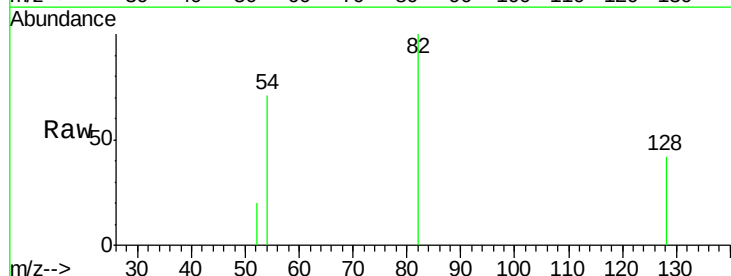

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

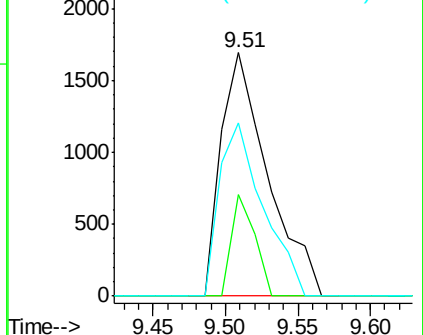

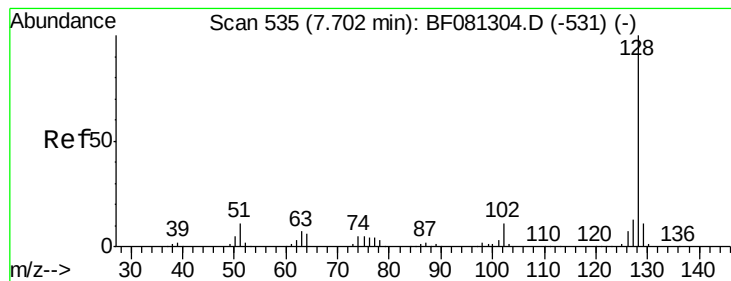

#31

Naphthalene

Concen: 4.62 ng

RT: 11.15 min Scan# 859

Delta R.T. -0.03 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59

Instrument :

BNA_F

ClientSampleId :

GP-3(0-5)DL


Tgt Ion:128 Resp: 50922

Ion Ratio Lower Upper

128 100

129 10.7 8.4 12.6




127 12.8 9.9 14.9



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

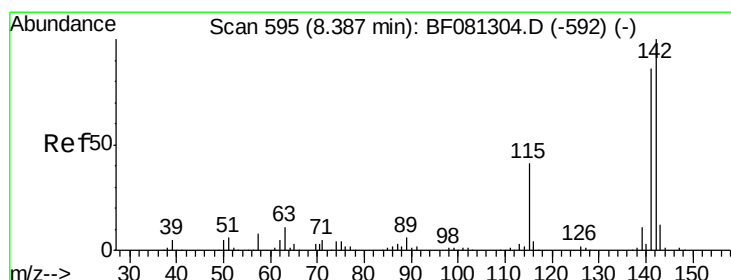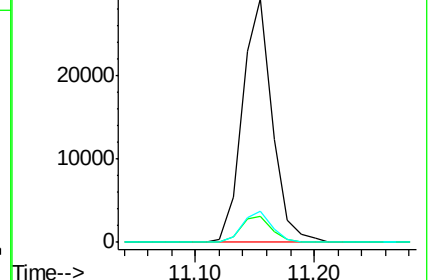

#37

2-Methylnaphthalene

Concen: 2.77 ng

RT: 12.81 min Scan# 1004

Delta R.T. -0.02 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59


Tgt Ion:142 Resp: 19857

Ion Ratio Lower Upper

142 100

141 86.1 67.5 101.3



115 36.7 18.2 27.2#




Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

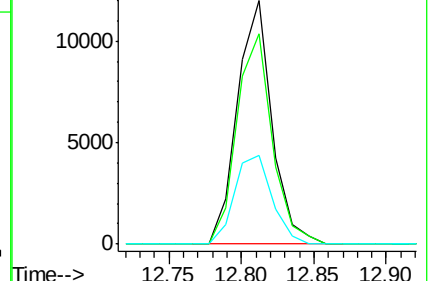



#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 15.24 min Scan# 1216

Delta R.T. -0.03 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59

Instrument :

BNA_F

ClientSampleId :

GP-3(0-5)DL


Tgt Ion:164 Resp: 96987

Ion Ratio Lower Upper

164 100

162 101.0 75.2 112.8




160 46.2 31.5 47.3

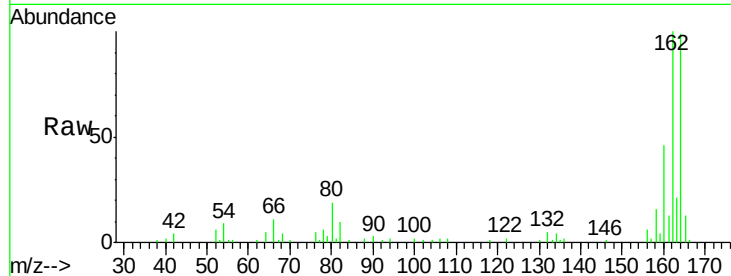

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

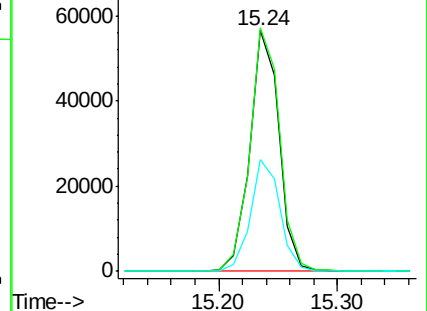

#41

2,4,6-Tribromophenol

Concen: 1.13 ng

RT: 17.14 min Scan# 1383

Delta R.T. -0.03 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59


Tgt Ion:330 Resp: 976

Ion Ratio Lower Upper

330 100

332 75.9 76.6 114.8#



141 29.6 29.7 44.5#

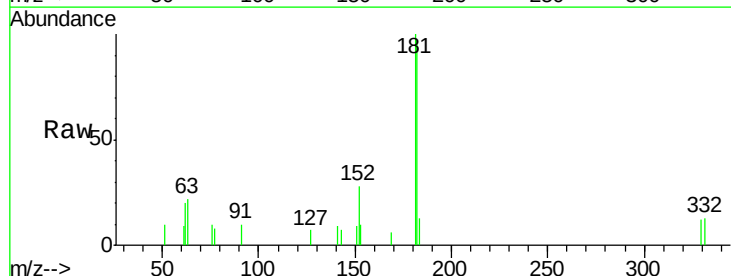


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




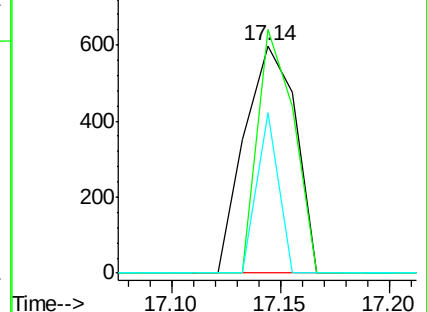


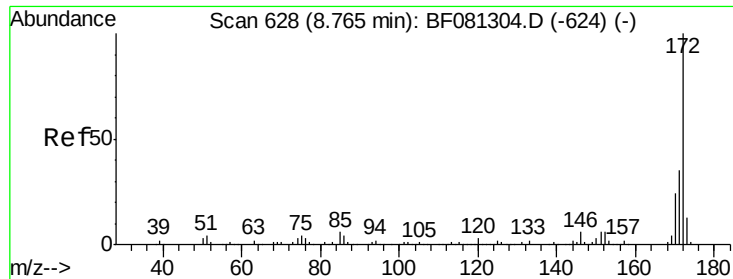

#44
2-Fluorobiphenyl
Concen: 1.18 ng
RT: 13.75 min Scan# 1086
Delta R.T. -0.03 min
Lab File: BF081626.D
Acq: 15 Sep 2015 12:59




Instrument :
BNA_F
ClientSampleId :
GP-3(0-5)DL


Tgt Ion:172 Resp: 8946
Ion Ratio Lower Upper
172 100
171 33.8 26.1 39.1
170 24.0 17.4 26.2

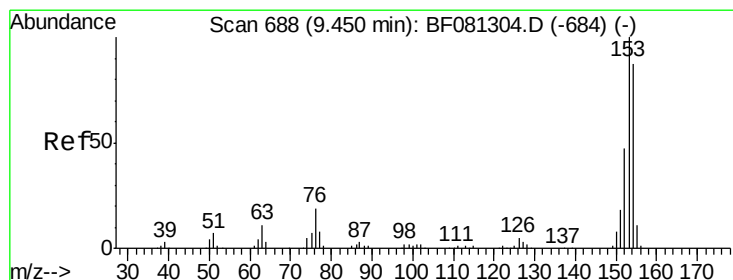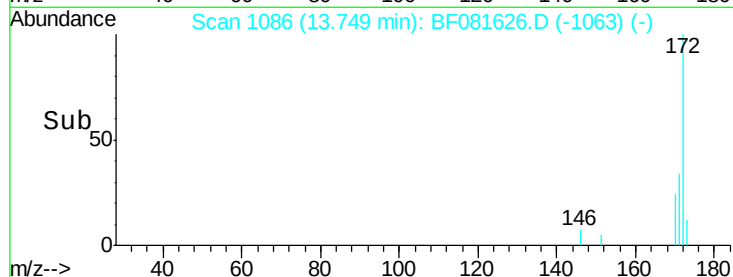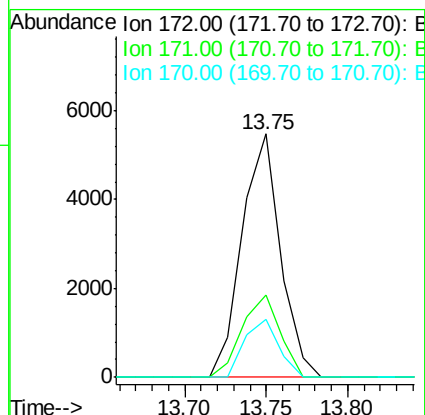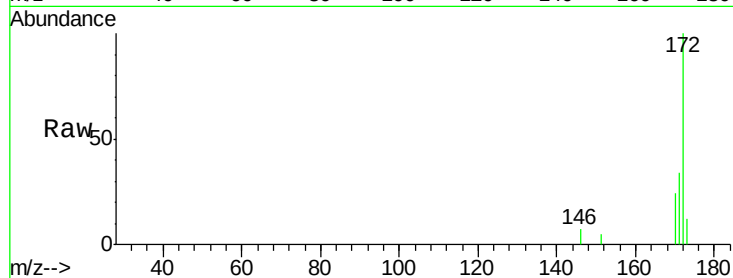

#51
Acenaphthene
Concen: 3.62 ng
RT: 15.32 min Scan# 1223
Delta R.T. -0.03 min
Lab File: BF081626.D
Acq: 15 Sep 2015 12:59

Tgt Ion:154 Resp: 23560
Ion Ratio Lower Upper
154 100
153 123.3 82.1 123.1#
152 60.4 37.9 56.9#

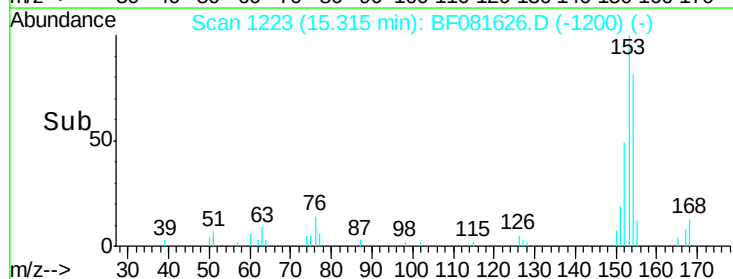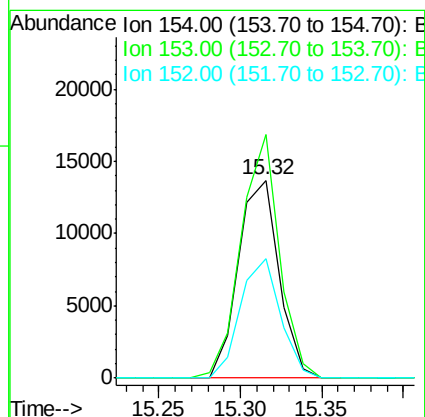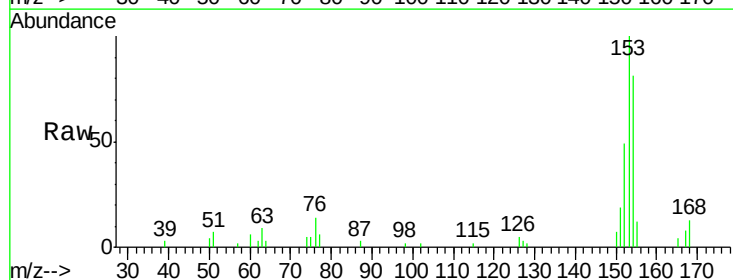



#54

Dibenzofuran

Concen: 3.39 ng

RT: 15.74 min Scan# 1260

Delta R.T. -0.03 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59

Instrument :

BNA_F

ClientSampleId :

GP-3(0-5)DL





Tgt Ion:168 Resp: 32213

Ion Ratio Lower Upper

168 100

139 42.7 24.2 36.2#

169 14.5 10.6 15.8

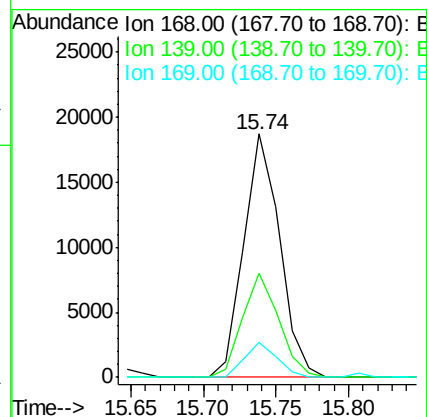

#55

4-Nitrophenol

Concen: 11.33 ng

RT: 15.74 min Scan# 1260

Delta R.T. -0.19 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59




Tgt Ion:139 Resp: 13864


Ion Ratio Lower Upper

139 100

109 0.0 12.7 52.7#

65 0.0 45.9 85.9#



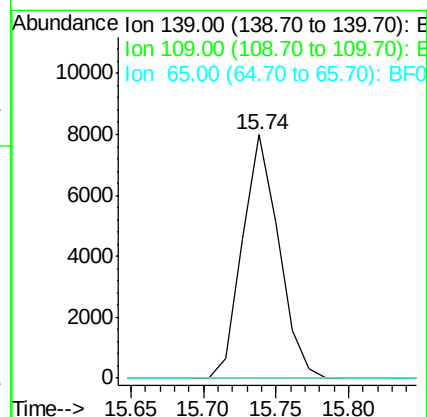



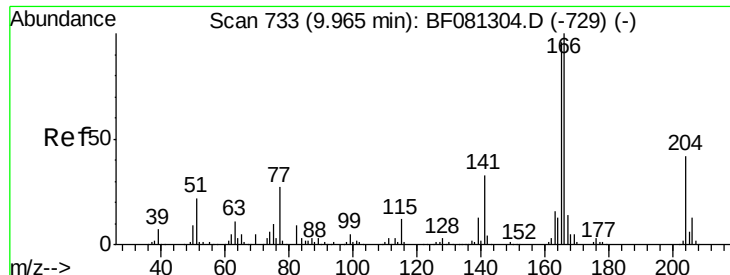

#57
 Fluorene
 Concen: 5.58 ng
 RT: 16.55 min Scan# 1331
 Delta R.T. -0.03 min
 Lab File: BF081626.D
 Acq: 15 Sep 2015 12:59




Instrument :
 BNA_F
 ClientSampleId :
 GP-3(0-5)DL


Tgt Ion:166 Resp: 40192
 Ion Ratio Lower Upper
 166 100
 165 97.3 72.6 109.0
 167 14.4 10.6 16.0

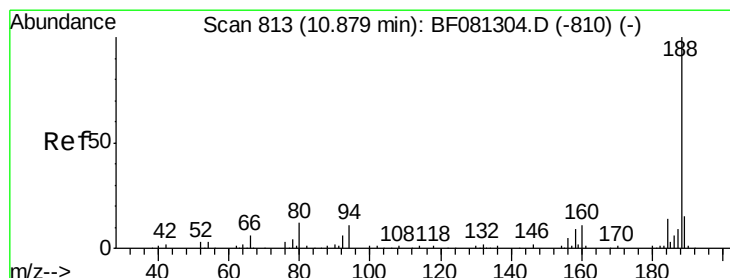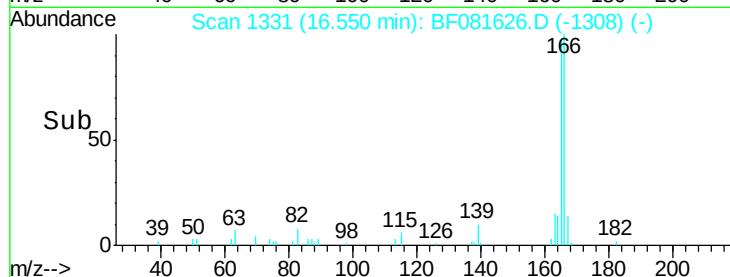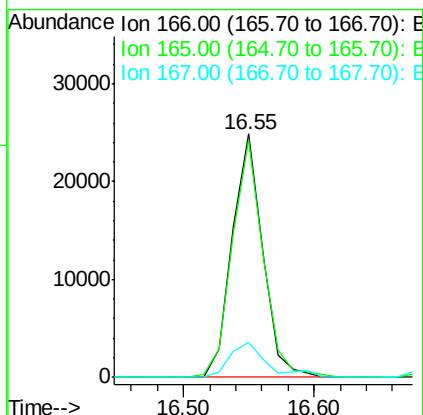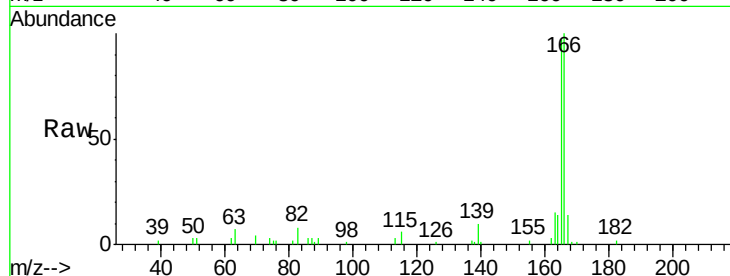

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 18.74 min Scan# 1523
 Delta R.T. -0.02 min
 Lab File: BF081626.D
 Acq: 15 Sep 2015 12:59

Tgt Ion:188 Resp: 185719
 Ion Ratio Lower Upper
 188 100
 94 8.8 11.1 16.7#
 80 9.0 11.0 16.4#

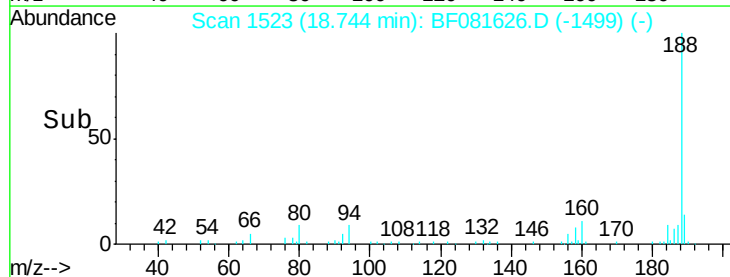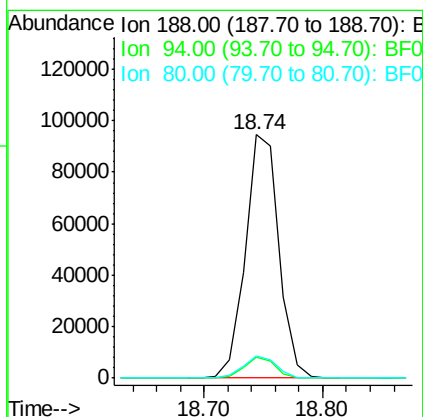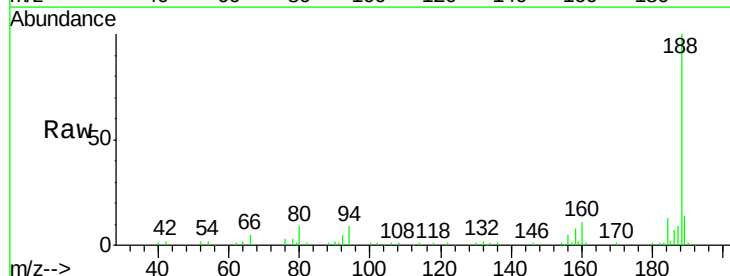







#70
 Phenanthrene
 Concen: 44.14 ng
 RT: 18.81 min Scan# 1529
 Delta R.T. -0.02 min
 Lab File: BF081626.D
 Acq: 15 Sep 2015 12:59

Instrument :
 BNA_F
 ClientSampleId :
 GP-3(0-5)DL

Tgt Ion:178 Resp: 455705
 Ion Ratio Lower Upper
 178 100
 176 19.7 13.8 20.8
 179 15.0 12.2 18.2




Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 176.00 (175.70 to 176.70): E
 Ion 179.00 (178.70 to 179.70): E

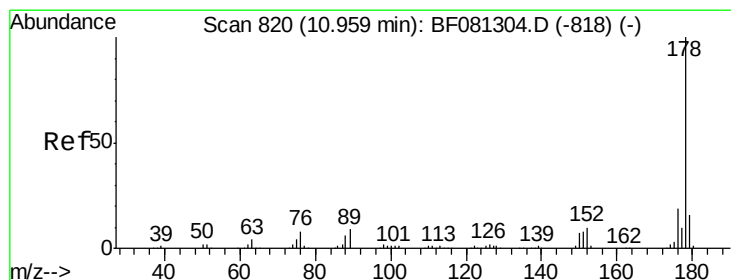
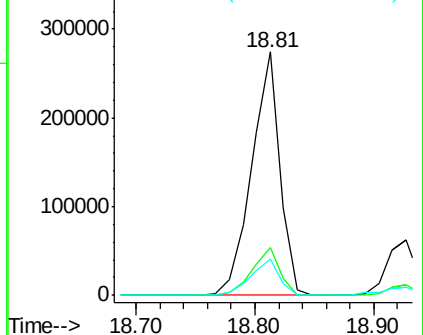



#71
 Anthracene
 Concen: 10.31 ng
 RT: 18.93 min Scan# 1539
 Delta R.T. -0.02 min
 Lab File: BF081626.D
 Acq: 15 Sep 2015 12:59

Tgt Ion:178 Resp: 109337
 Ion Ratio Lower Upper
 178 100
 176 19.3 14.1 21.1
 179 15.5 12.2 18.2

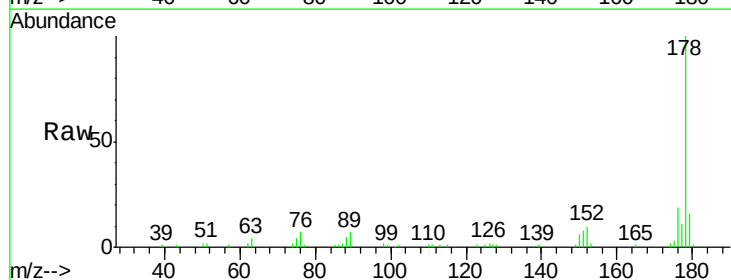

Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 176.00 (175.70 to 176.70): E
 Ion 179.00 (178.70 to 179.70): E

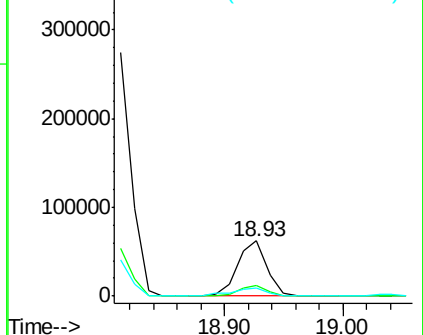



#72

Carbazole

Concen: 2.79 ng

RT: 19.40 min Scan# 1580

Delta R.T. -0.03 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59

Instrument :

BNA_F

ClientSampleId :

GP-3(0-5)DL





Tgt Ion:167 Resp: 27750

Ion Ratio Lower Upper

167 100

166 21.9 15.7 23.5

139 14.5 9.5 14.3#

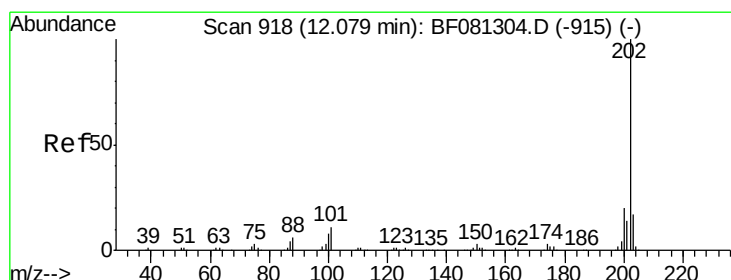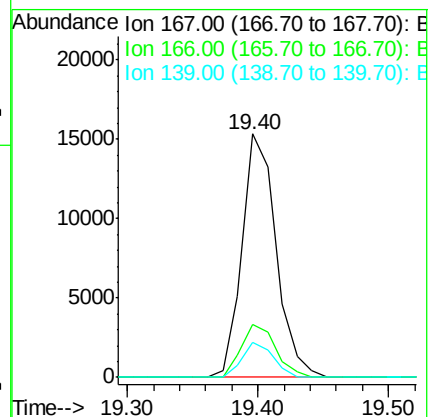

#74

Fluoranthene

Concen: 35.48 ng

RT: 21.43 min Scan# 1758

Delta R.T. -0.01 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59




Tgt Ion:202 Resp: 396543


Ion Ratio Lower Upper

202 100

101 7.9 0.0 38.3

203 17.2 0.0 37.3

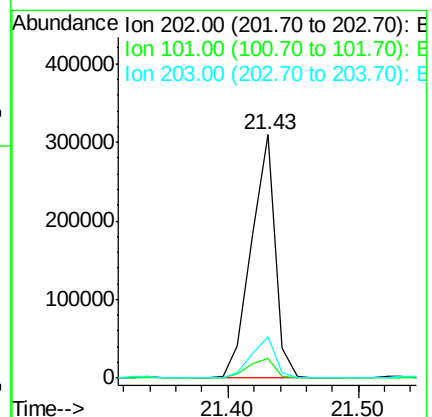



#75

Chrysene-d12

Concen: 20.00 ng

RT: 23.38 min Scan# 1929

Delta R.T. -0.01 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59

Instrument :

BNA_F

ClientSampleId :

GP-3(0-5)DL


Tgt Ion:240 Resp: 126077

Ion Ratio Lower Upper

240 100

120 5.4 16.2 24.2#




236 25.9 18.4 27.6



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

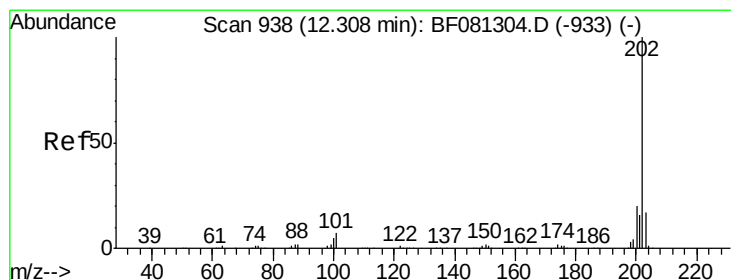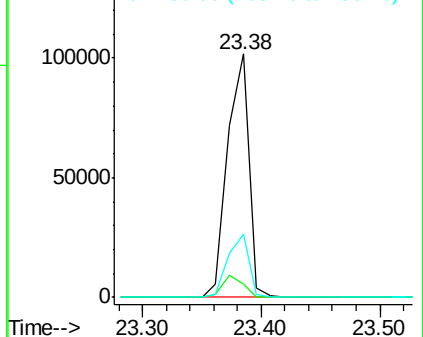

#77

Pyrene

Concen: 37.57 ng

RT: 21.77 min Scan# 1788

Delta R.T. -0.01 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59


Tgt Ion:202 Resp: 350876

Ion Ratio Lower Upper

202 100

200 20.0 15.0 22.4



203 20.1 14.1 21.1




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

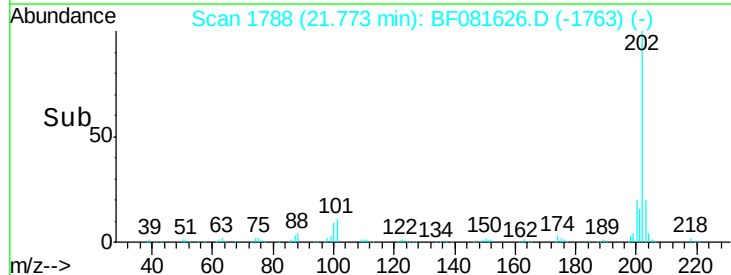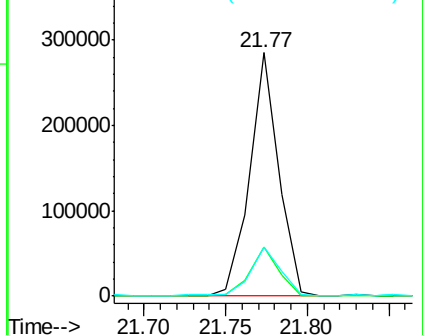



#78

Terphenyl-d14

Concen: 1.39 ng

RT: 22.09 min Scan# 1816

Delta R.T. -0.02 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59

Instrument :

BNA_F

ClientSampleId :

GP-3(0-5)DL


Tgt Ion:244 Resp: 7546

Ion Ratio Lower Upper

244 100

212 11.0 4.3 6.5#




122 12.0 17.4 26.2#

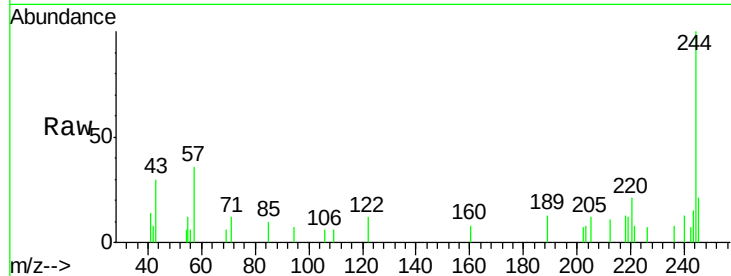

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

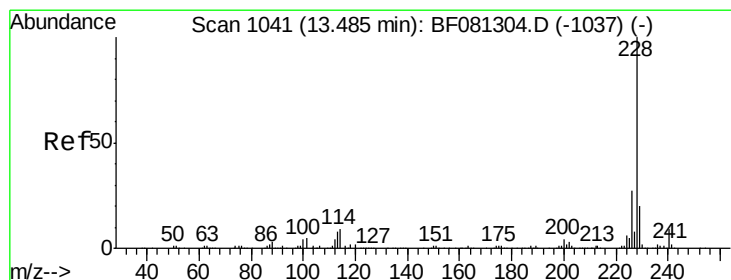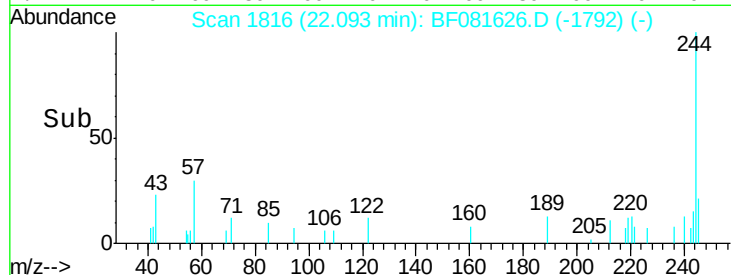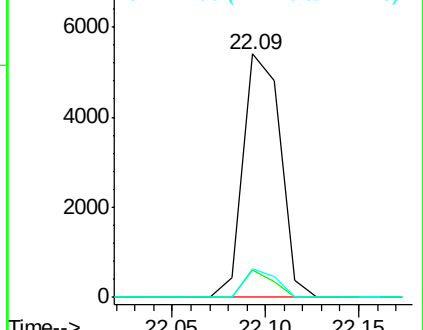

#80

Benzo(a)anthracene

Concen: 16.80 ng

RT: 23.37 min Scan# 1928

Delta R.T. -0.00 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59


Tgt Ion:228 Resp: 134860

Ion Ratio Lower Upper

228 100

226 28.0 20.0 30.0



229 19.7 15.4 23.2




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E




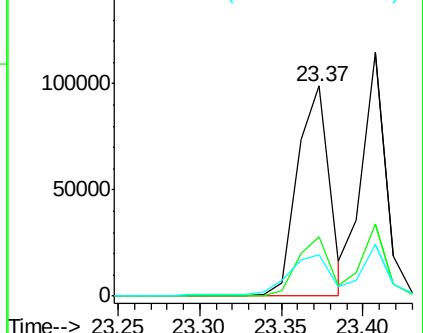




#82
 Chrysene
 Concen: 16.54 ng
 RT: 23.41 min Scan# 1931
 Delta R.T. -0.01 min
 Lab File: BF081626.D
 Acq: 15 Sep 2015 12:59




Instrument :
 BNA_F
 ClientSampleId :
 GP-3(0-5)DL


Tgt Ion: 228 Resp: 119063
 Ion Ratio Lower Upper
 228 100
 226 29.7 21.0 31.4
 229 21.4 15.6 23.4

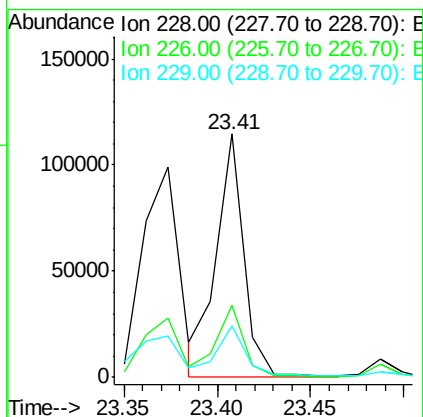

#85
 Indeno(1,2,3-cd)pyrene
 Concen: 8.66 ng
 RT: 25.86 min Scan# 2146
 Delta R.T. -0.01 min
 Lab File: BF081626.D
 Acq: 15 Sep 2015 12:59

Tgt Ion: 276 Resp: 45711
 Ion Ratio Lower Upper
 276 100
 138 19.1 25.7 38.5#
 277 23.4 15.6 23.4


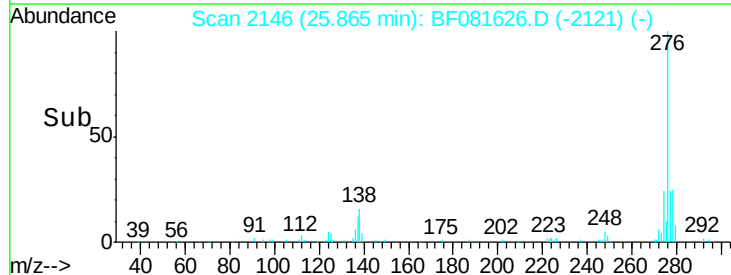
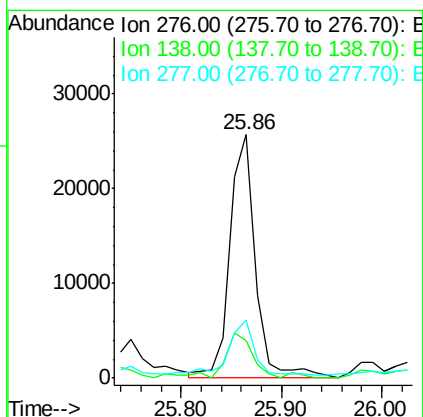





#86
Perylene-d12
Concen: 20.00 ng
RT: 24.81 min Scan# 2054
Delta R.T. -0.01 min
Lab File: BF081626.D
Acq: 15 Sep 2015 12:59




Instrument :
BNA_F
ClientSampleId :
GP-3(0-5)DL


Tgt Ion:264 Resp: 91370
Ion Ratio Lower Upper
264 100
260 24.4 16.7 25.1
265 21.5 17.2 25.8

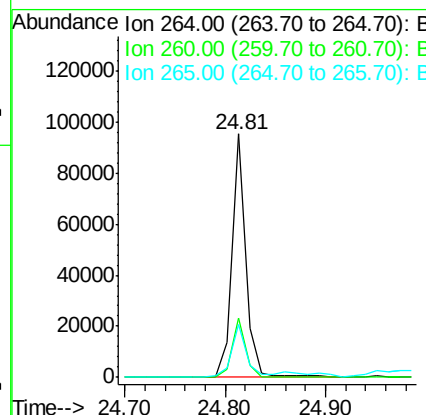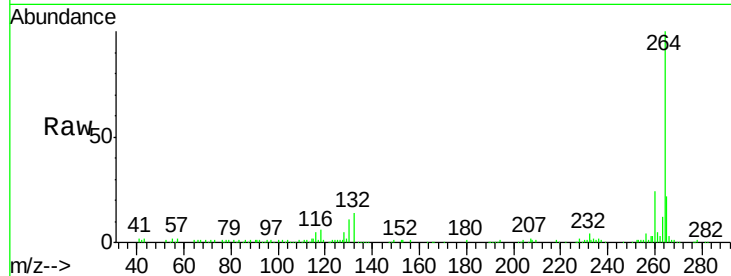

#87
Benzo(b)fluoranthene
Concen: 19.53 ng
RT: 24.47 min Scan# 2024
Delta R.T. -0.01 min
Lab File: BF081626.D
Acq: 15 Sep 2015 12:59

Tgt Ion:252 Resp: 127415
Ion Ratio Lower Upper
252 100
253 23.5 17.5 26.3
125 11.4 17.1 25.7#

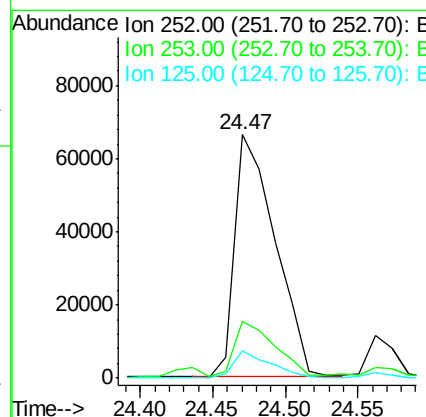



#88

Benzo(k)fluoranthene

Concen: 23.48 ng

RT: 24.47 min Scan# 2024

Delta R.T. -0.03 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59





Instrument :

BNA_F

ClientSampleId :

GP-3(0-5)DL

Tgt Ion:	252	Resp:	127097
Ion Ratio	Lower	Upper	
252	100		
253	23.5	17.0	25.4
125	11.4	16.0	24.0#

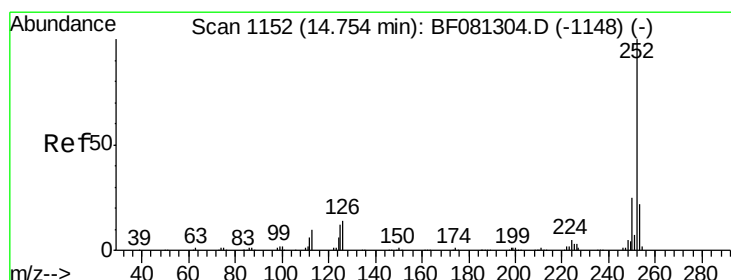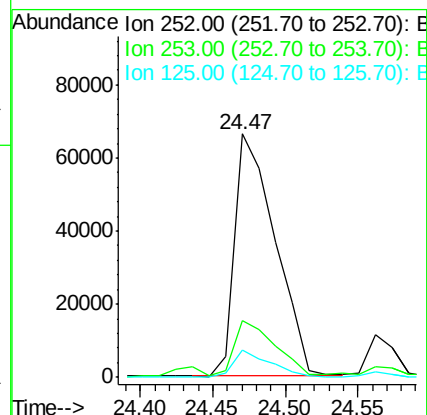

#89

Benzo(a)pyrene

Concen: 13.65 ng




RT: 24.77 min Scan# 2050


Delta R.T. -0.01 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59

Tgt Ion:	252	Resp:	75458
Ion Ratio	Lower	Upper	
252	100		
253	23.4	17.2	25.8
125	7.5	18.0	27.0#

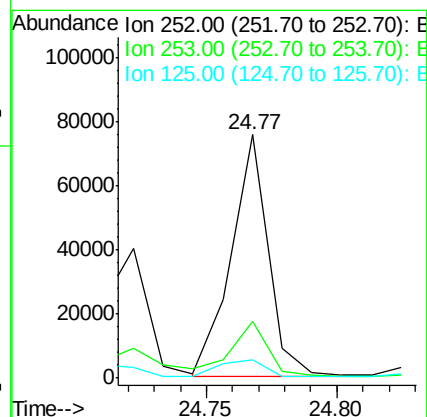



#90

Dibenzo(a,h)anthracene

Concen: 2.38 ng

RT: 25.86 min Scan# 2146

Delta R.T. -0.02 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59

Instrument :

BNA_F

ClientSampleId :

GP-3(0-5)DL


Tgt Ion:278 Resp: 10162

Ion Ratio Lower Upper

278 100

139 17.8 26.3 39.5#




279 33.2 18.2 27.4#

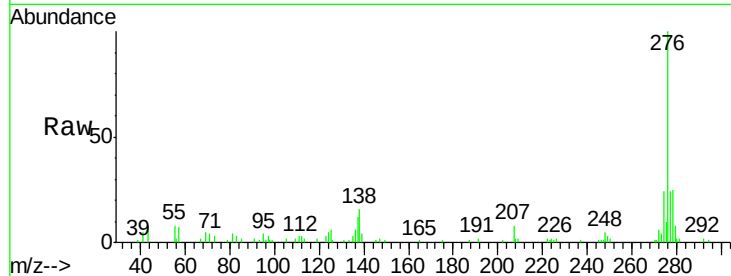

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

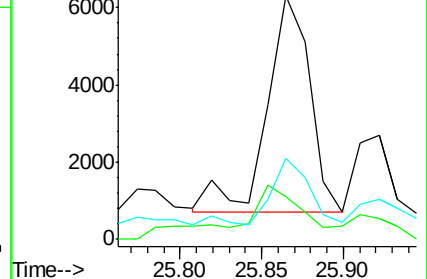

#91

Benzo(g,h,i)perylene

Concen: 9.85 ng

RT: 26.16 min Scan# 2172

Delta R.T. -0.02 min

Lab File: BF081626.D

Acq: 15 Sep 2015 12:59


Tgt Ion:276 Resp: 40154

Ion Ratio Lower Upper

276 100

277 25.4 17.8 26.6

138 18.6 34.6 51.8#



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

