
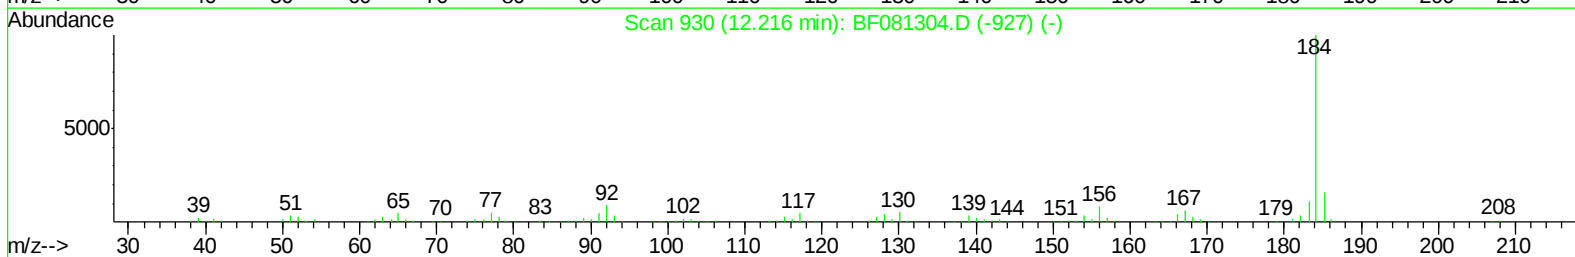
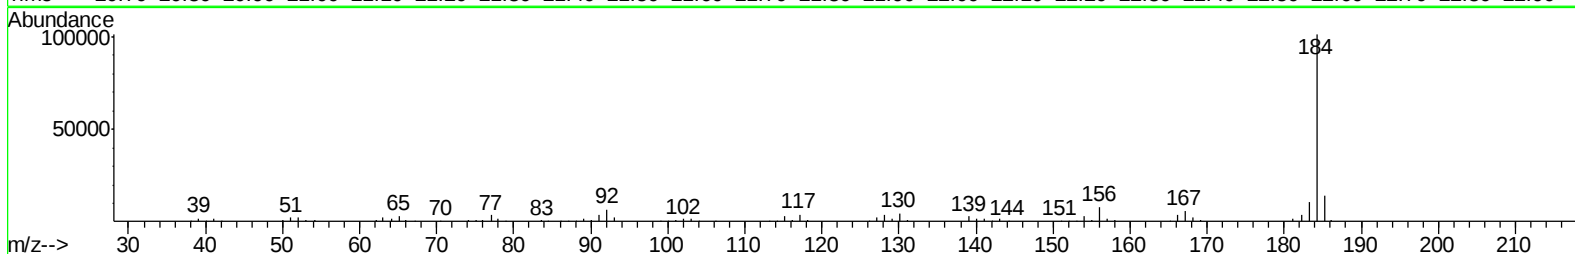


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091515\
Data File : BF081624.D
Acq On : 15 Sep 2015 11:06
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 17:23:02 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 15 14:03:59 2015
Response via : Initial Calibration

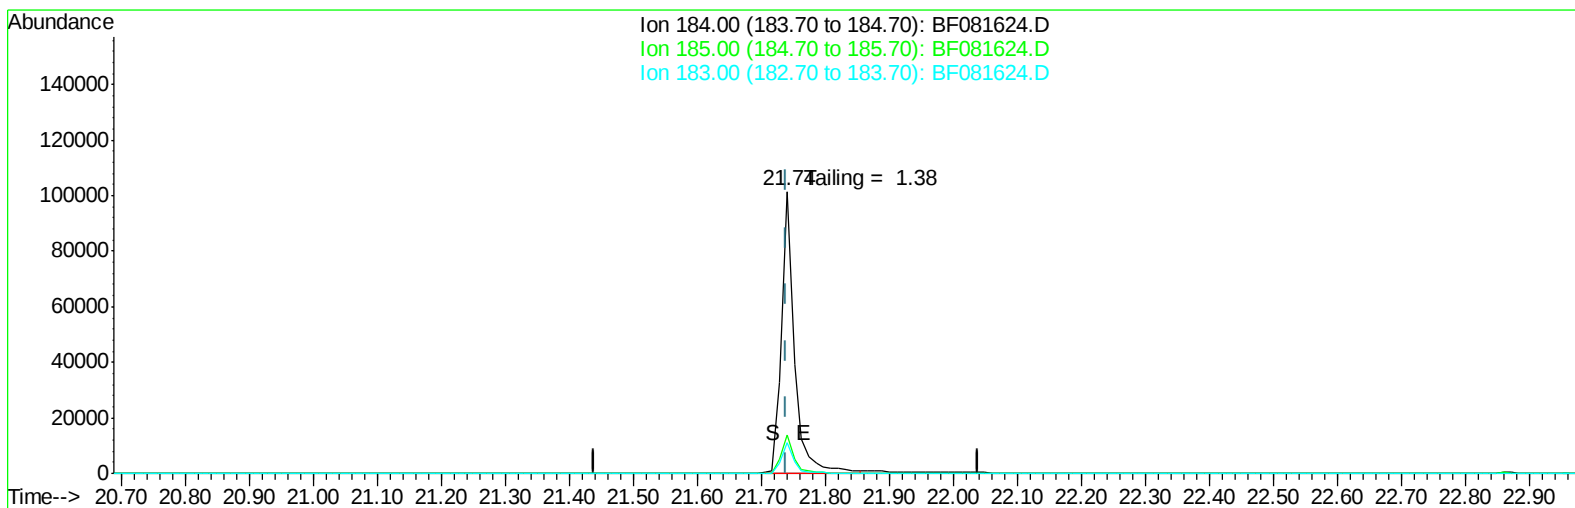

TIC: BF081624.D

(76) Benzidine




21.739min (+0.000) 0.00ng

response 145234

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.78
183.00	9.50	10.86
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091515\
Data File : BF081624.D
Acq On : 15 Sep 2015 11:06
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 17:23:02 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 15 14:03:59 2015
Response via : Initial Calibration

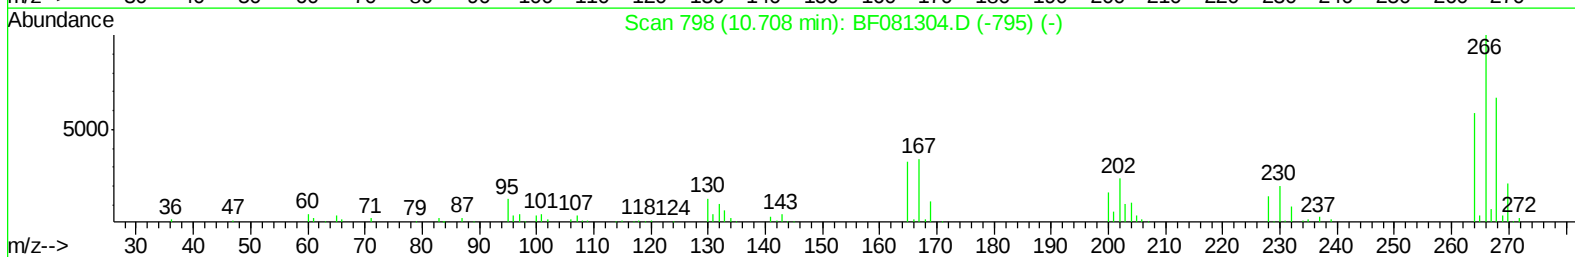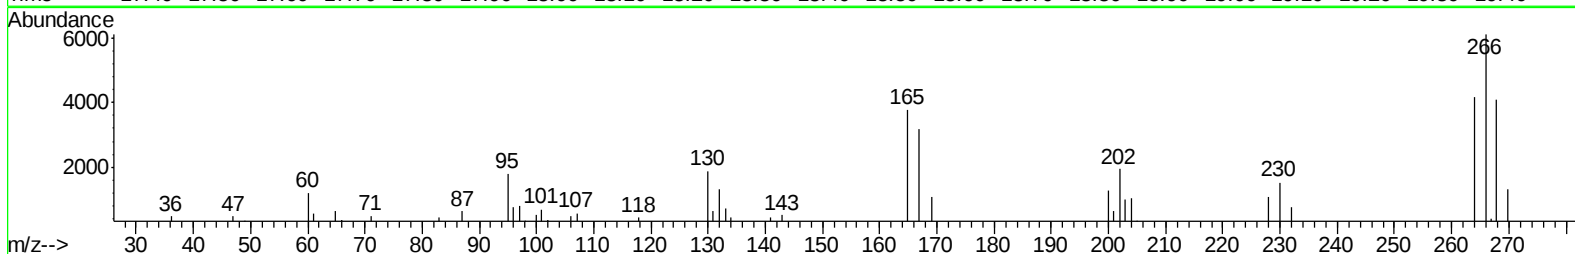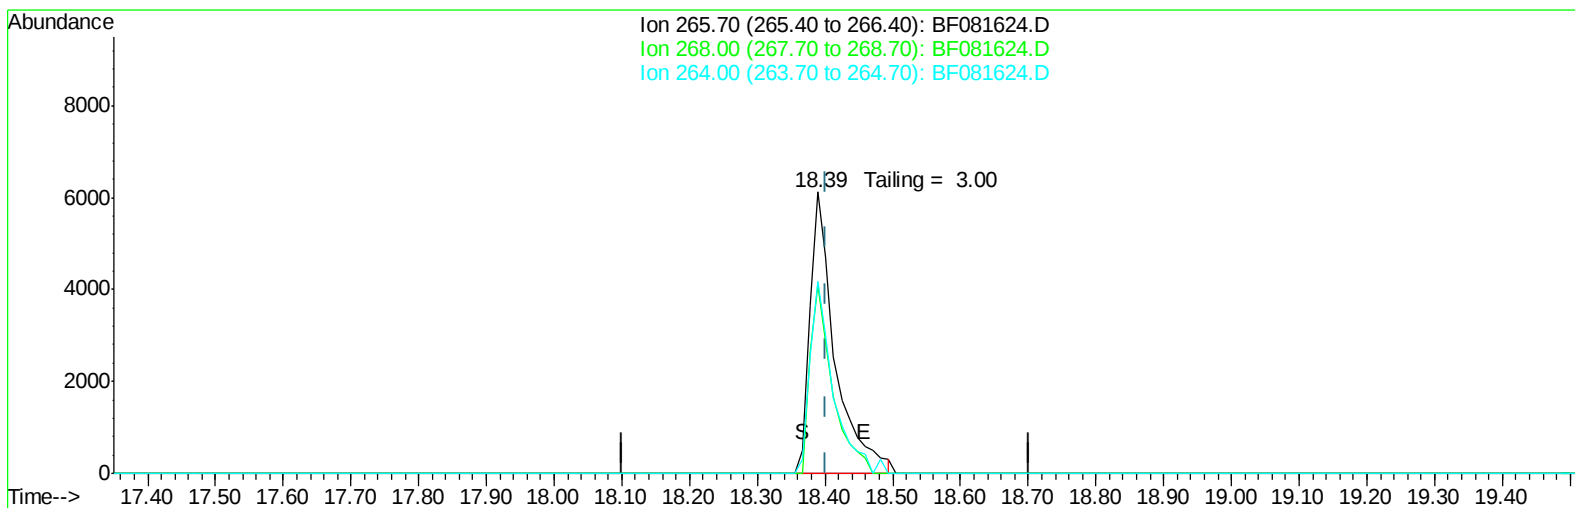

TIC: BF081624.D

(69) Pentachlorophenol (C)

18.390min (-0.011) 0.00ng

response 15642

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	66.84
264.00	62.70	68.34
0.00	0.00	0.00