



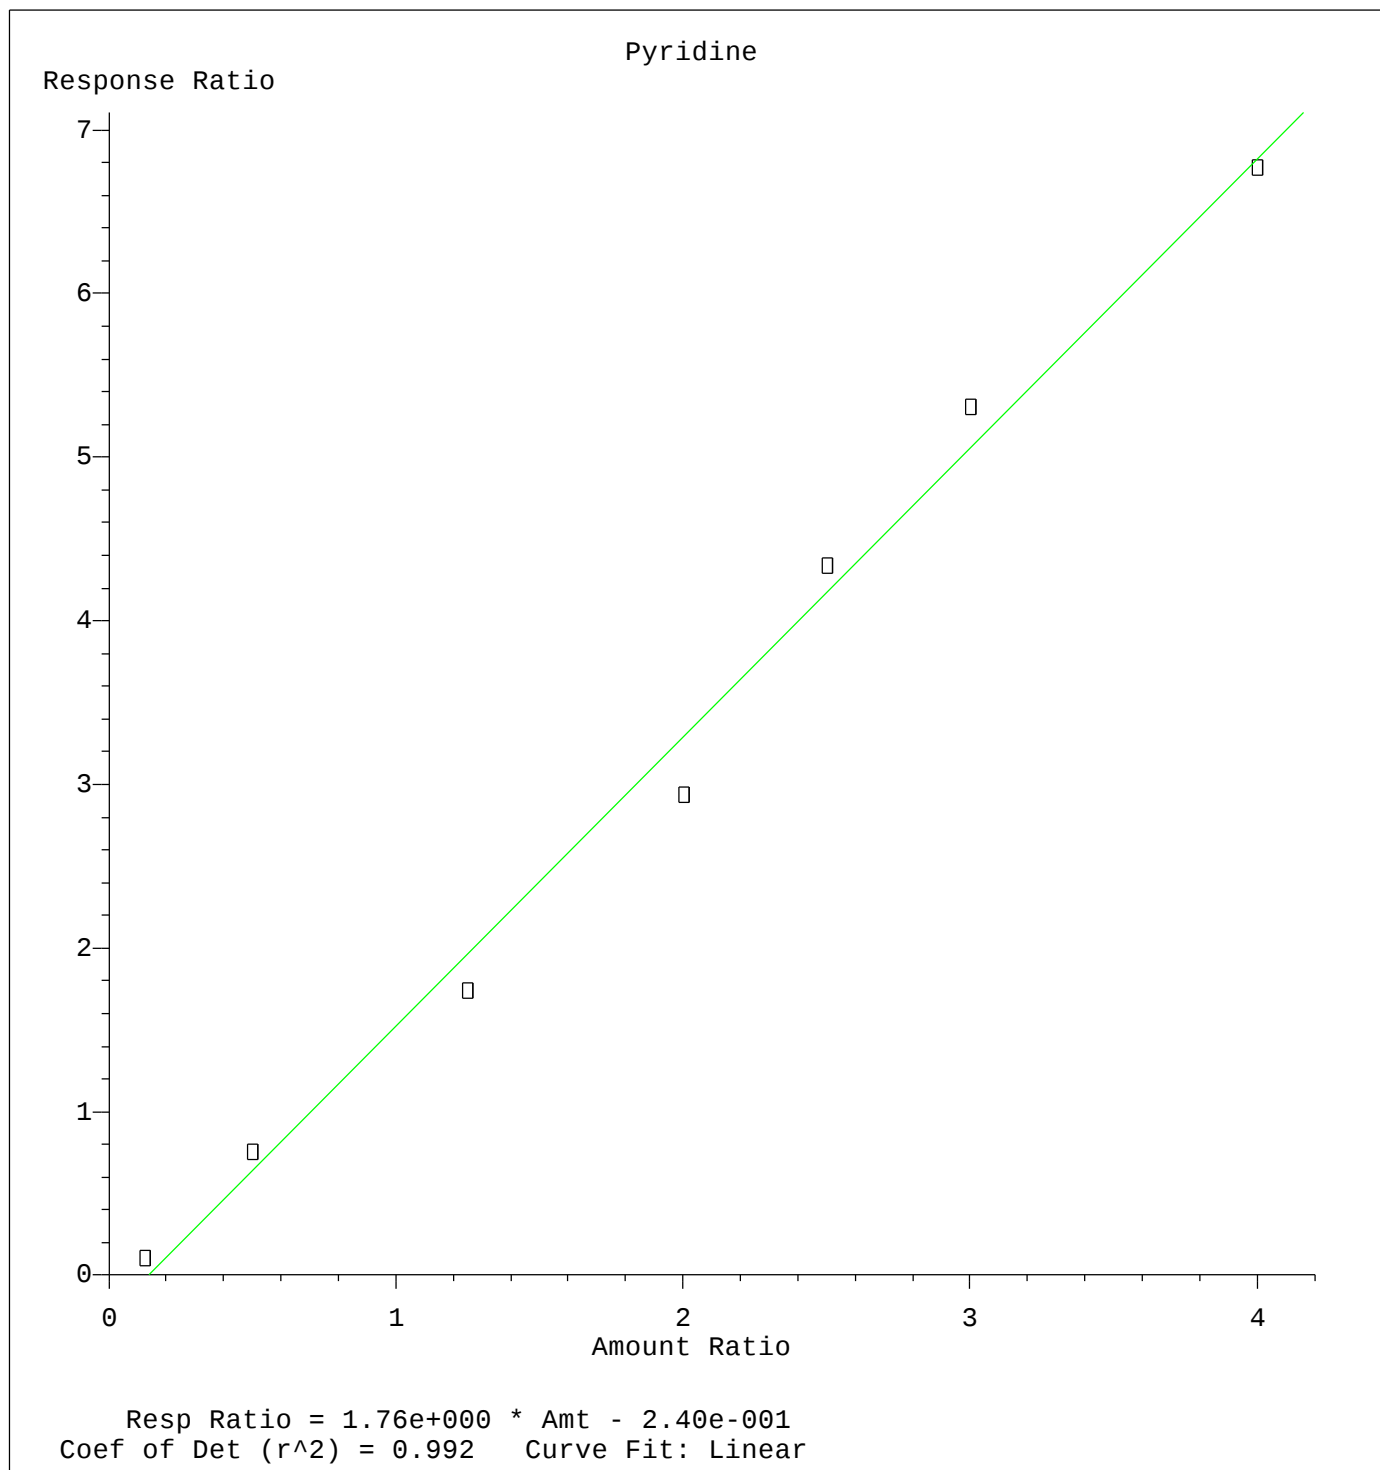

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF091516.M
Calibration Table Last Updated: Thu Sep 15 11:18:43 2016


n-Nitrosodimethylamine

Response Ratio

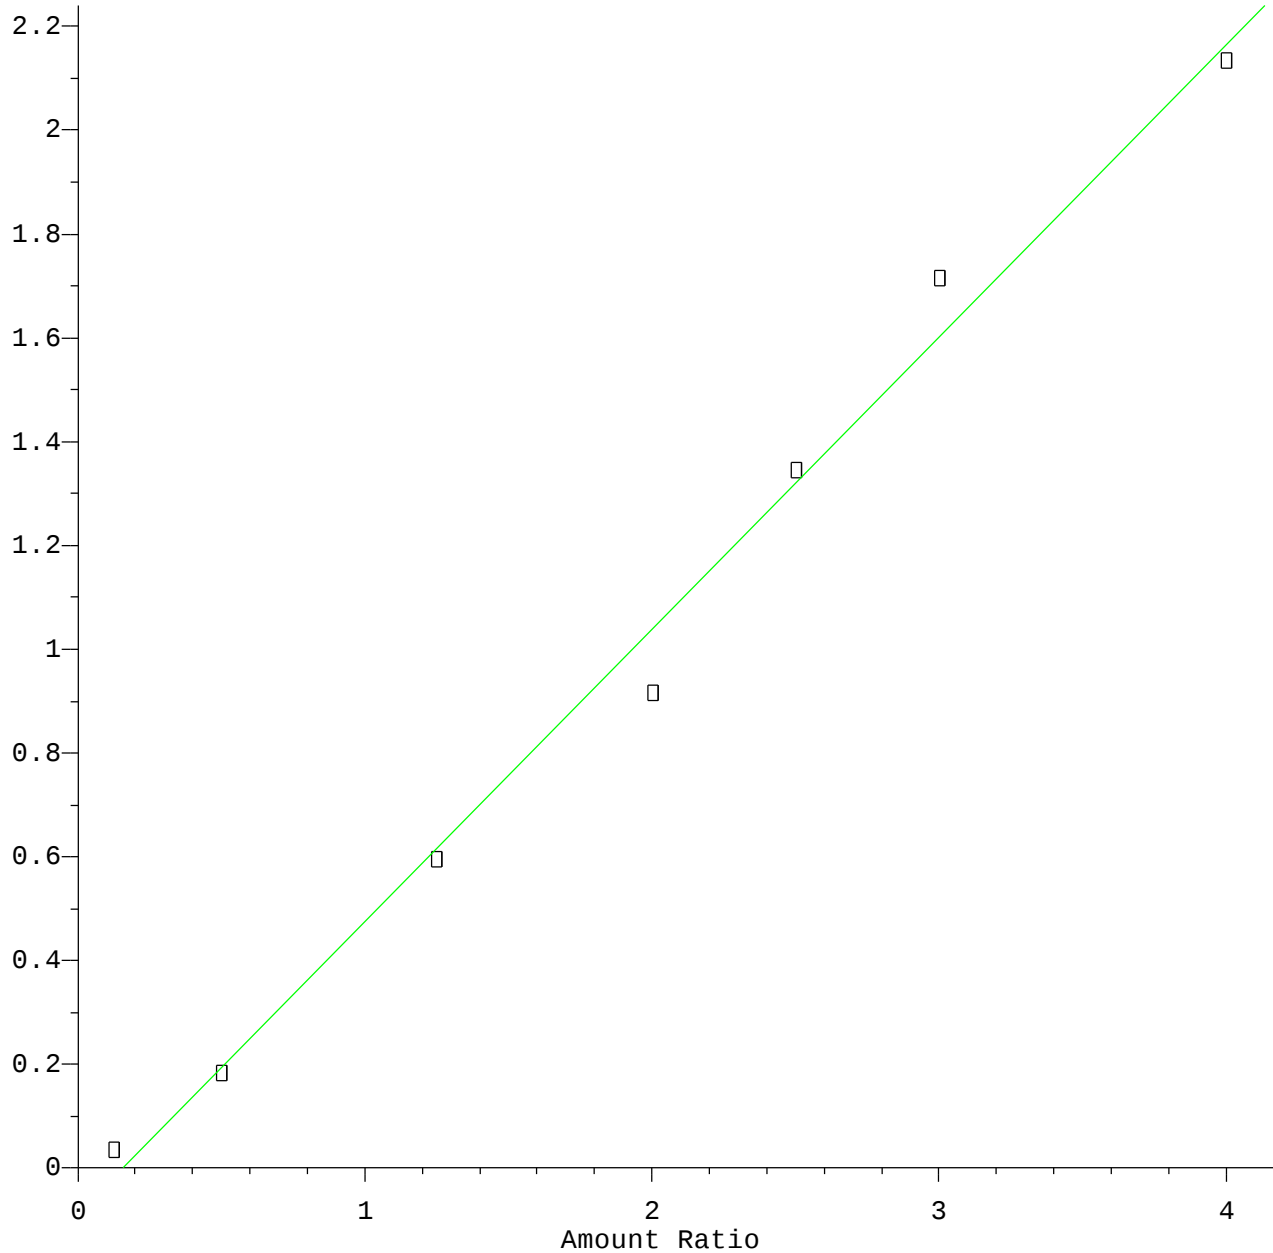


Resp Ratio = $5.63 \times 10^{-1} \times \text{Amt} - 8.70 \times 10^{-2}$
Coef of Det (r^2) = 0.991 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF091516.M
Calibration Table Last Updated: Thu Sep 15 11:18:43 2016

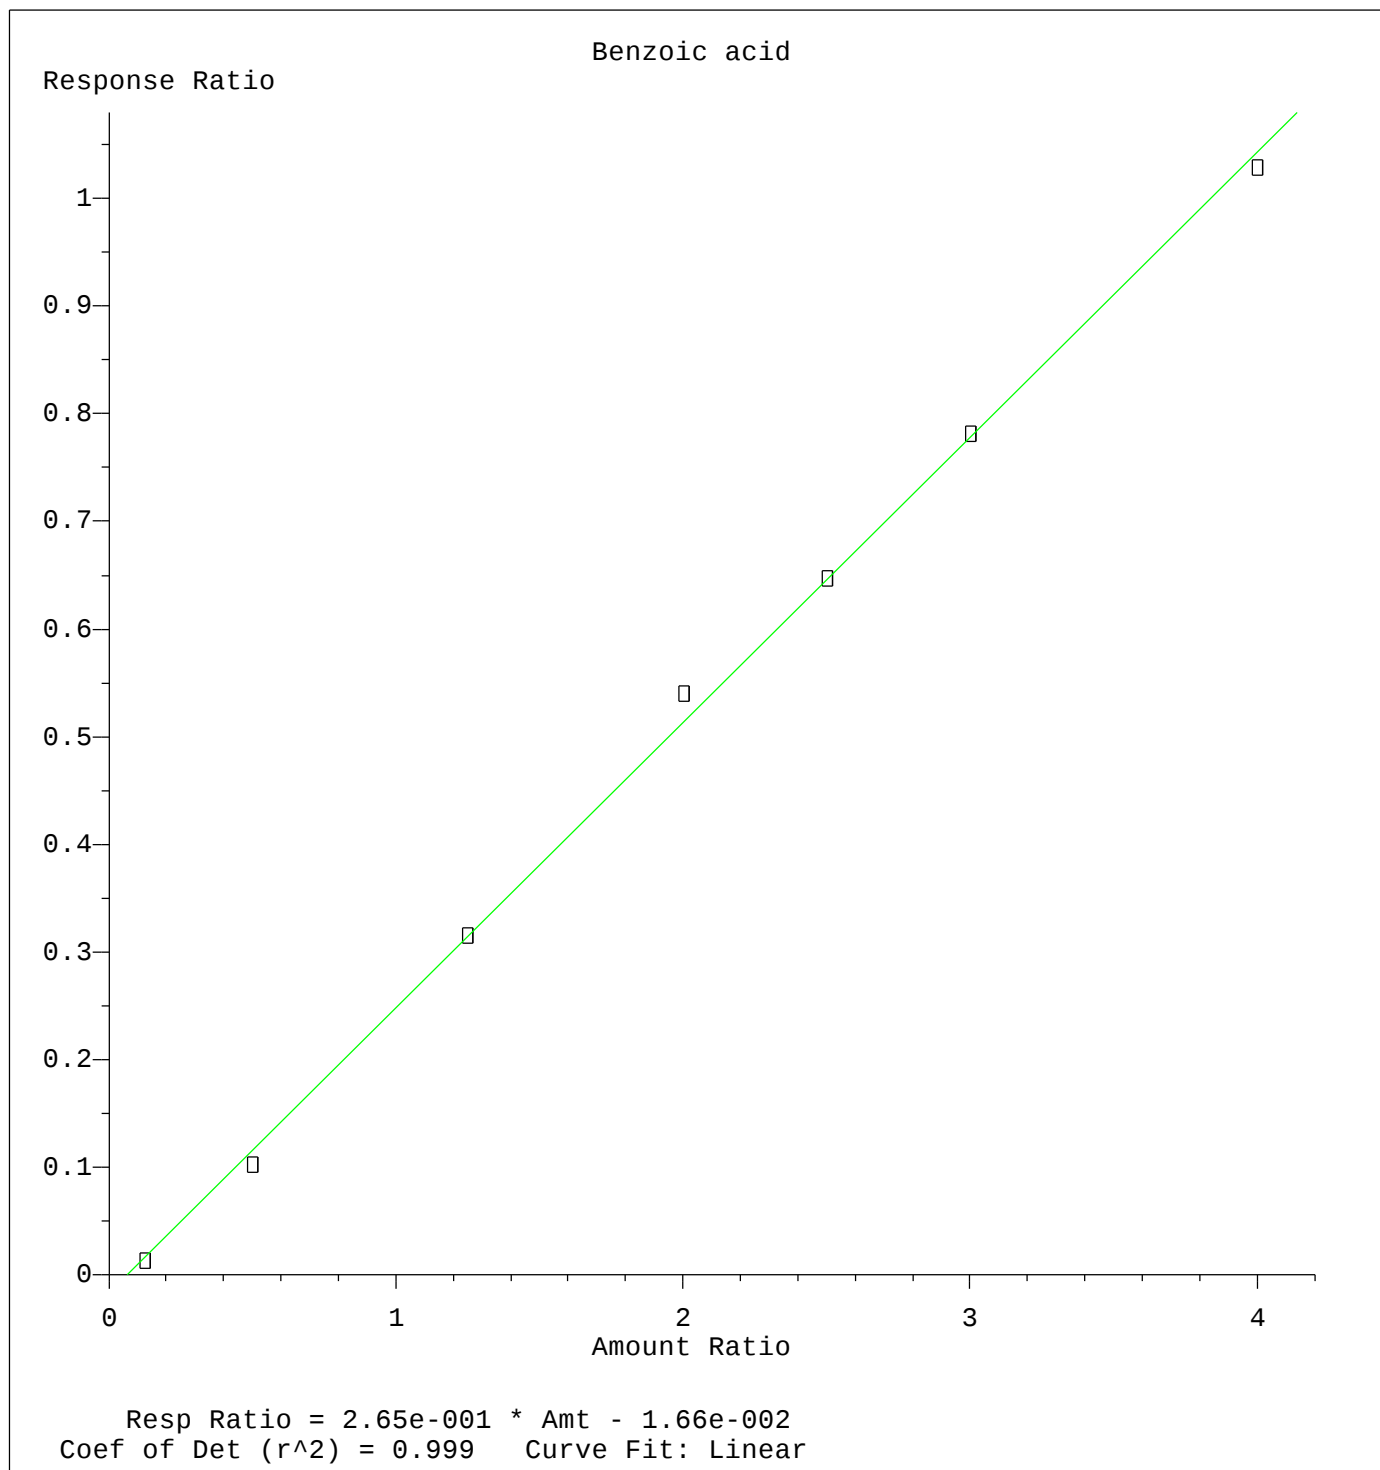


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF091516.M
Calibration Table Last Updated: Thu Sep 15 11:18:43 2016

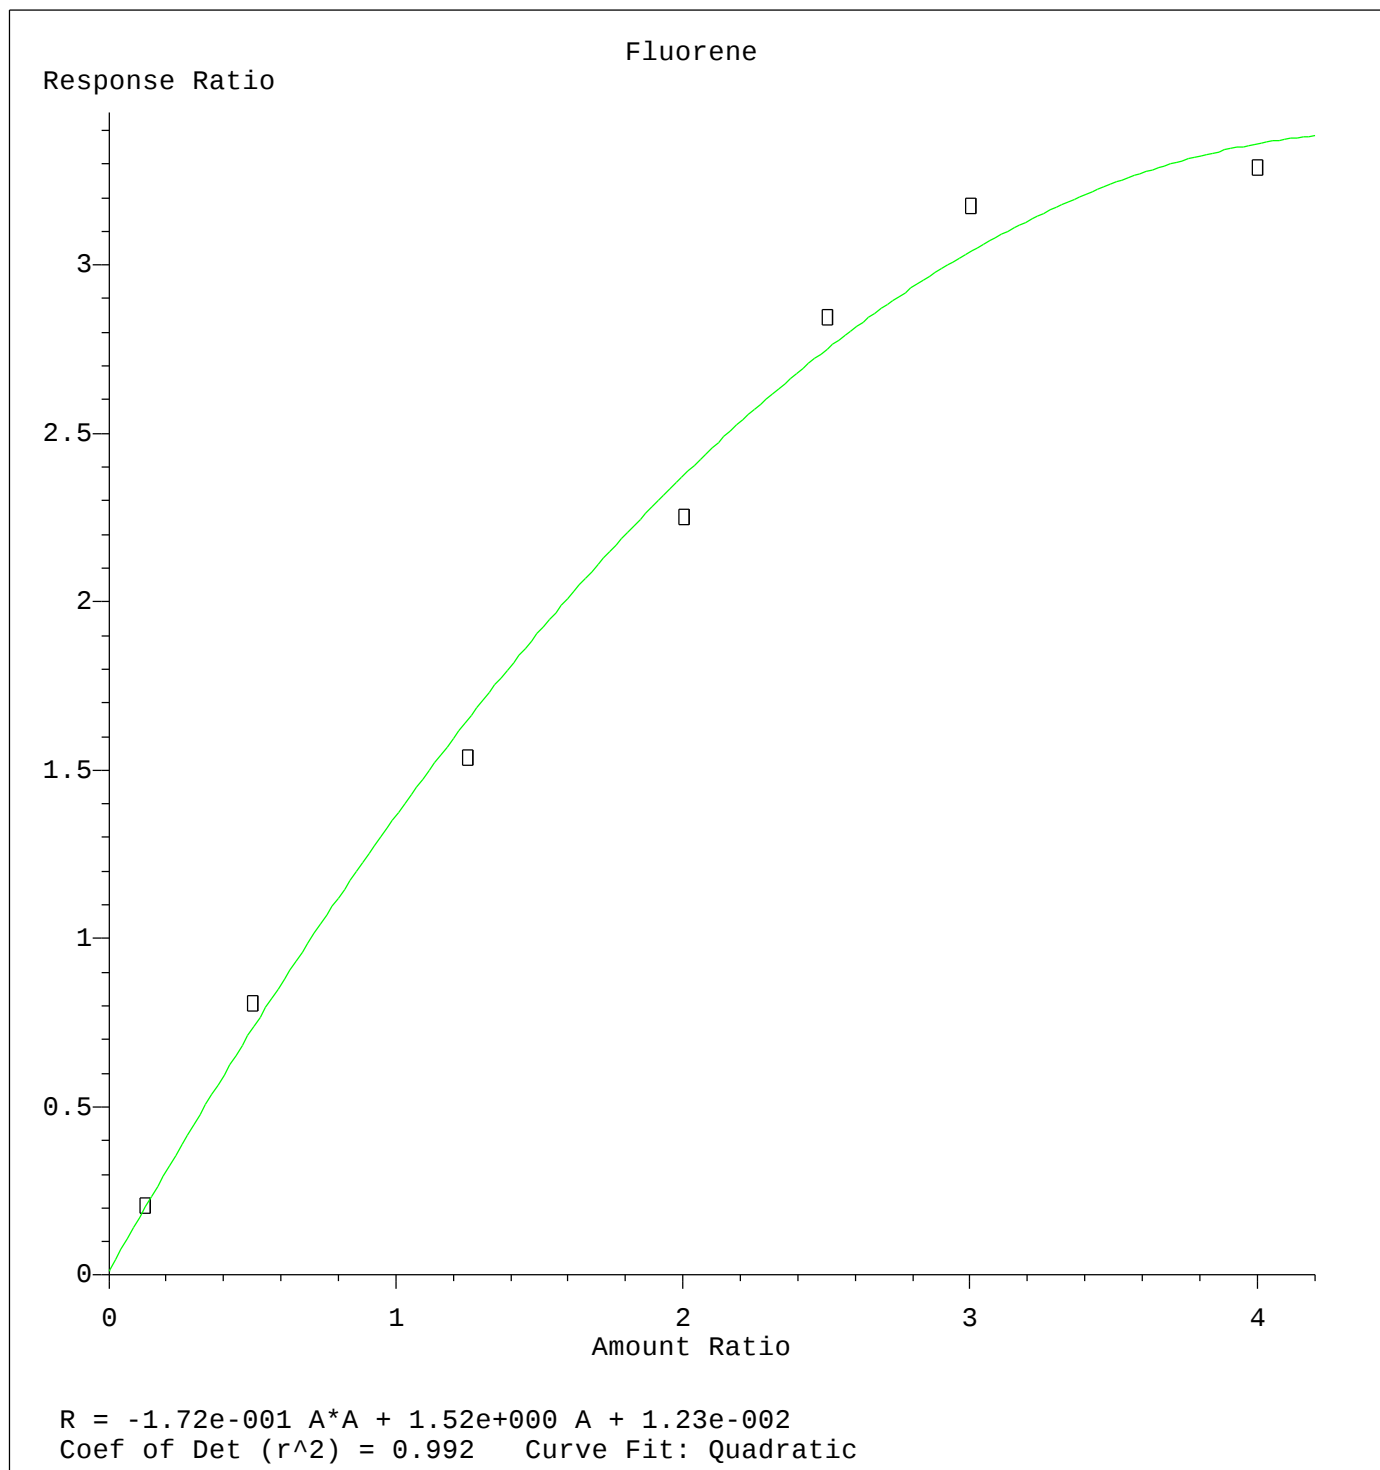

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF091516.M
Calibration Table Last Updated: Thu Sep 15 11:18:43 2016

4-Chlorophenyl-phenylether


Response Ratio

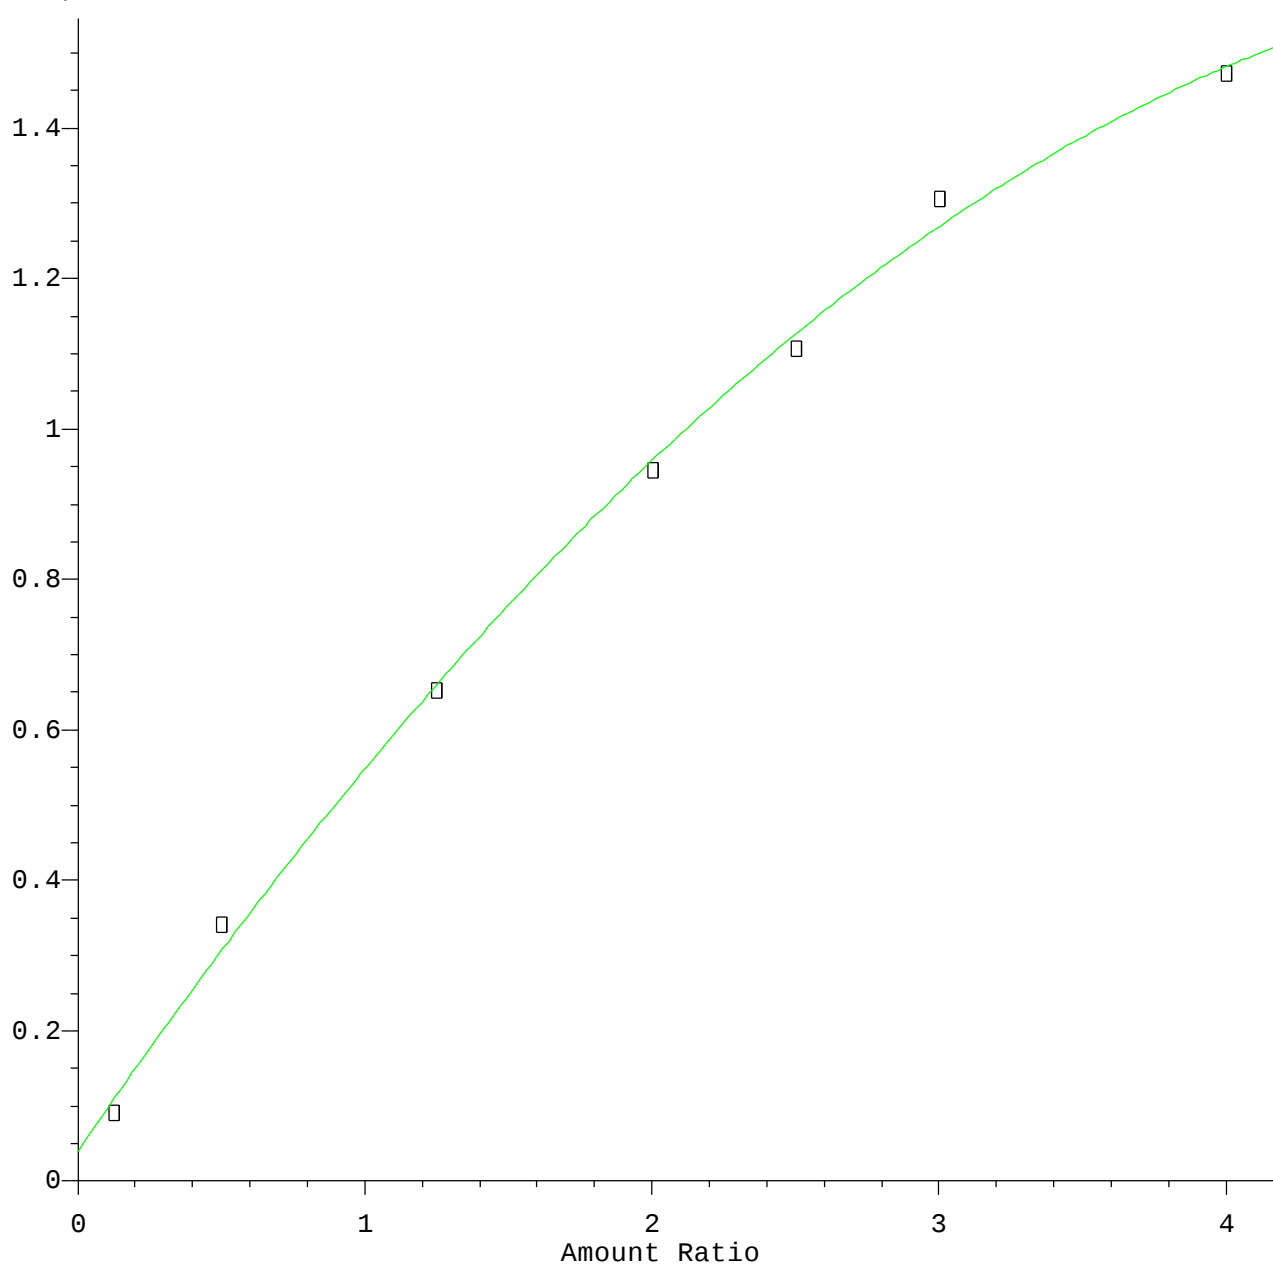

$R = -4.94e-002 A^2 + 5.58e-001 A + 4.02e-002$
Coef of Det (r^2) = 0.998 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF091516.M
Calibration Table Last Updated: Thu Sep 15 11:18:43 2016

4,6-Dinitro-2-methylphenol

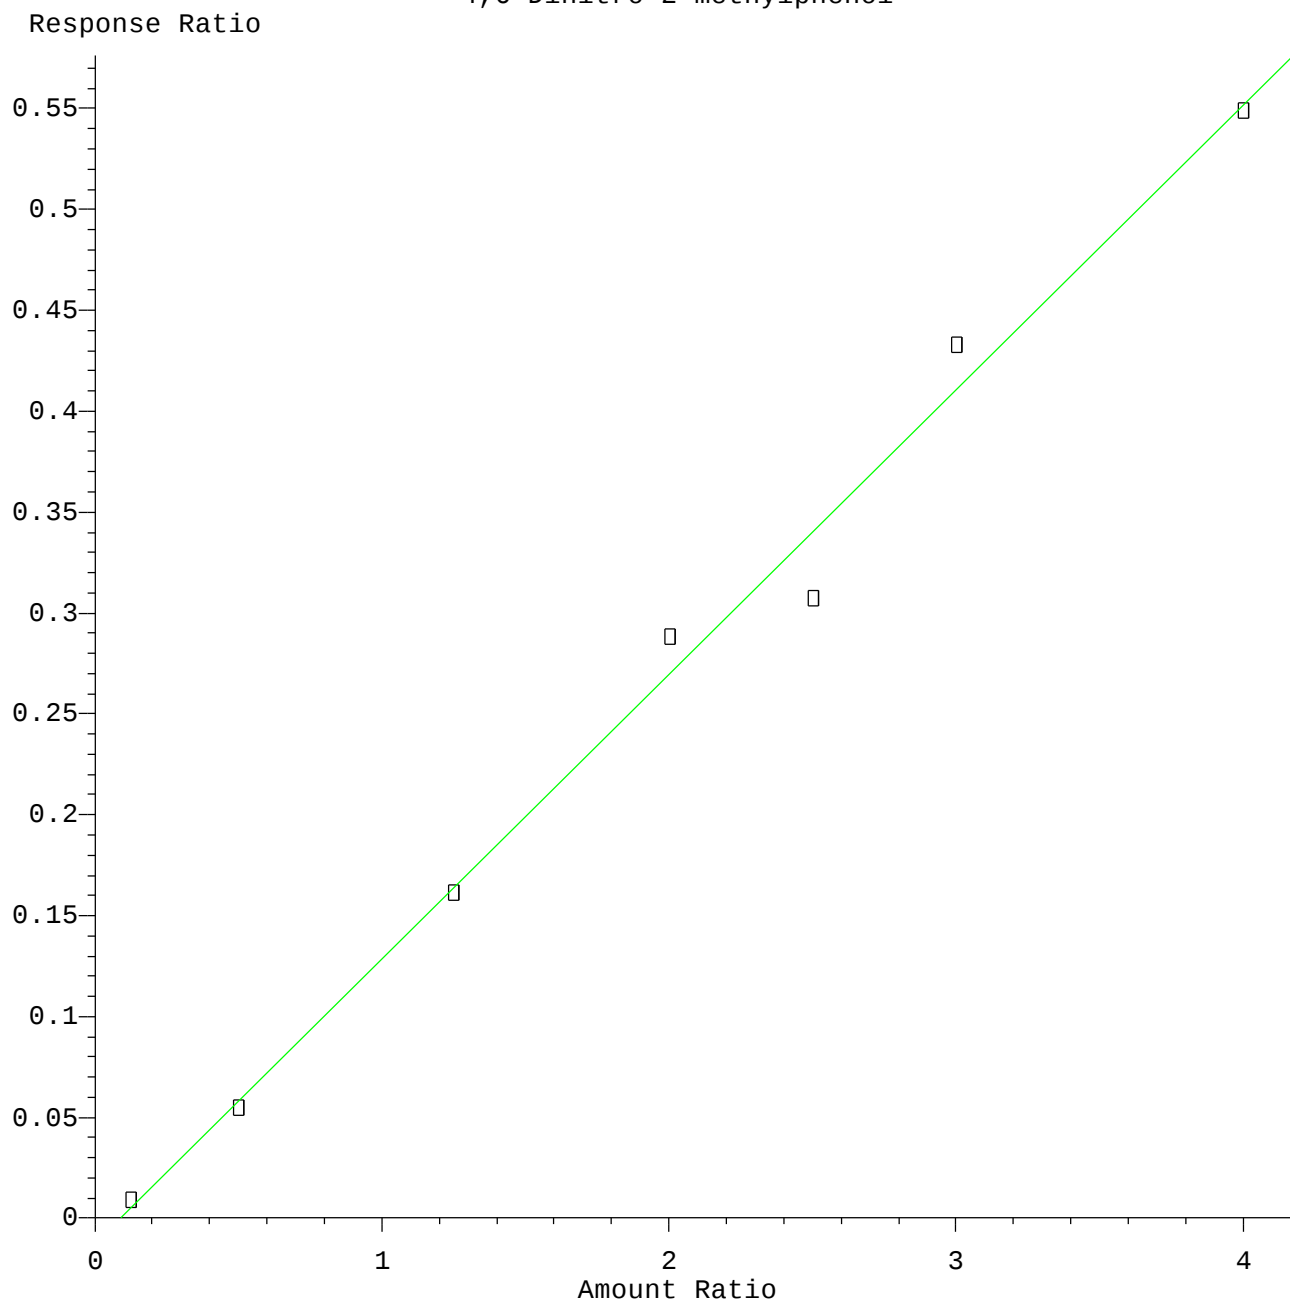

Resp Ratio = $1.41 \times 10^{-1} \times \text{Amt} - 1.23 \times 10^{-2}$
Coef of Det (r^2) = 0.991 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF091516.M
Calibration Table Last Updated: Thu Sep 15 11:18:43 2016