
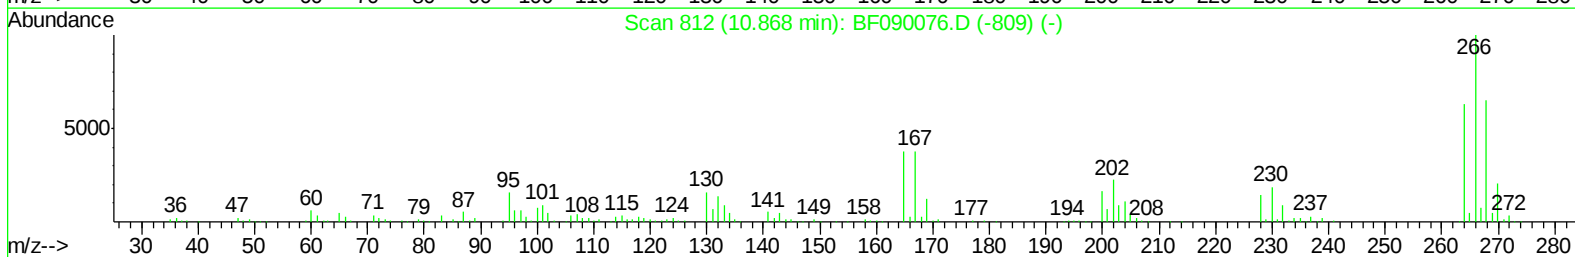
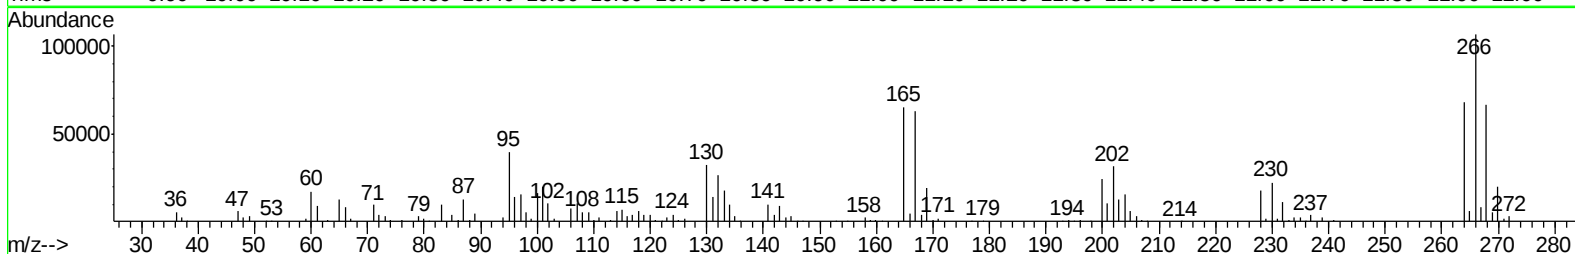


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091516\
Data File : BF090081.D
Acq On : 15 Sep 2016 8:48
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 01:59:00 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 15 11:18:43 2016
Response via : Initial Calibration

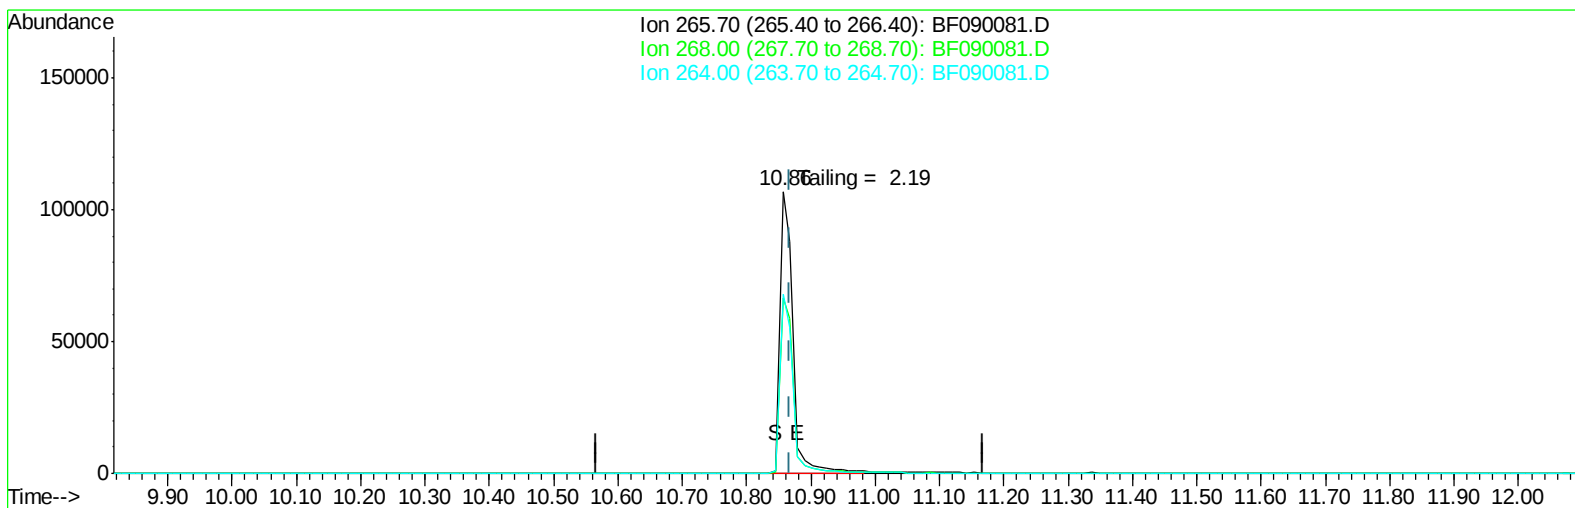

TIC: BF090081.D

(69) Pentachlorophenol (C)




10.856min (-0.011) 111516.14ng

response 156580

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	62.51
264.00	62.90	63.87
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091516\
Data File : BF090081.D
Acq On : 15 Sep 2016 8:48
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 01:59:00 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 15 11:18:43 2016
Response via : Initial Calibration

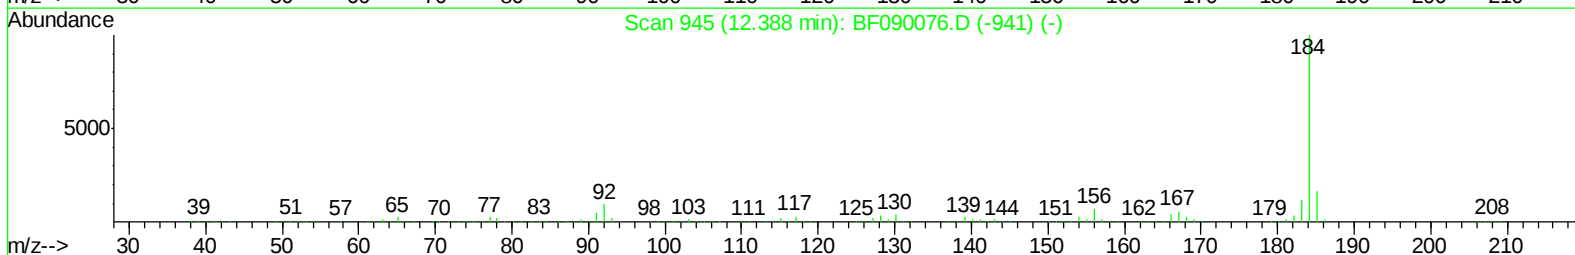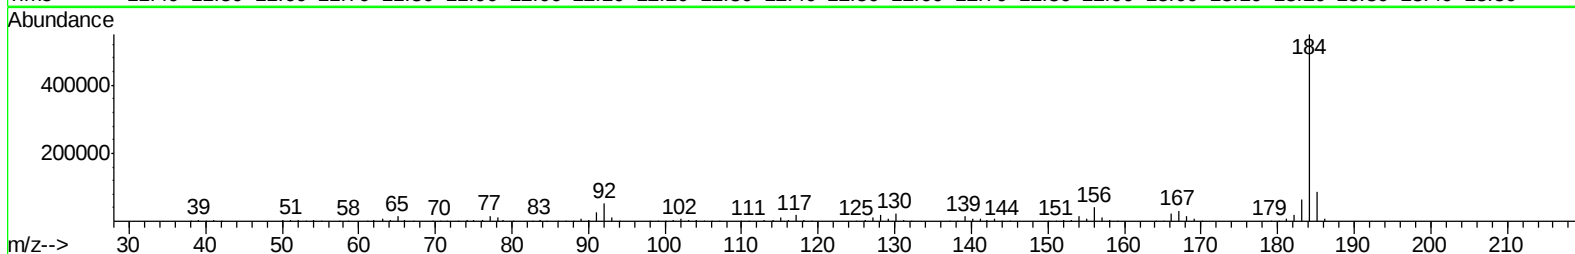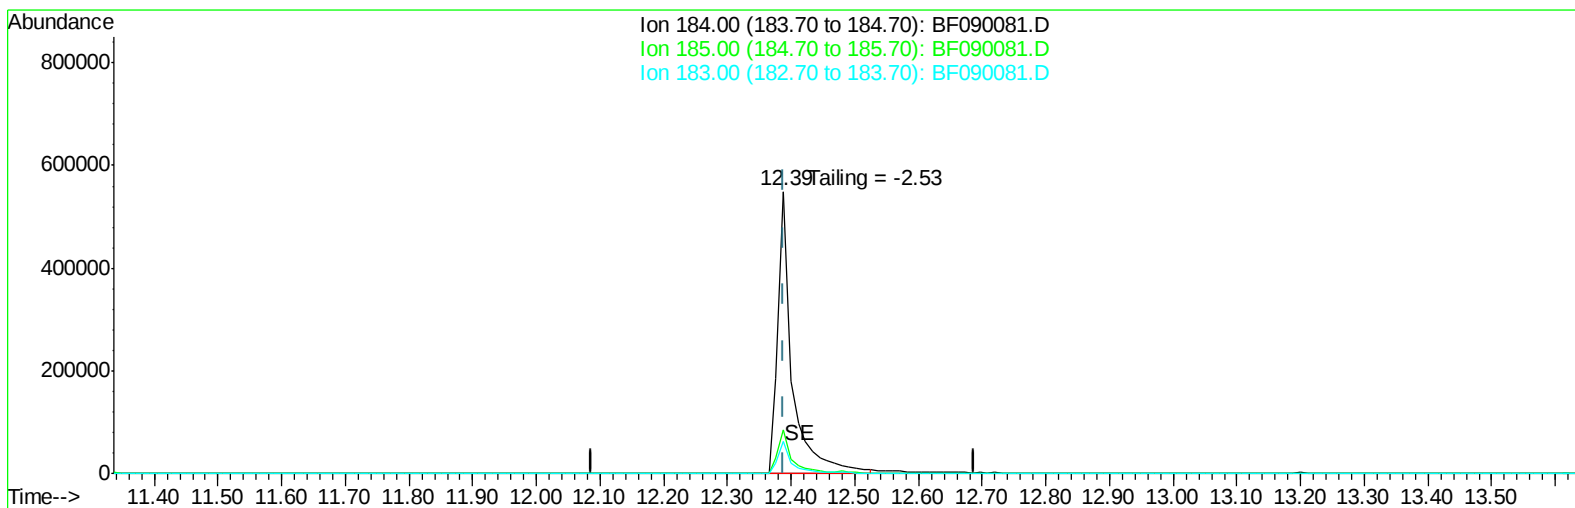

TIC: BF090081.D

(76) Benzidine

12.388min (+0.000) 33102.39ng m

response 854724

Ion	Exp%	Act%
184.00	100	100
185.00	16.50	15.65
183.00	11.50	11.59
0.00	0.00	0.00