


Data Path : Z:\HPCHEM1\BNA_F\Data\BF091516\
 Data File : BF090072.D
 Acq On : 15 Sep 2016 1:44
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 15 11:18:43 2016

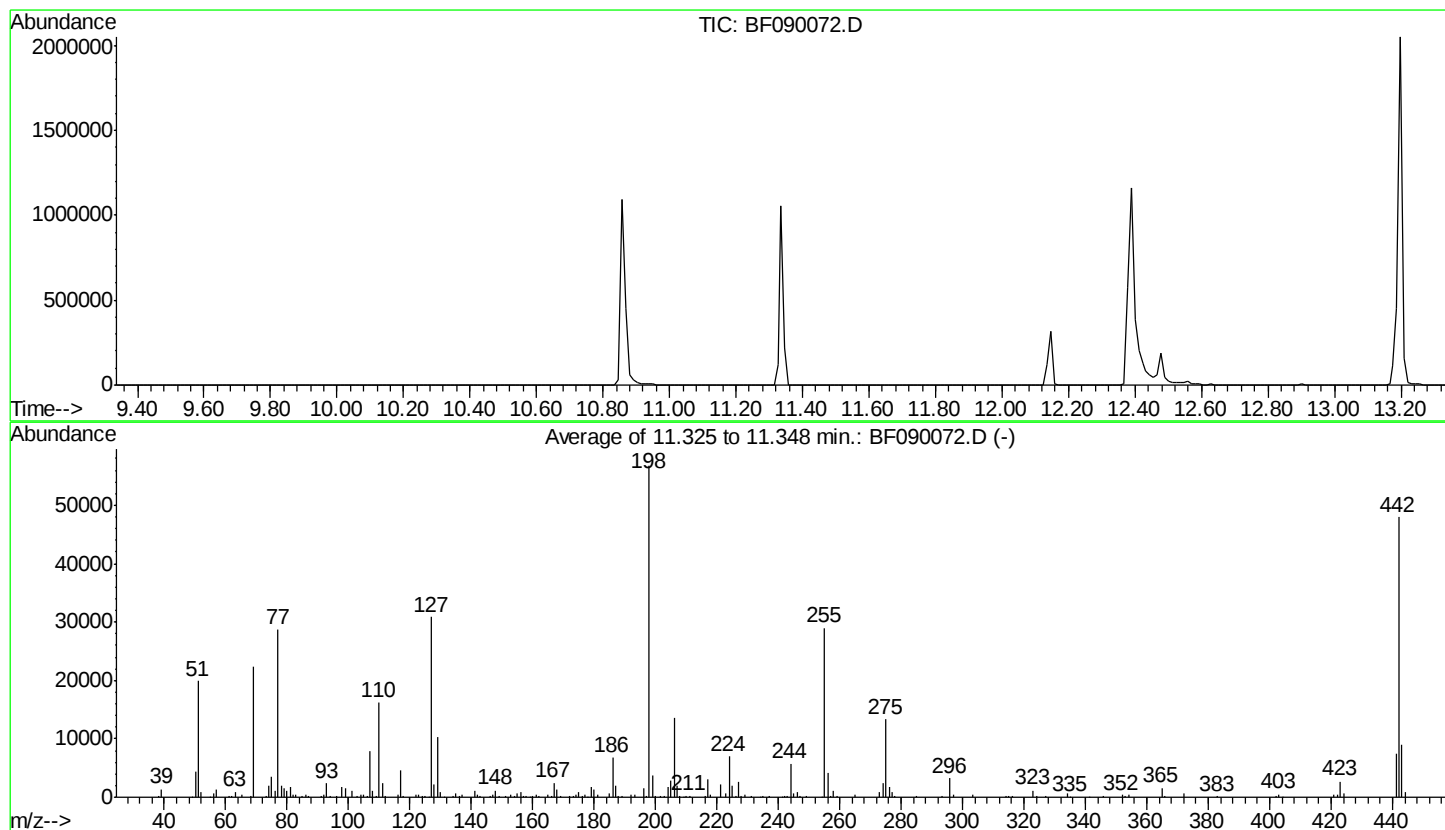

AutoFind: Scans 852, 853, 854; Background Corrected with Scan 849

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	19908	PASS
68	69	0.00	2	1.0	226	PASS
69	198	0.00	100	39.4	22365	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.3	30862	PASS
197	198	0.00	2	0.5	264	PASS
198	198	100	100	100.0	56794	PASS
199	198	5	9	6.7	3823	PASS
275	198	10	60	23.5	13343	PASS
365	198	1	100	2.8	1596	PASS
441	442	0.01	24	15.7	7554	PASS
442	198	50	100	84.5	47988	PASS
443	442	15	24	18.8	9004	PASS