
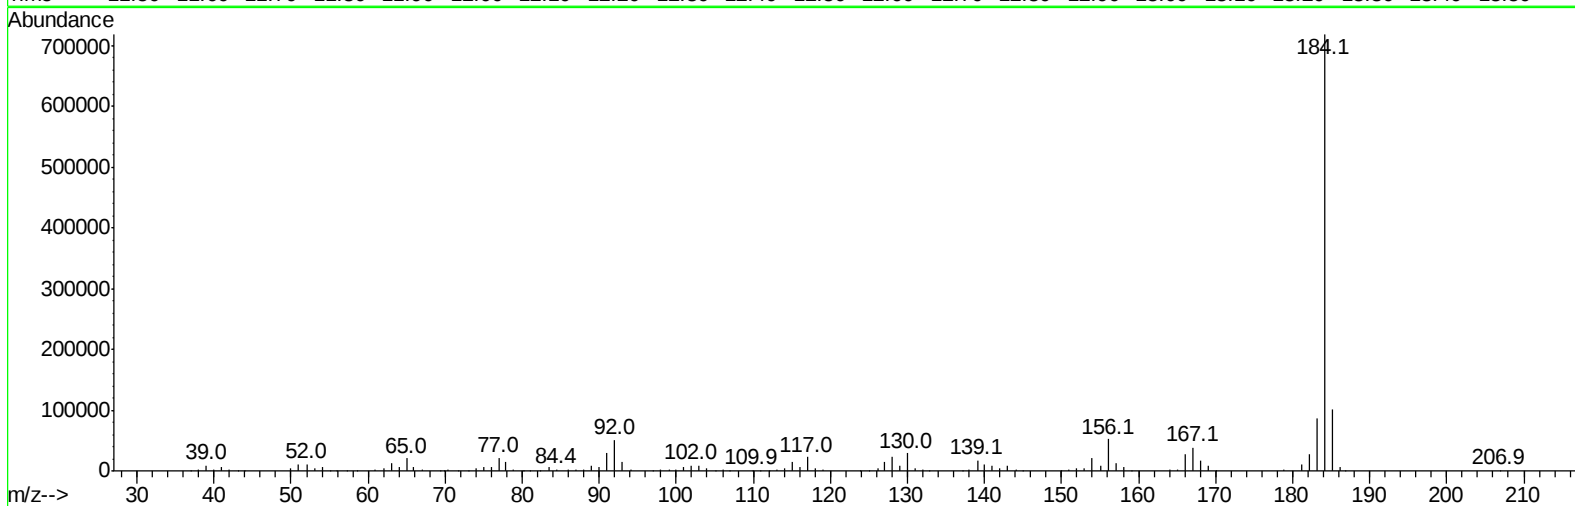


Data Path : Z:\HPCHEM1\BNA F\Data\BF091517\
Data File : BF098557.D
Acq On : 15 Sep 2017 9:01
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 07:09:08 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:14:50 2017
Response via : Initial Calibration

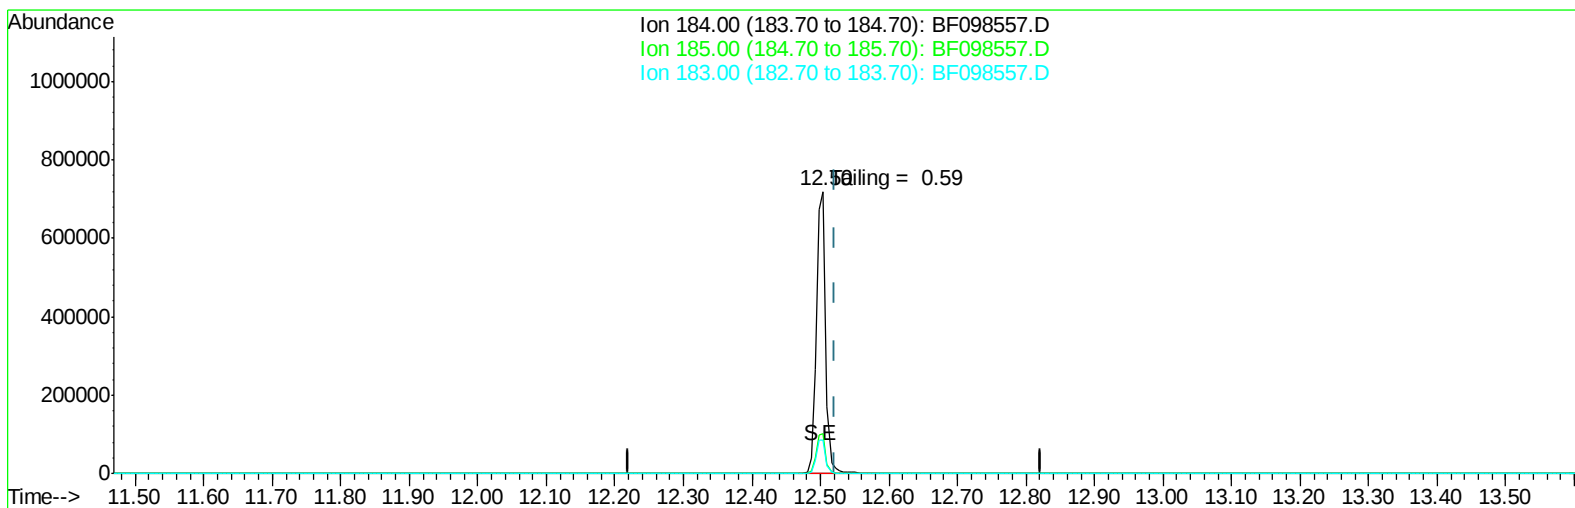

TIC: BF098557.D

(76) Benzidine



12.504min (-0.017) 0.00ng

response 681853

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.00#
183.00	12.20	11.97
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF091517\
Data File : BF098557.D
Acq On : 15 Sep 2017 9:01
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 07:09:08 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:14:50 2017
Response via : Initial Calibration

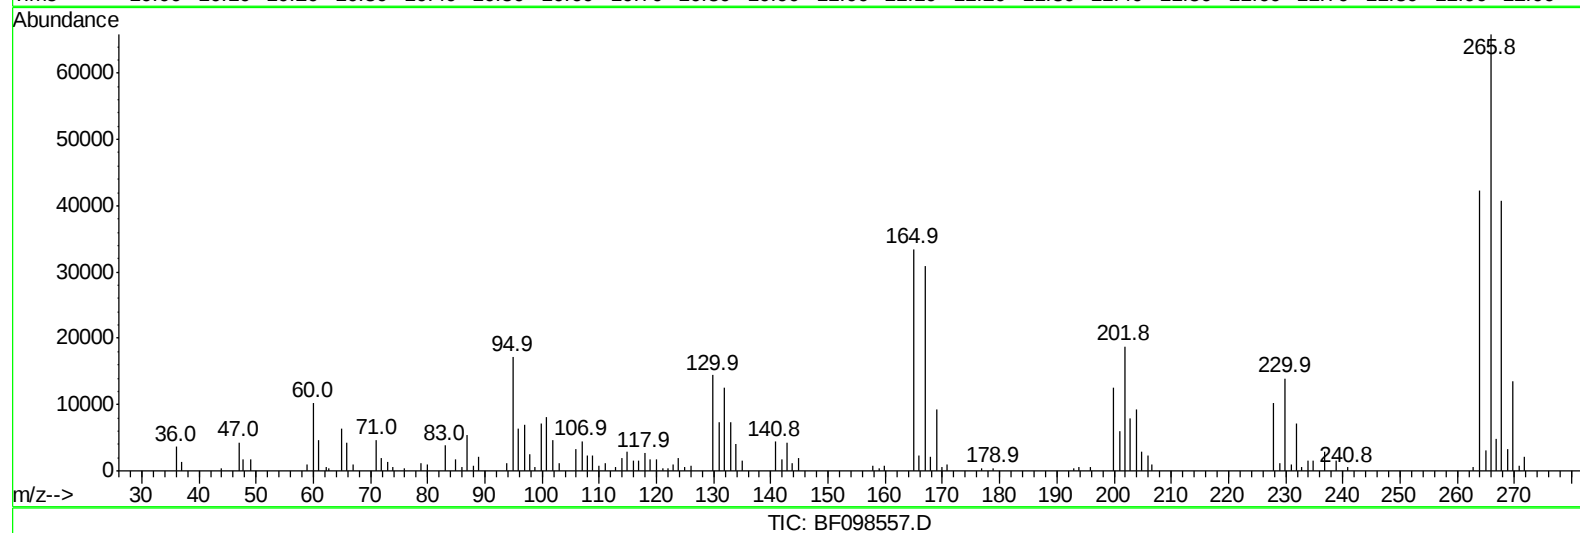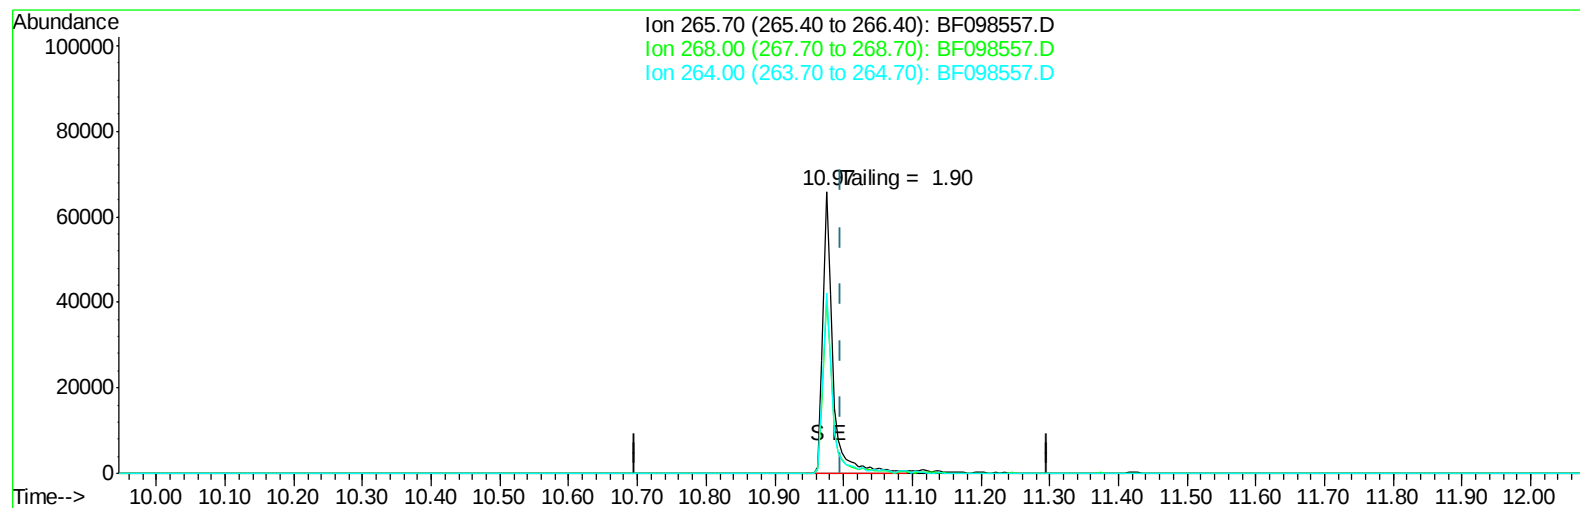

TIC: BF098557.D

(69) Pentachlorophenol (C)

10.975min (-0.022) 23501.68ng

response 64573

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.74
264.00	64.60	64.31
0.00	0.00	0.00