
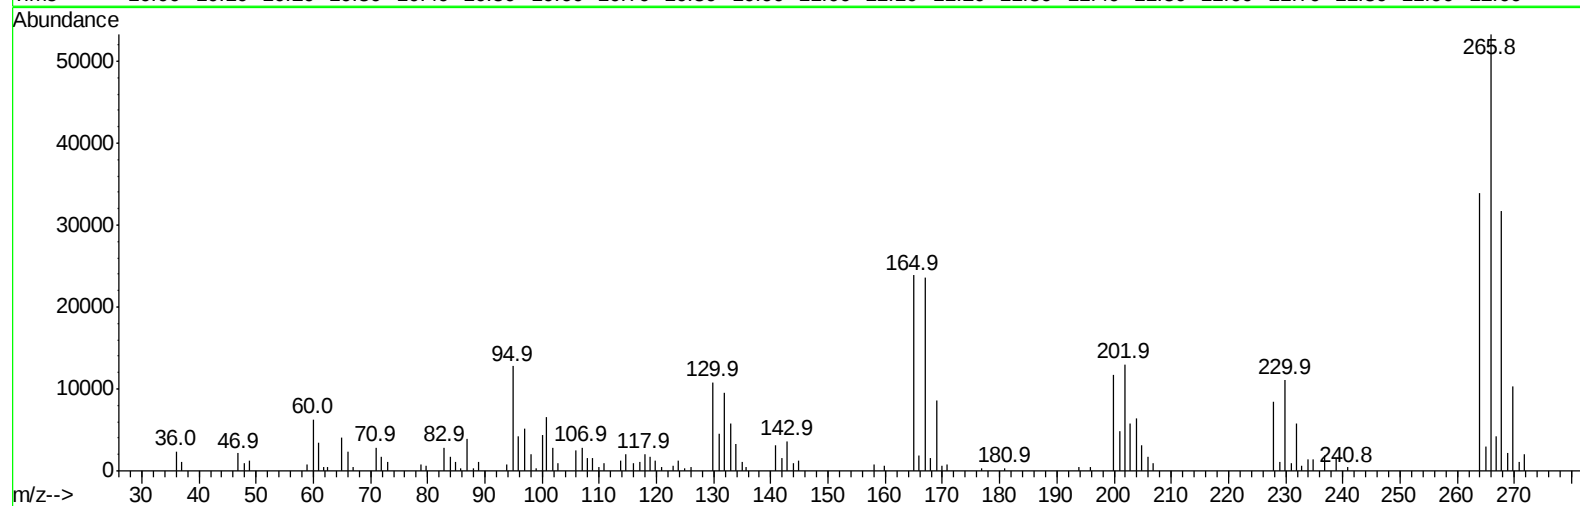


Data Path : Z:\HPCHEM1\BNA F\Data\BF091517\
Data File : BF098572.D
Acq On : 15 Sep 2017 16:38
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 07:10:17 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:14:50 2017
Response via : Initial Calibration

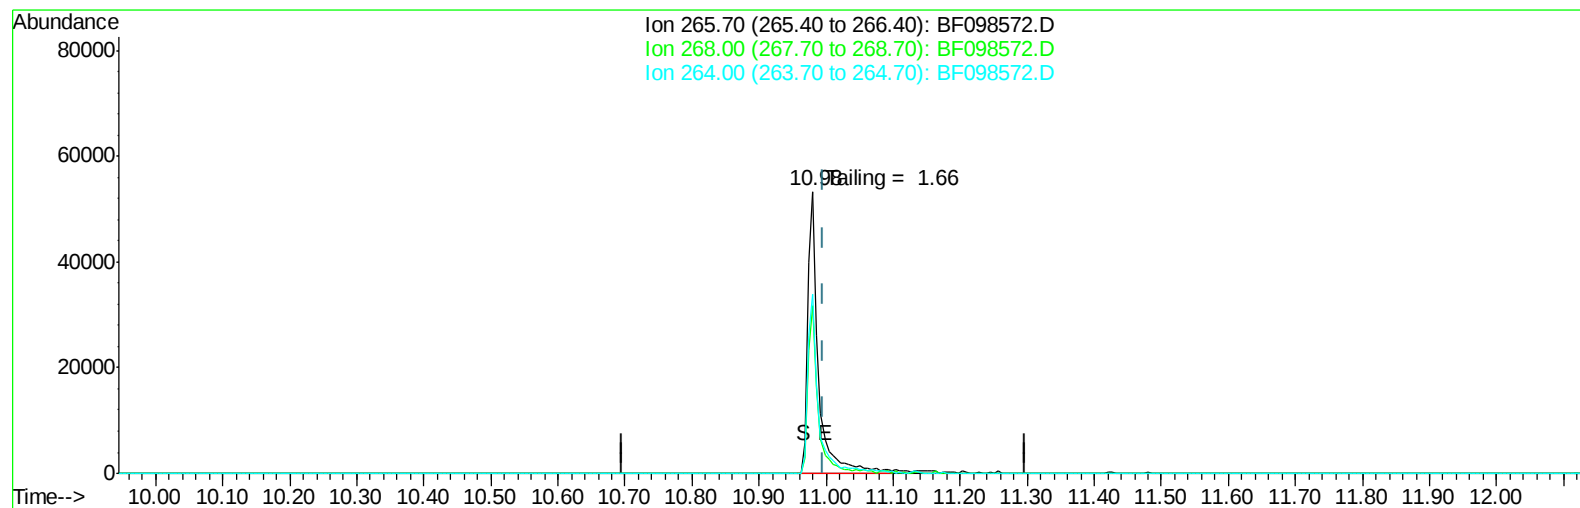

TIC: BF098572.D

(69) Pentachlorophenol (C)



10.980min (-0.017) 30785.28ng

response 60607

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.42
264.00	64.60	63.74
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA F\Data\BF091517\  
Data File : BF098572.D  
Acq On    : 15 Sep 2017  16:38  
Operator  : SJ/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Sep 16 07:10:17 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:14:50 2017
Response via : Initial Calibration

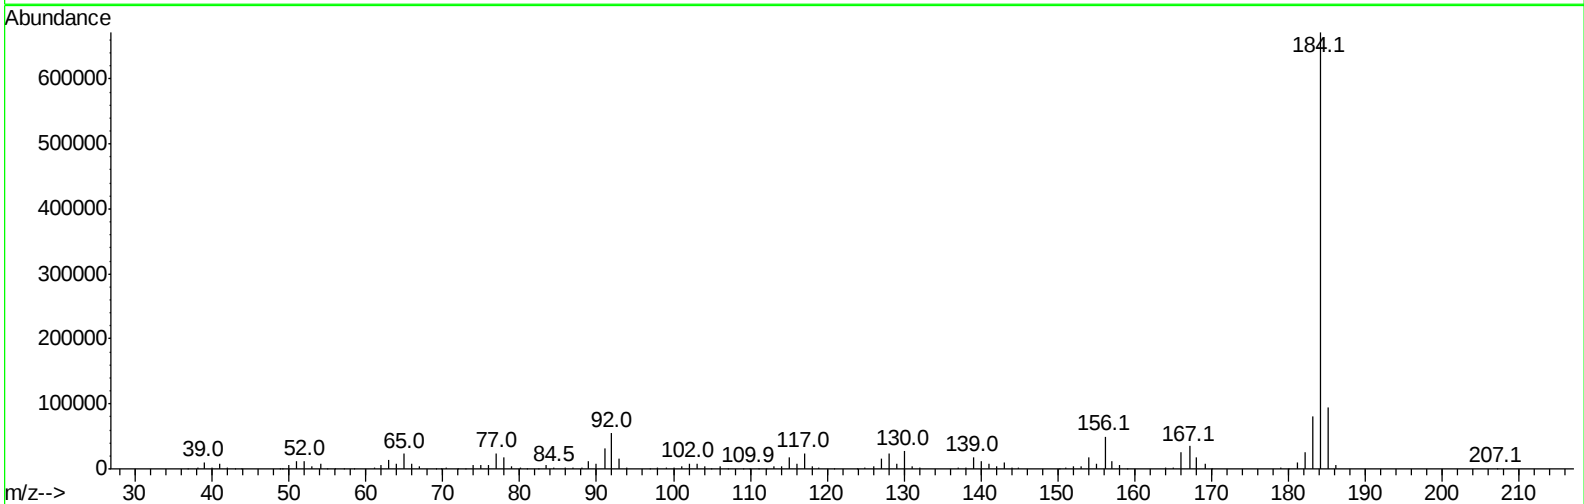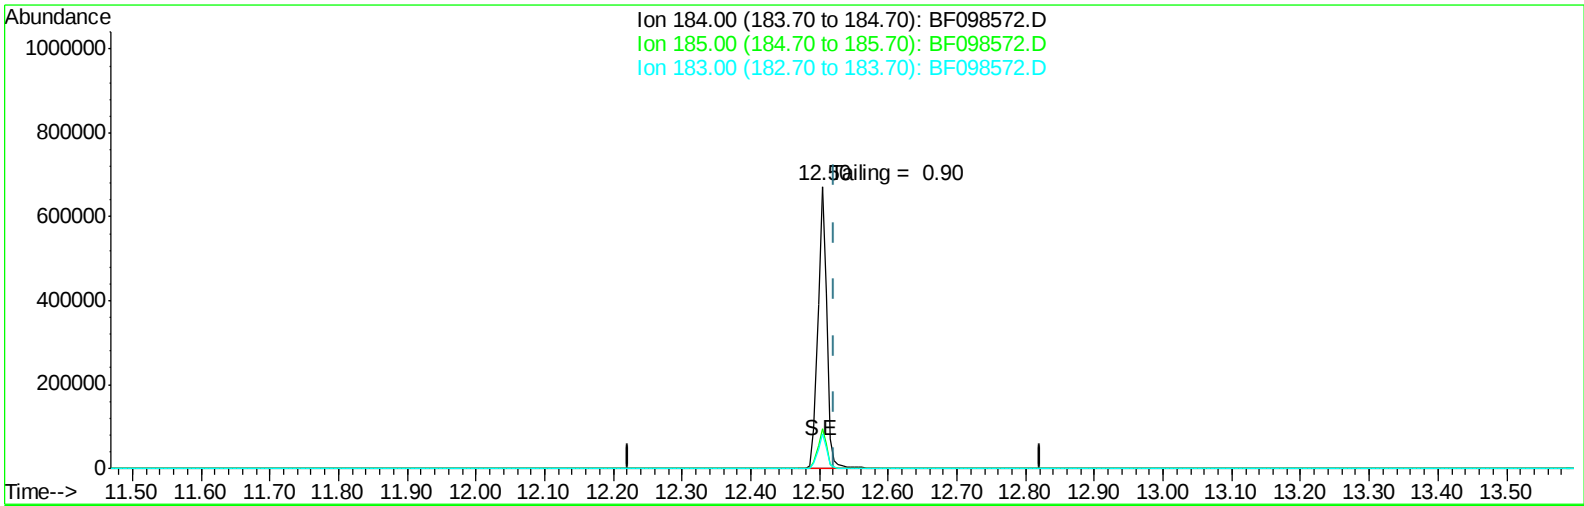

TIC: BF098572.D

(76) Benzidine

12.504min (-0.018) 0.00ng

response 603456

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.08#
183.00	12.20	12.07
0.00	0.00	0.00