

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091517\
 Data File : BF098584.D
 Acq On : 15 Sep 2017 22:26
 Operator : SJ/JU
 Sample : I5229-11 50X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 UT5400S21

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.263	538	540	548	rBV	34961	51618	4.54%	0.873%
2	6.310	715	718	734	rBV	39013	66047	5.81%	1.117%
3	6.422	734	737	746	rVV	63879	69606	6.13%	1.177%
4	6.639	771	774	784	rBV	850237	750156	66.01%	12.684%
5	6.798	797	801	811	rBV	52901	51102	4.50%	0.864%
6	7.216	869	872	886	rBB	27552	36902	3.25%	0.624%
7	7.928	989	993	1009	rBV	1126484	949197	83.53%	16.049%
8	9.004	1173	1176	1184	rBV	83727	68608	6.04%	1.160%
9	9.680	1286	1291	1299	rBV	1089930	983916	86.58%	16.636%
10	10.474	1423	1426	1433	rVB	31166	32427	2.85%	0.548%
11	11.163	1539	1543	1551	rBV	1337731	1136397	100.00%	19.215%
12	12.386	1748	1751	1755	rBV2	12803	15326	1.35%	0.259%
13	12.745	1808	1812	1816	rBV	81976	72360	6.37%	1.223%
14	13.286	1897	1904	1909	rBV9	10804	27990	2.46%	0.473%
15	13.798	1987	1991	1996	rBV	918632	806015	70.93%	13.628%
16	14.874	2170	2174	2177	rBV	32992	42099	3.70%	0.712%
17	15.198	2224	2229	2236	rBV	611129	754451	66.39%	12.757%


Sum of corrected areas: 5914217

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091517\
Data File : BF098584.D
Acq On : 15 Sep 2017 22:26
Operator : SJ/JU
Sample : I5229-11 50X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
UT5400S21

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

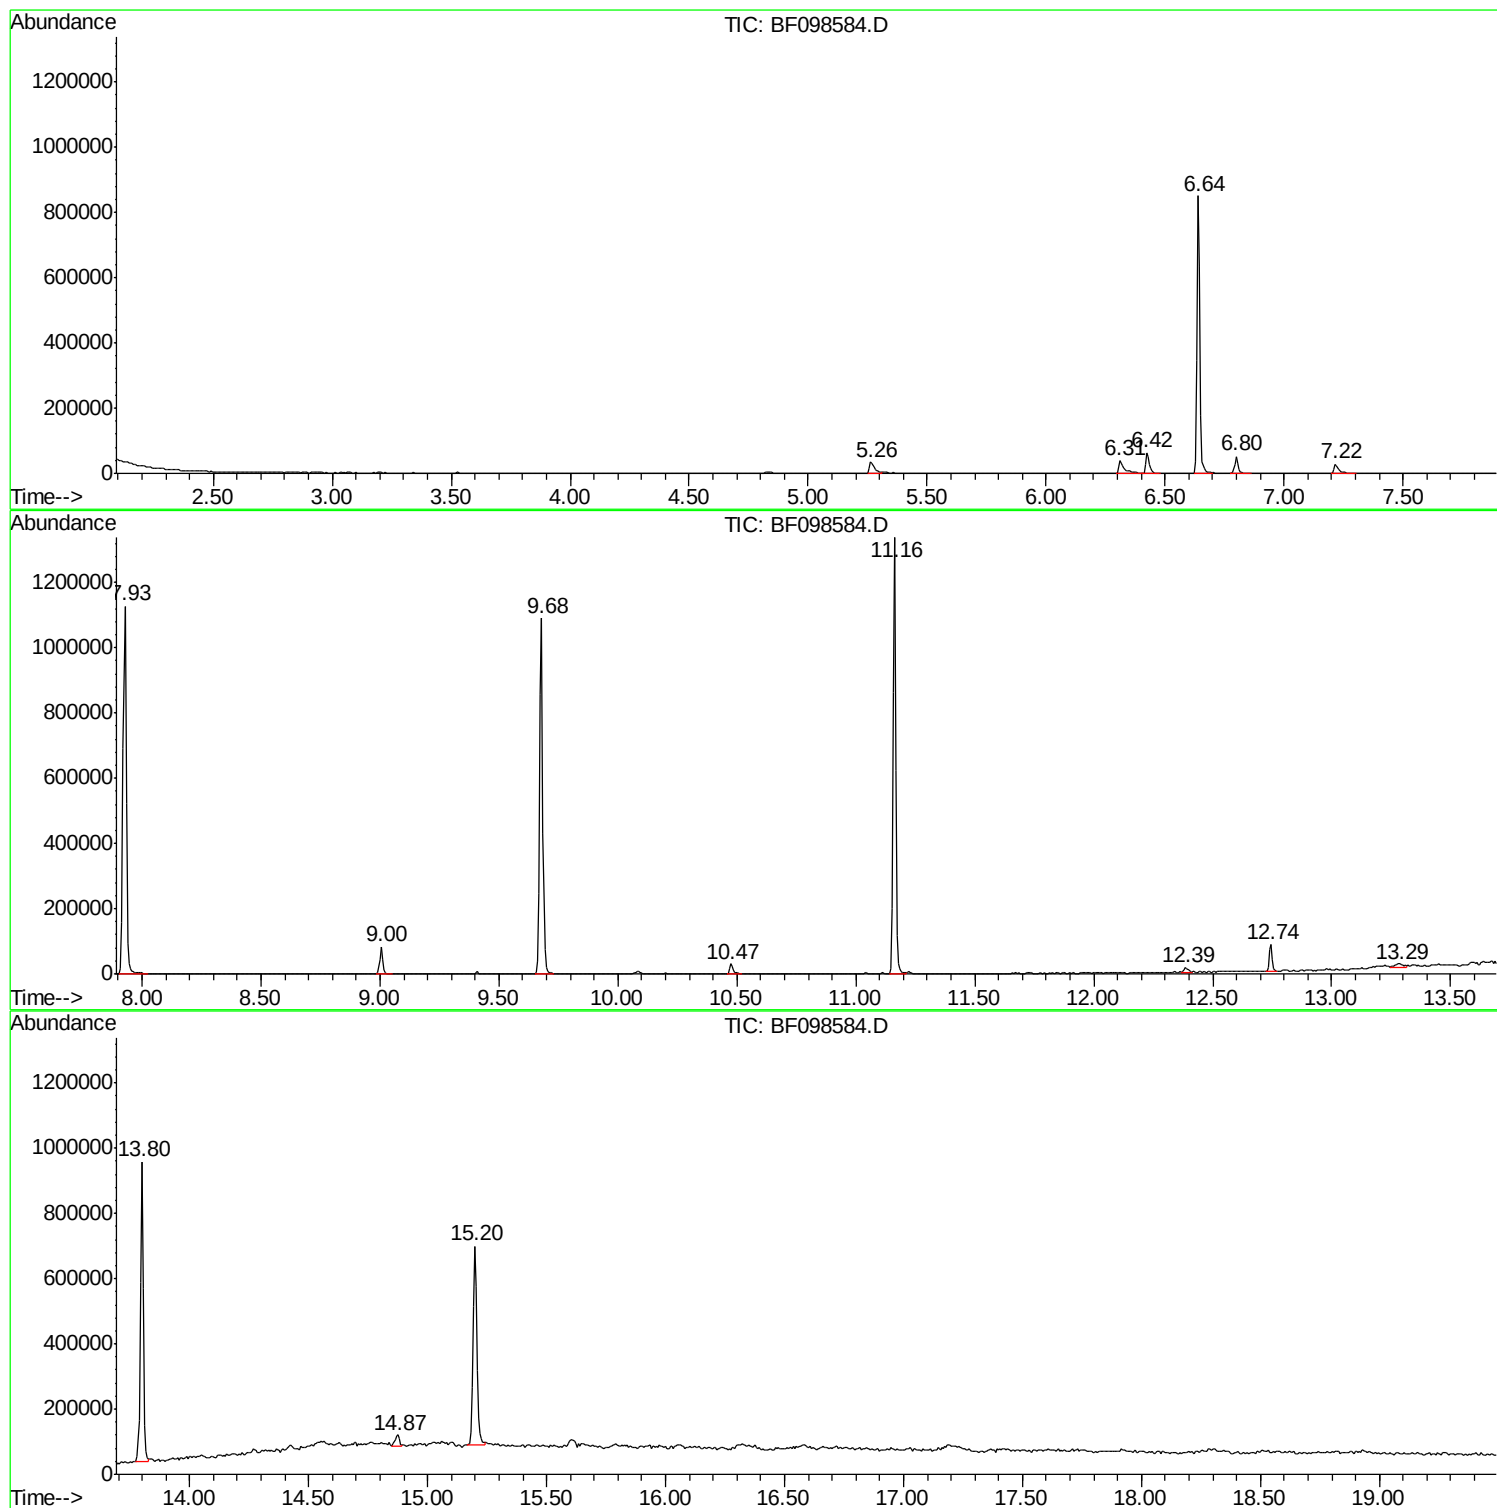

DbaaaPbath::ZZ\NRPBEMM\BBAFNDAA\BB00955IX\
 DbaaaFfile::BB009884DD
 Aeqq00n ::155S8pp20017 222206
 Opeaaor ::S3JUU
 Samplee ::I5229111500X
 Misc ::
 AASSVaal ::133 SampleeMMultiplier:11

Instrument :
 BNA_F
 ClientSampleId :
 UT5400S21

QqaabtMebbdd::ZZ\NRPBEMM\BBAFMEH00S82Z00BB0091117MM
 QqaabtTitee ::ASBPBNASSANDABBSF00R55P000NTC6AIBBATION

TICCLibbaay ::CC\DAABASSEN0\$SI11LL
 TICInteggaafionPaaameess:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
