


Data Path : Z:\HPCHEM1\BNA_F\Data\BF091517\
 Data File : BF098557.D
 Acq On : 15 Sep 2017 9:01
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 18 13:37:24 2017

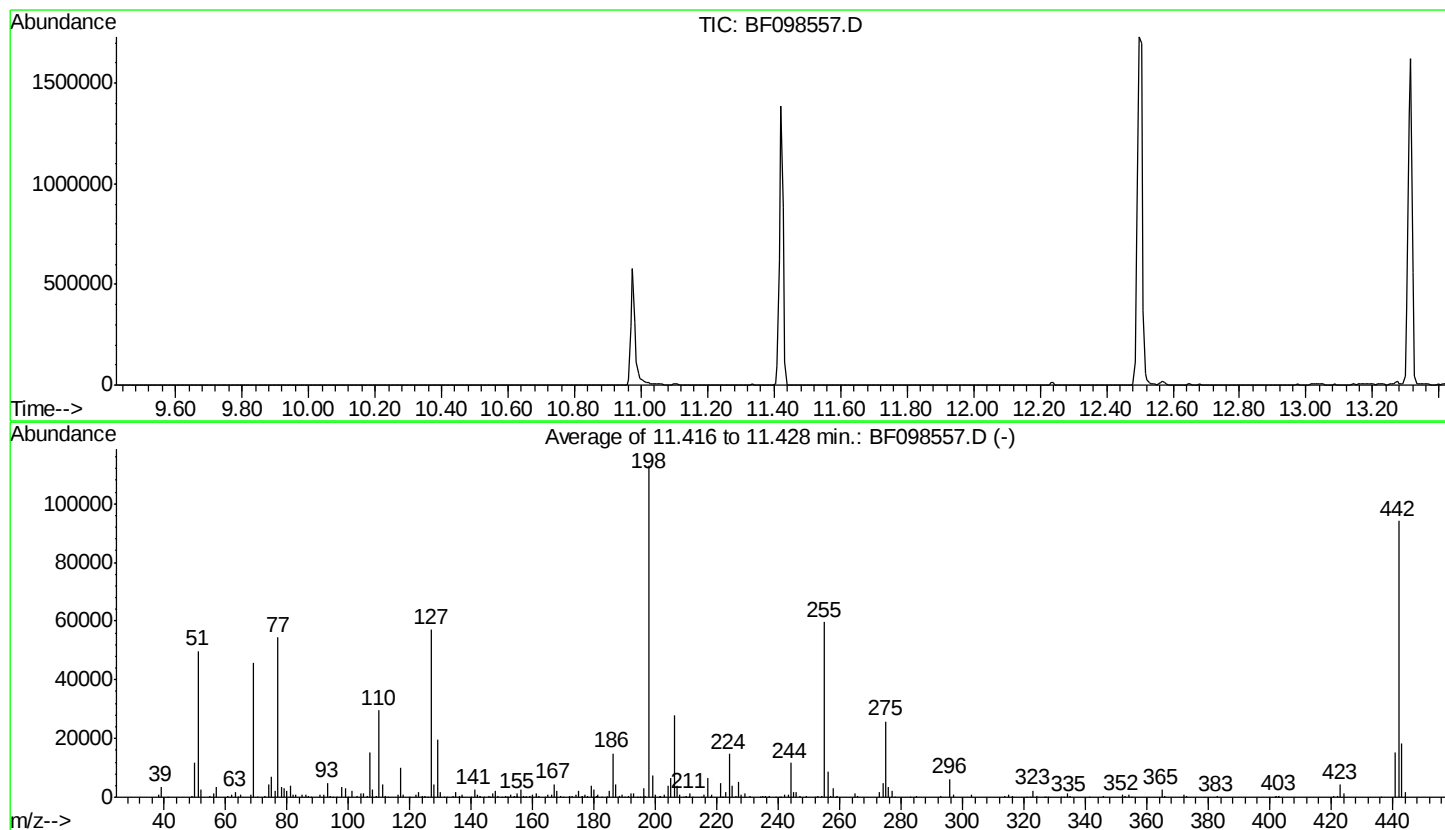

AutoFind: Scans 1586, 1587, 1588; Background Corrected with Scan 1581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.1	49765	PASS
68	69	0.00	2	1.8	820	PASS
69	198	0.00	100	40.5	45720	PASS
70	69	0.00	2	0.3	117	PASS
127	198	10	80	50.6	57117	PASS
197	198	0.00	2	0.5	568	PASS
198	198	100	100	100.0	112949	PASS
199	198	5	9	6.6	7431	PASS
275	198	10	60	22.8	25773	PASS
365	198	1	100	2.2	2531	PASS
441	442	0.01	24	16.1	15127	PASS
442	198	50	100	83.2	94005	PASS
443	442	15	24	19.7	18488	PASS