


Data Path : Z:\HPCHEM1\BNA_F\Data\BF091517\
 Data File : BF098572.D
 Acq On : 15 Sep 2017 16:38
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 18 13:37:24 2017

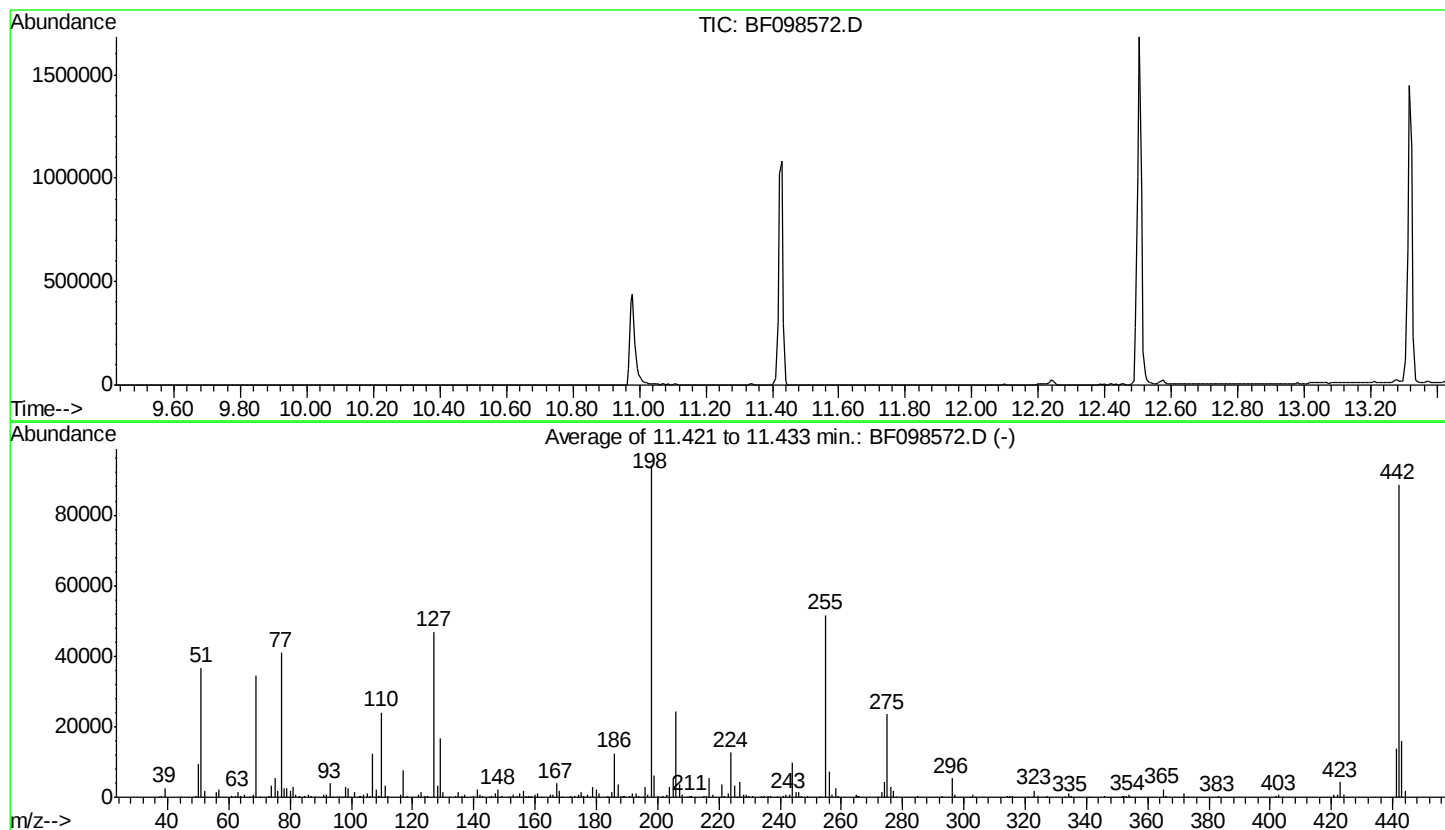

AutoFind: Scans 1587, 1588, 1589; Background Corrected with Scan 1581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	36825	PASS
68	69	0.00	2	1.6	569	PASS
69	198	0.00	100	36.7	34508	PASS
70	69	0.00	2	0.4	123	PASS
127	198	10	80	49.8	46835	PASS
197	198	0.00	2	0.7	611	PASS
198	198	100	100	100.0	93986	PASS
199	198	5	9	6.4	6039	PASS
275	198	10	60	25.1	23576	PASS
365	198	1	100	2.5	2362	PASS
441	442	0.01	24	15.5	13762	PASS
442	198	50	100	94.3	88600	PASS
443	442	15	24	18.1	16037	PASS