
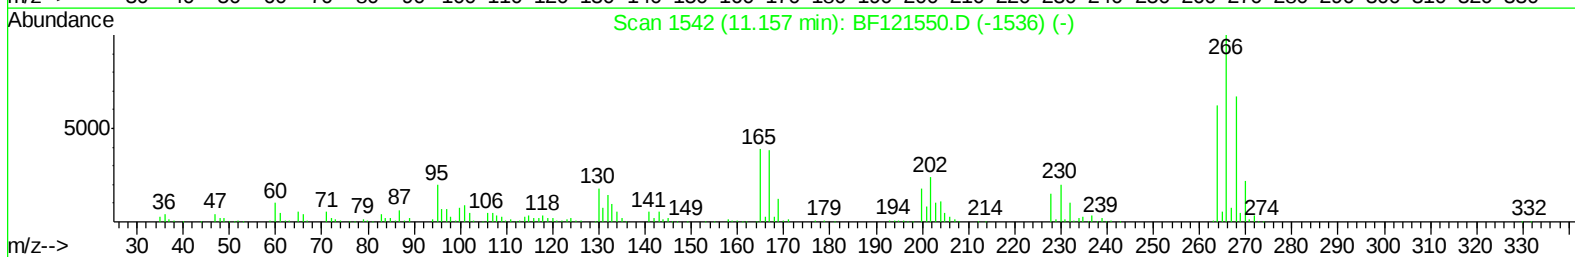
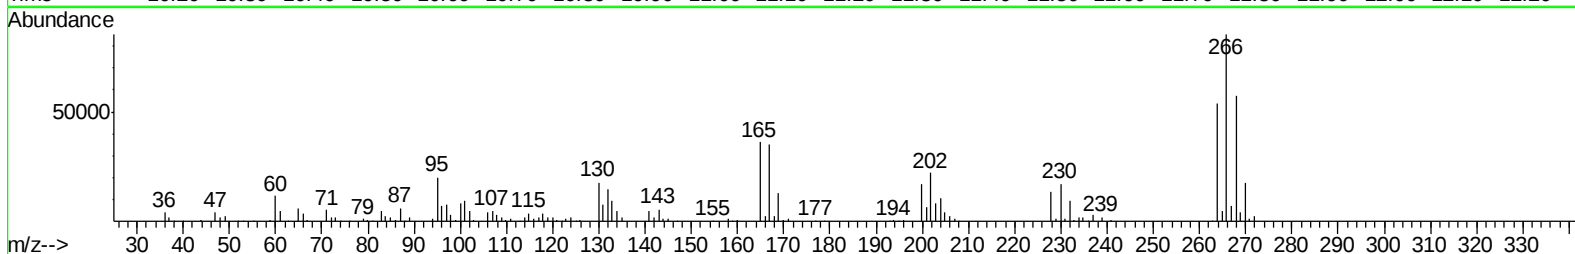


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF091520\
Data File : BF121568.D
Acq On : 15 Sep 2020 9:43
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 04:29:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 10 16:47:54 2020
Response via : Initial Calibration

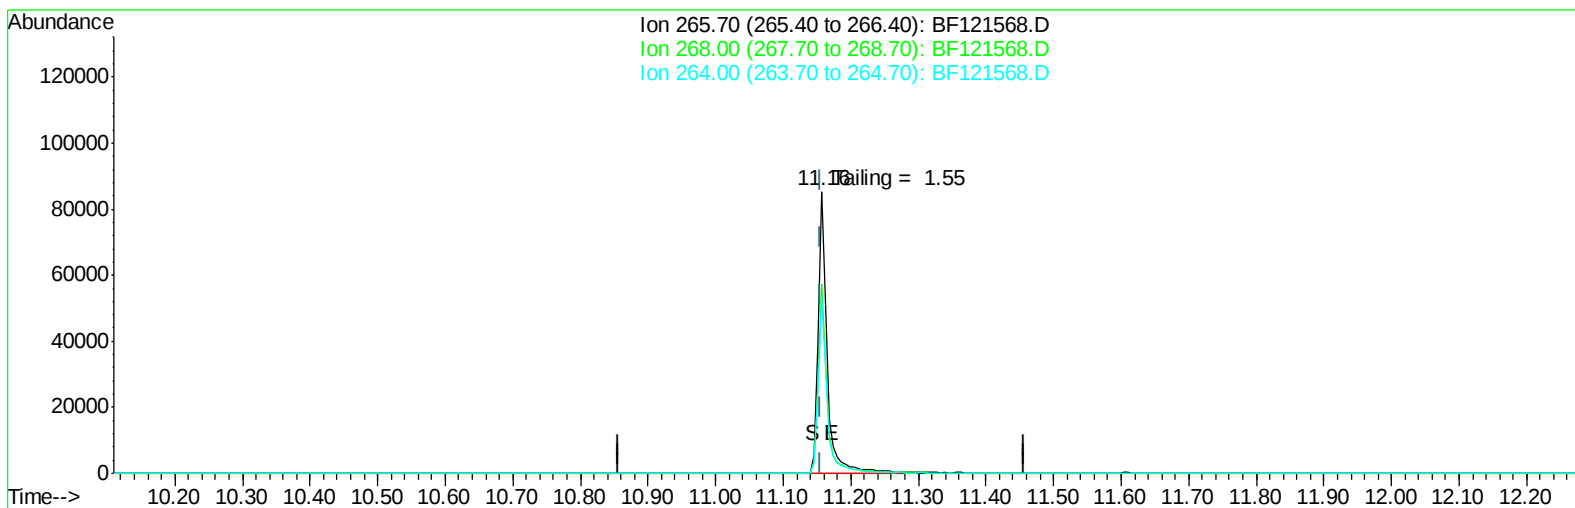

TIC: BF121568.D

(70) Pentachlorophenol (C)




11.157min (-0.000) 24898.23ng

response 81521

Ion	Exp%	Act%
265.70	100	100
268.00	66.90	67.16
264.00	62.30	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF091520\
Data File : BF121568.D
Acq On : 15 Sep 2020 9:43
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 04:29:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 10 16:47:54 2020
Response via : Initial Calibration

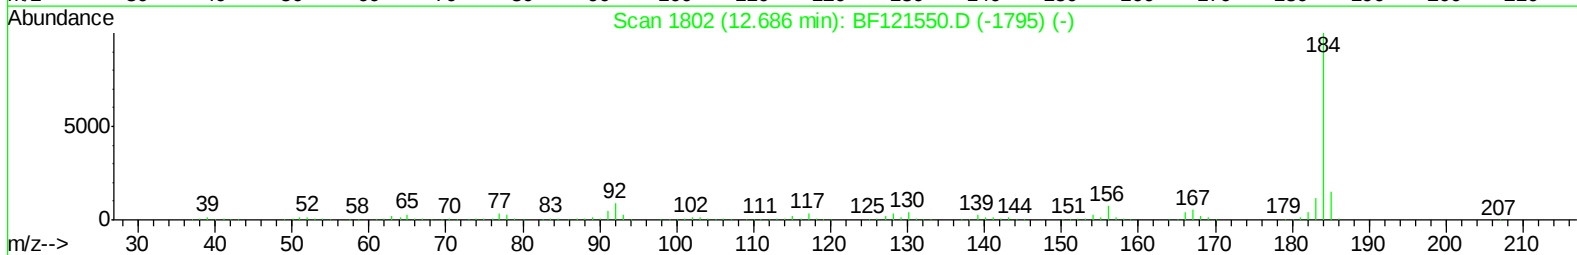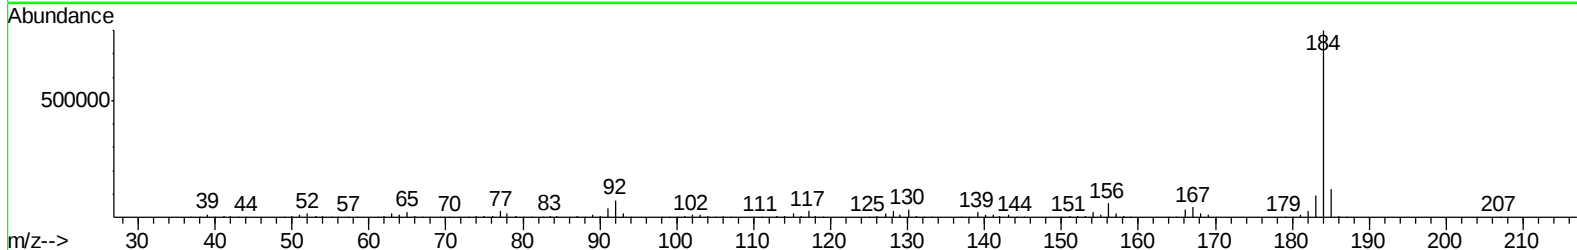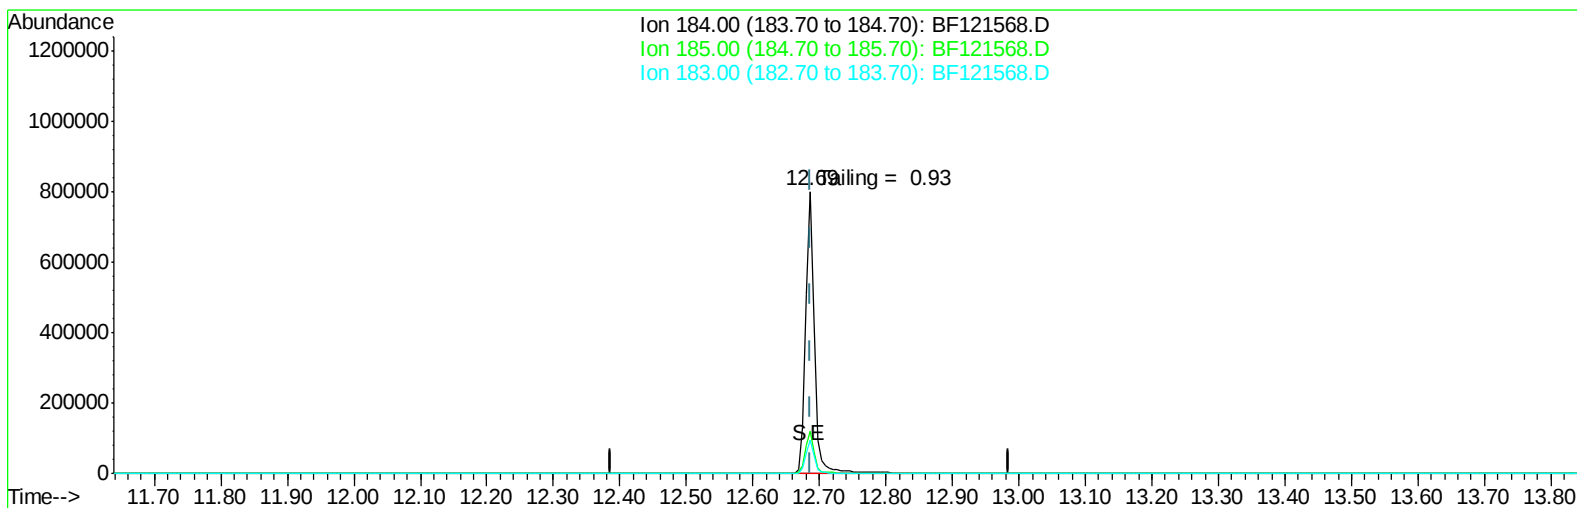

TIC: BF121568.D

(77) Benzidine

12.686min (-0.000) 0.00ng

response 753496

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.99
183.00	11.90	11.86
0.00	0.00	0.00