

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091520\
 Data File : BF121570.D
 Acq On : 15 Sep 2020 10:45
 Operator : JU/CG
 Sample : PB131580BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB131580BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.199	15	19	23	rVB	75921	105412	1.52%	0.251%
2	5.081	505	509	519	rVB	96470	139075	2.01%	0.331%
3	5.469	570	575	578	rBV	4873292	5044994	72.75%	12.025%
4	6.469	740	745	748	rBV	4334912	5046424	72.78%	12.029%
5	6.828	803	806	810	rBV	1426803	1278283	18.43%	3.047%
6	7.392	896	902	905	rBV	3267377	3696621	53.31%	8.811%
7	8.110	1019	1024	1028	rBV	1648758	1701090	24.53%	4.055%
8	9.192	1201	1208	1211	rBV	5277426	6129908	88.40%	14.611%
9	9.863	1316	1322	1326	rBV	1760417	1818289	26.22%	4.334%
10	10.657	1450	1457	1460	rBV	3993088	3819748	55.09%	9.105%
11	11.351	1569	1575	1578	rBV	2238220	2066312	29.80%	4.925%
12	12.939	1837	1845	1848	rBV	6501044	6934228	100.00%	16.528%
13	13.986	2018	2023	2026	rBV	2377219	2169487	31.29%	5.171%
14	15.439	2264	2270	2283	rBV	1505230	2003634	28.89%	4.776%


Sum of corrected areas: 41953505

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091520\
Data File : BF121570.D
Acq On : 15 Sep 2020 10:45
Operator : JU/CG
Sample : PB131580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB131580BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

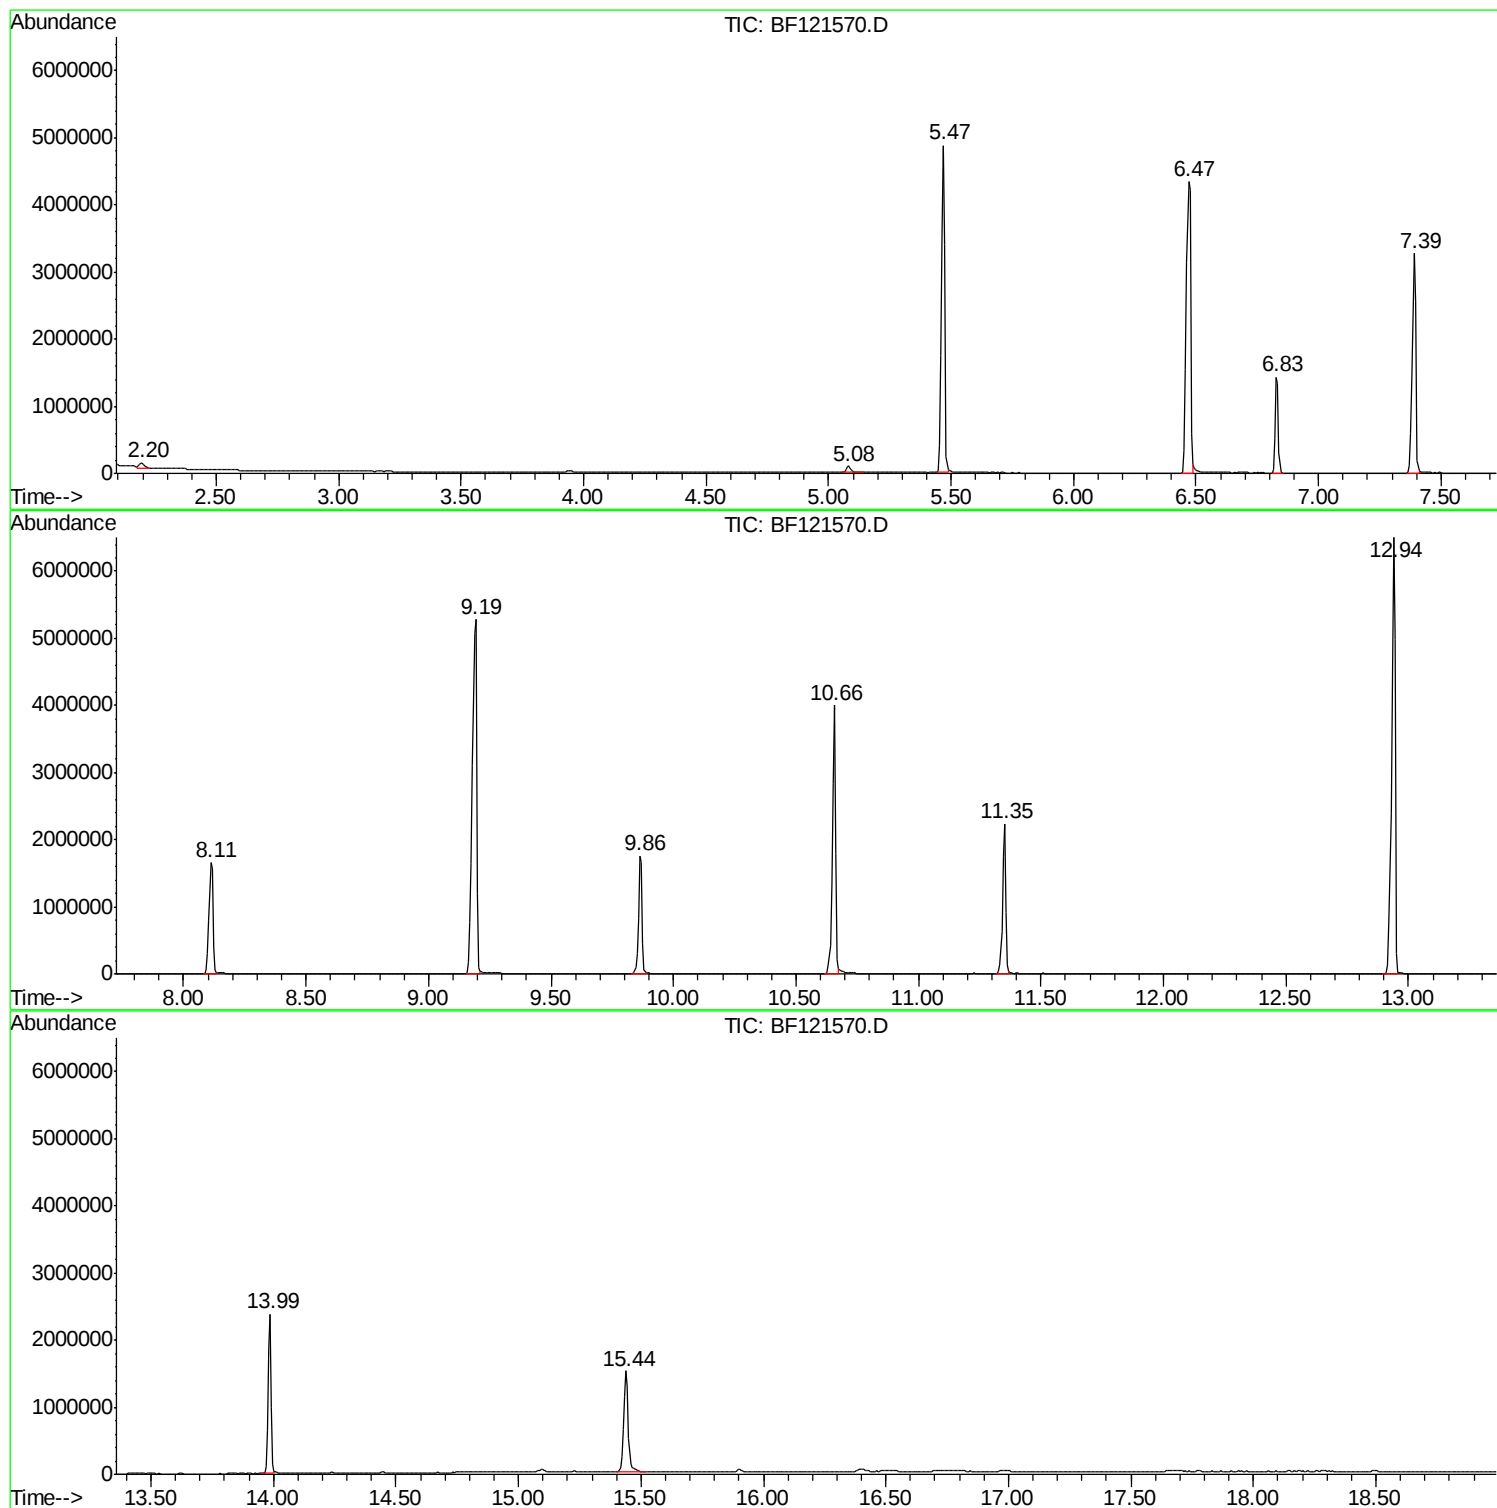

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091520\
Data File : BF121570.D
Acq On : 15 Sep 2020 10:45
Operator : JU/CG
Sample : PB131580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB131580BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.08	2.18 ng	139075	1,4-Dichlorobenzene-d4	6.83

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	27
3			Butane	58	C4H10	000106-97-8	9
4			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	9
5			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	9

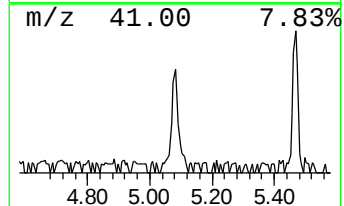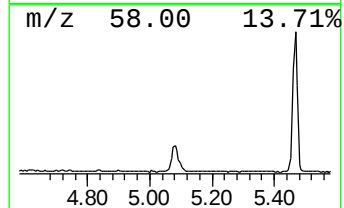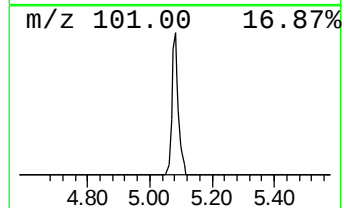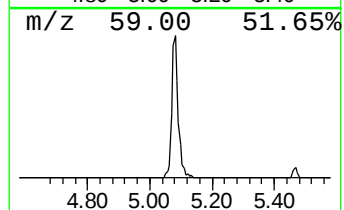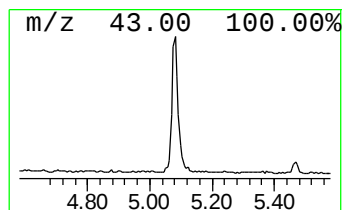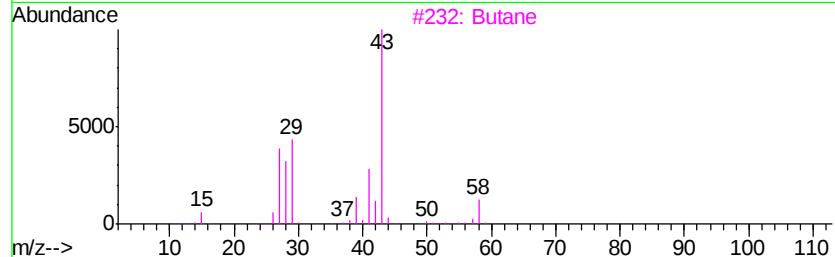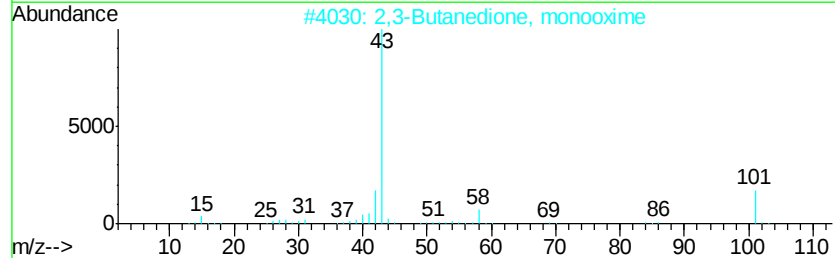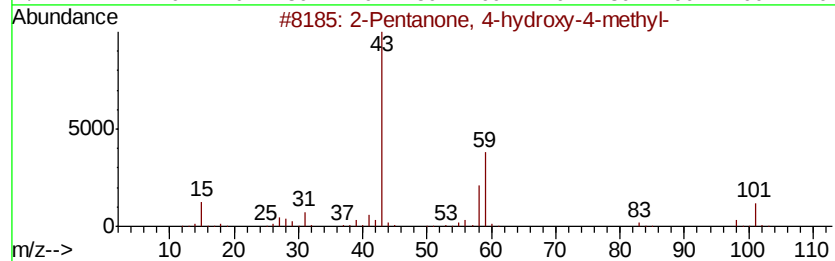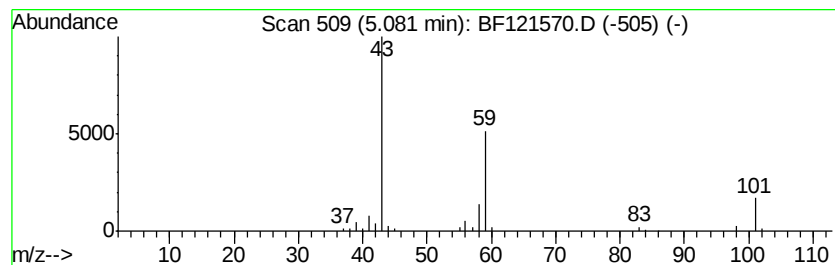

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091520\
Data File : BF121570.D
Acq On : 15 Sep 2020 10:45
Operator : JU/CG
Sample : PB131580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB131580BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.08	2.2	ng	139075	1	6.83	1278280	20.0