


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091520\
 Data File : BF121568.D
 Acq On : 15 Sep 2020 9:43
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 10 16:47:54 2020

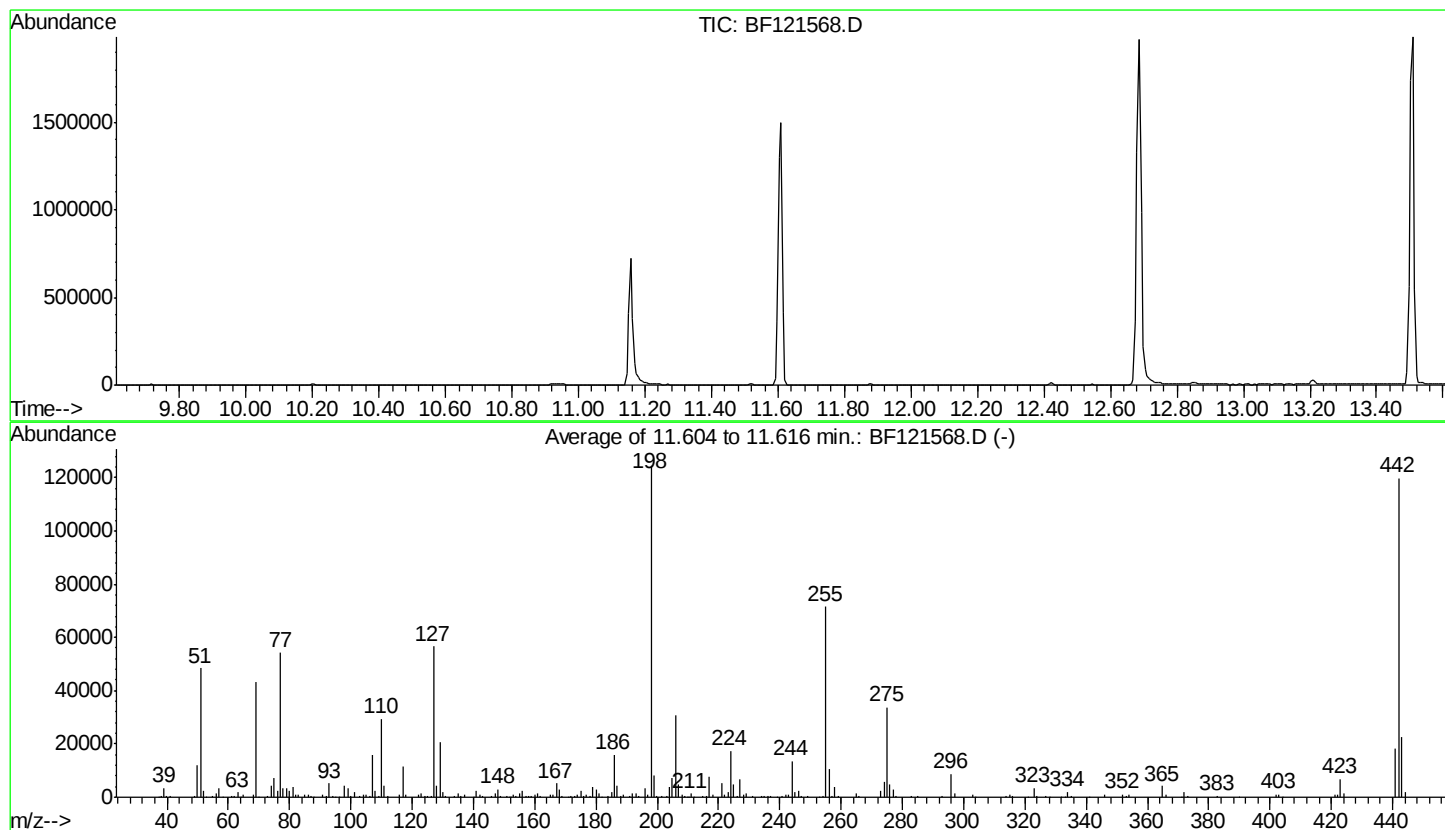

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	48418	PASS
68	69	0.00	2	1.8	781	PASS
69	198	0.00	100	34.6	43078	PASS
70	69	0.00	2	0.6	245	PASS
127	198	10	80	45.5	56632	PASS
197	198	0.00	2	0.7	859	PASS
198	198	100	100	100.0	124469	PASS
199	198	5	9	6.6	8245	PASS
275	198	10	60	27.2	33802	PASS
365	198	1	100	3.4	4288	PASS
441	198	0.01	100	14.8	18451	PASS
442	198	50	100	96.3	119885	PASS
443	442	15	24	18.7	22365	PASS