
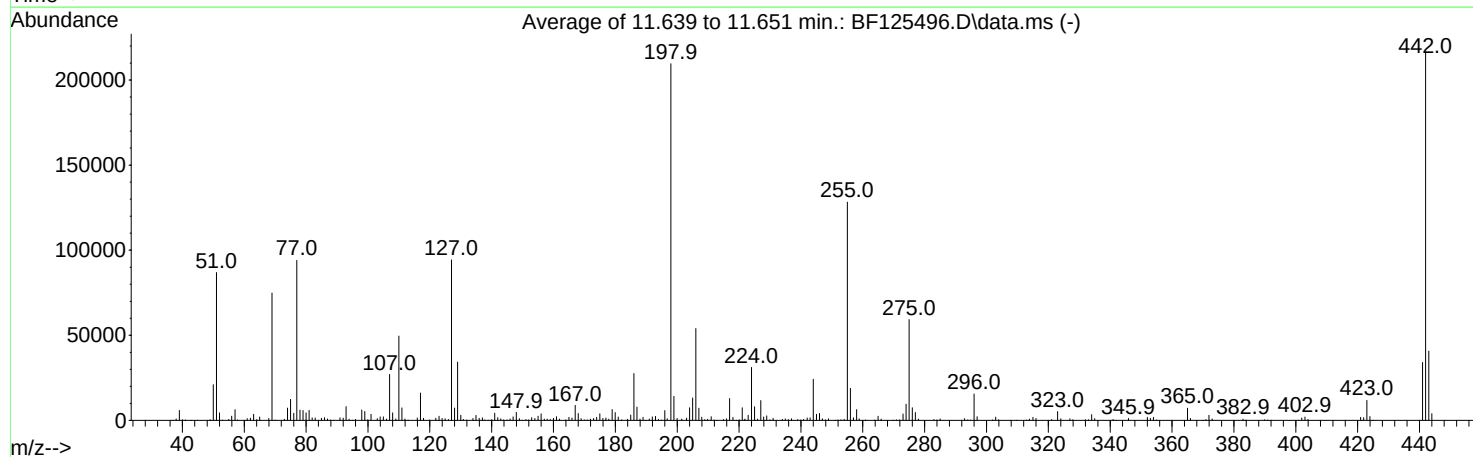


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091521\
 Data File : BF125496.D
 Acq On : 15 Sep 2021 10:06
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 15 15:08:32 2021

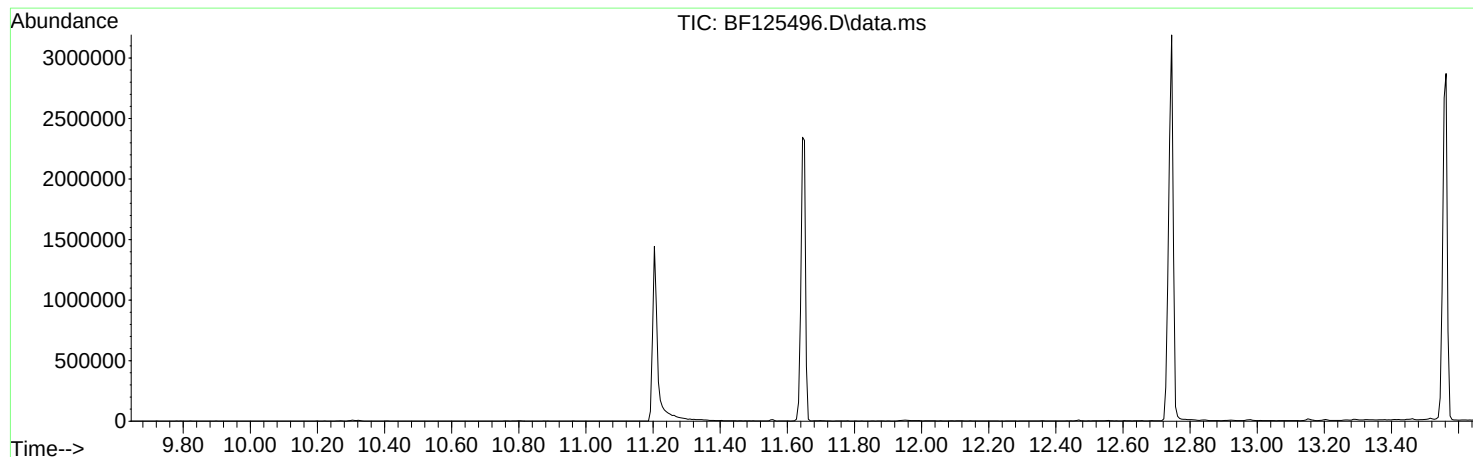

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	86864	PASS
68	69	0.00	2	1.5	1127	PASS
69	198	0.00	100	35.7	74845	PASS
70	69	0.00	2	0.2	183	PASS
127	198	10	80	45.0	94272	PASS
197	198	0.00	2	0.5	960	PASS
198	198	100	100	100.0	209536	PASS
199	198	5	9	6.7	14077	PASS
275	198	10	60	28.3	59224	PASS
365	198	1	100	3.4	7178	PASS
441	198	0.01	100	16.3	34070	PASS
442	442	50	100	100.0	216165	PASS
443	442	15	24	18.9	40763	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/15/2021	BNA_F	<u>BF125496.D</u>
Compound Name	Response	Retention Time
DDT	551405	13.56
DDD	1445	13.26
DDE	1281	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2726	554131	0.49

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091521\
 Data File : BF125496.D
 Acq On : 15 Sep 2021 10:06
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 15 10:56:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 15 10:52:20 2021
 Response via : Initial Calibration

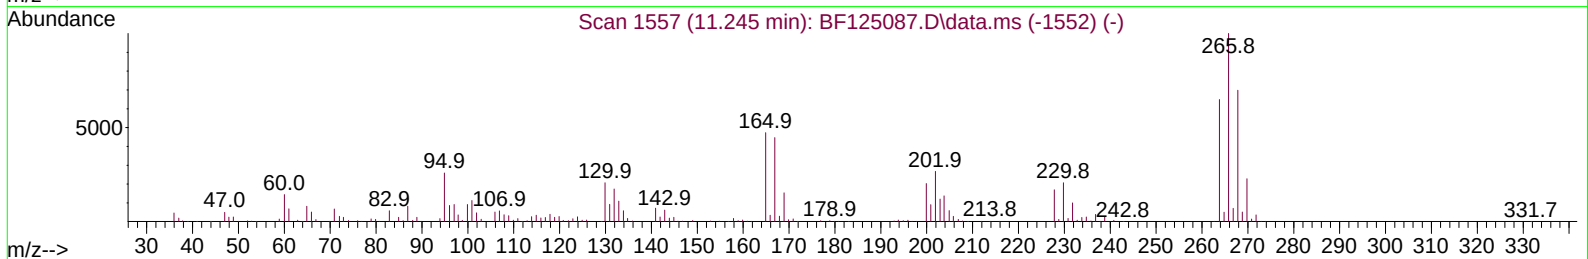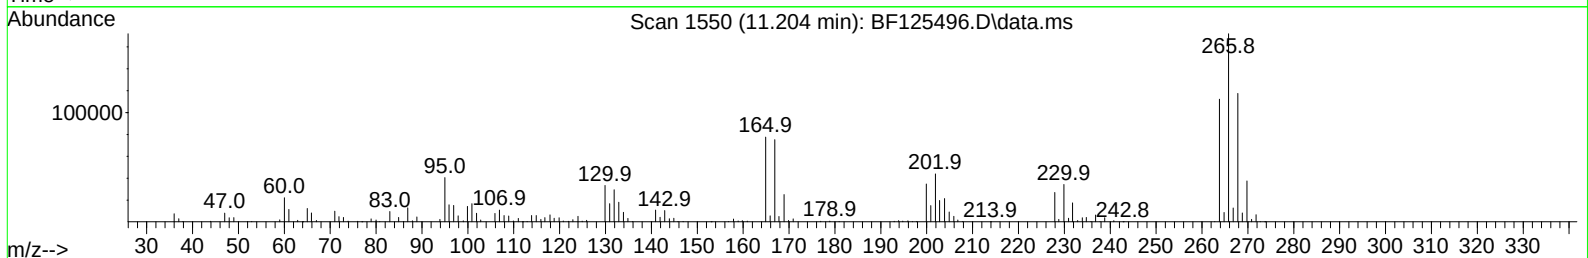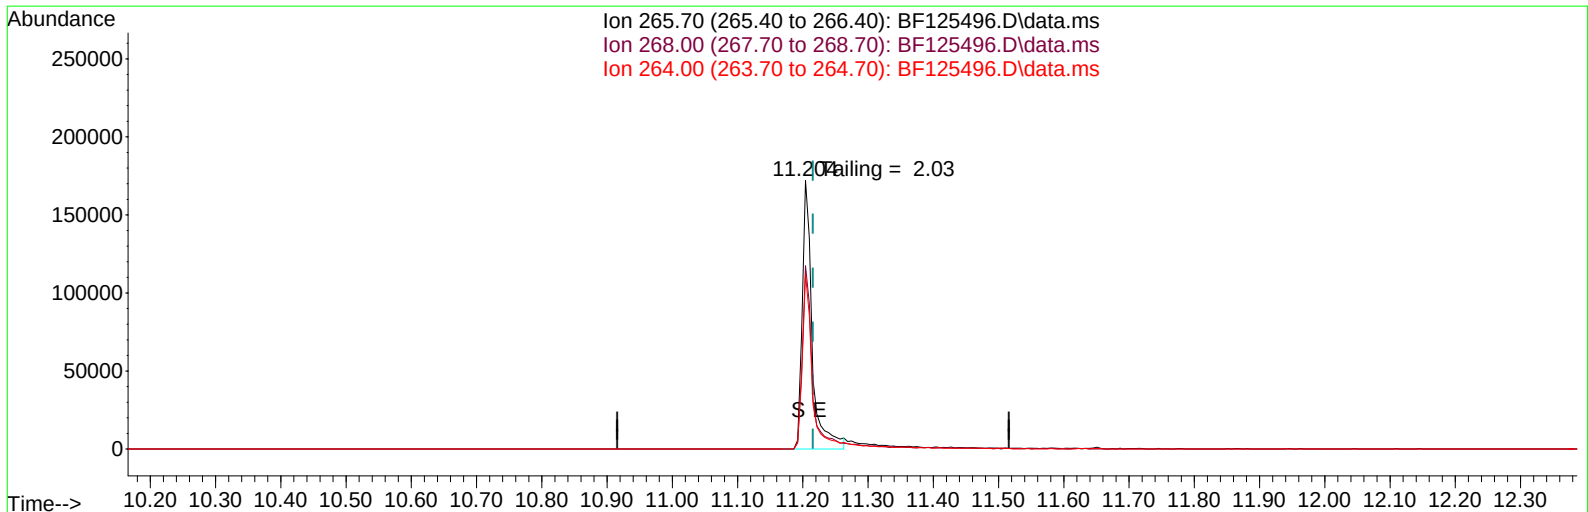

TIC: BF125496.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.012) 33025.92 ng




response 201532

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	68.28
264.00	69.90	65.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091521\
 Data File : BF125496.D
 Acq On : 15 Sep 2021 10:06
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 15 10:56:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 15 10:52:20 2021
 Response via : Initial Calibration

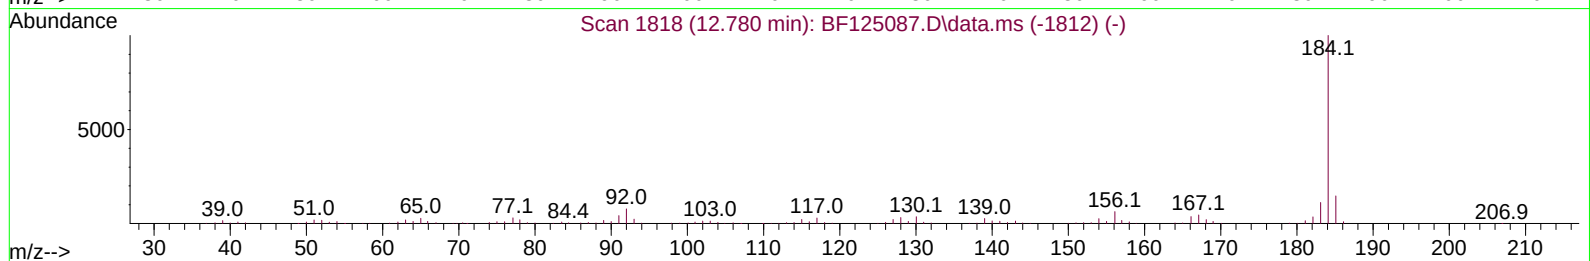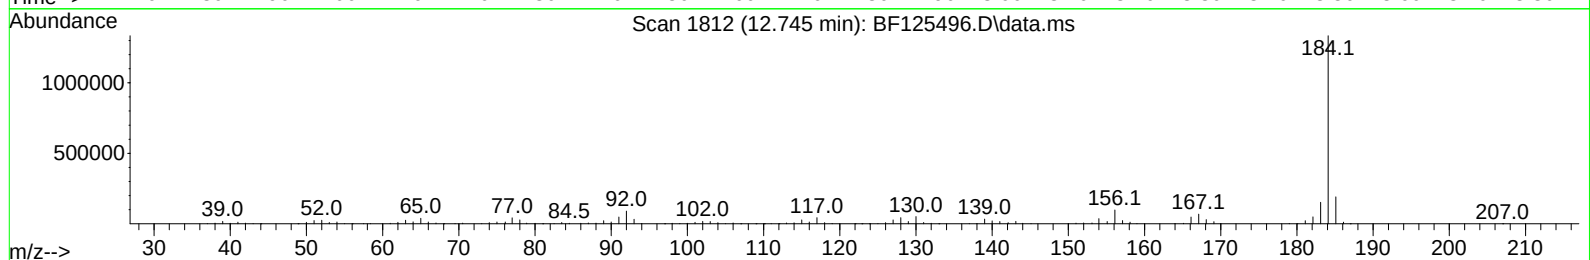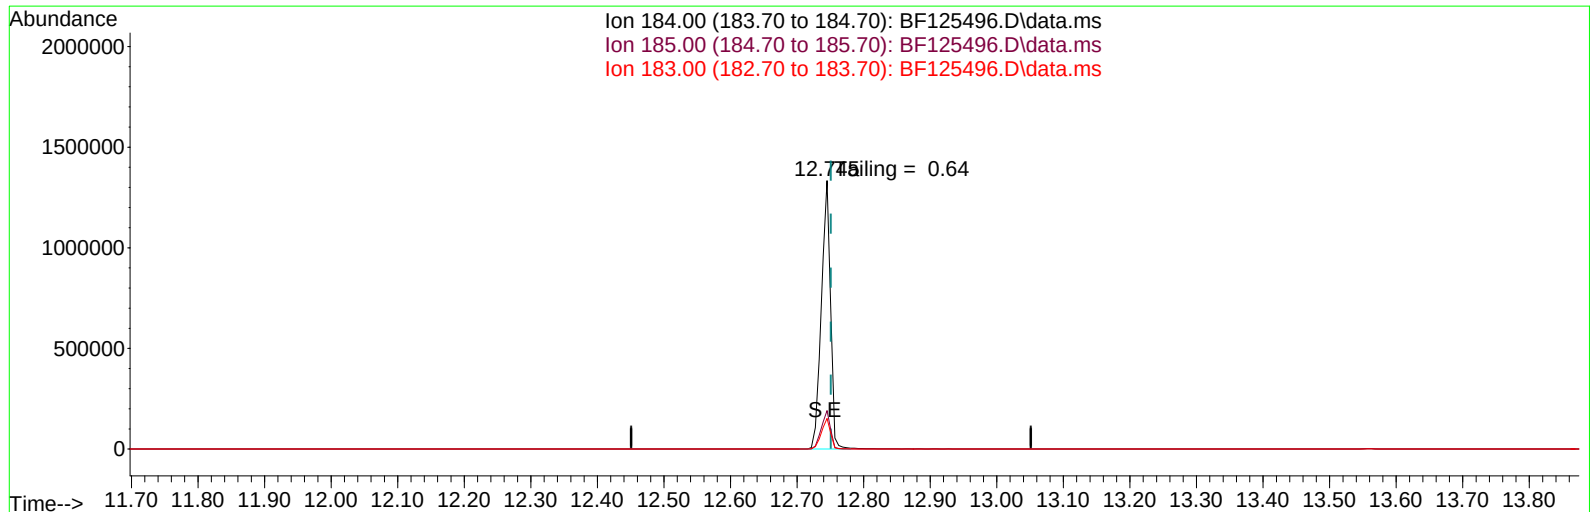

TIC: BF125496.D\data.ms

(77) Benzidine

12.745min (-0.006) 0.00 ng

response 1277876

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.34
183.00	10.10	11.41
0.00	0.00	0.00