
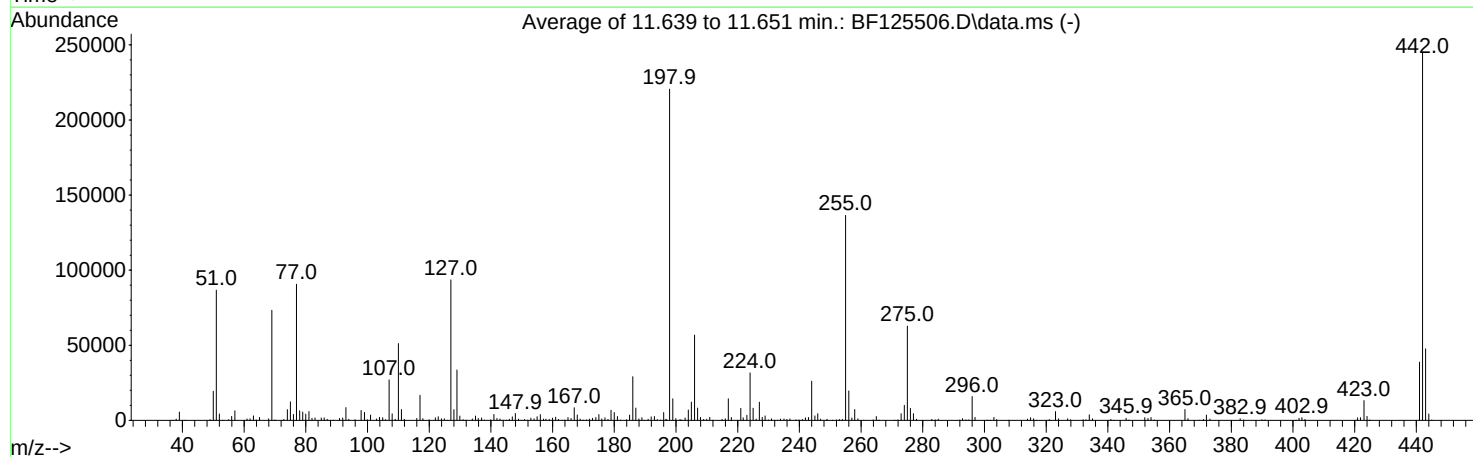


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091521\
 Data File : BF125506.D
 Acq On : 15 Sep 2021 16:07
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 15 15:08:32 2021

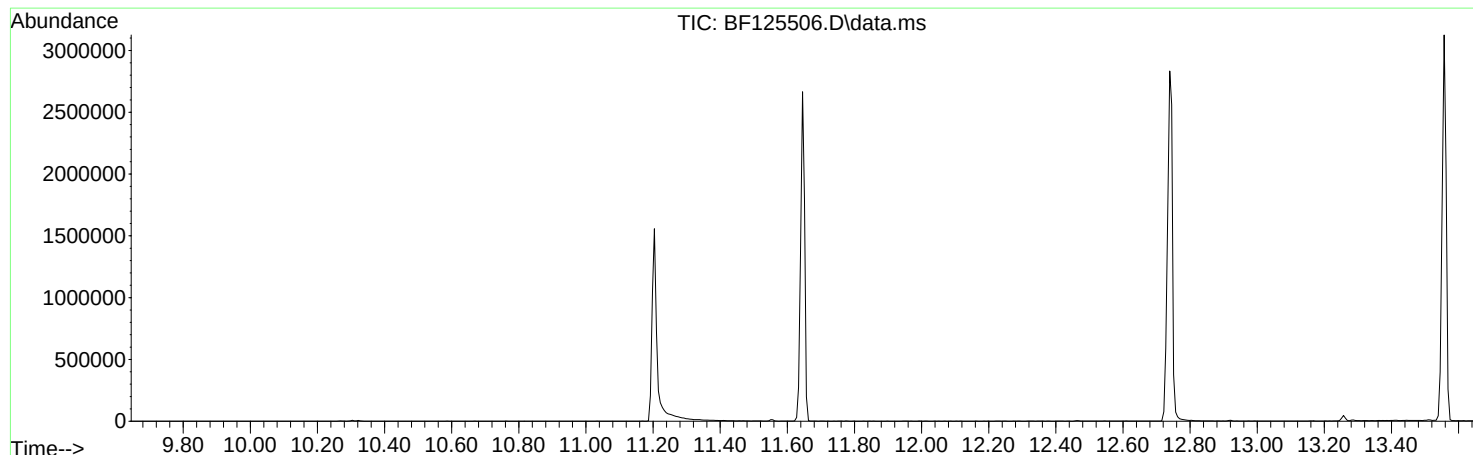

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	86712	PASS
68	69	0.00	2	1.5	1094	PASS
69	198	0.00	100	33.2	73296	PASS
70	69	0.00	2	0.4	268	PASS
127	198	10	80	42.4	93533	PASS
197	198	0.00	2	0.4	791	PASS
198	198	100	100	100.0	220544	PASS
199	198	5	9	6.5	14362	PASS
275	198	10	60	28.4	62715	PASS
365	198	1	100	3.3	7259	PASS
441	198	0.01	100	17.6	38765	PASS
442	442	50	100	100.0	244941	PASS
443	442	15	24	19.4	47592	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/15/2021	BNA_F	<u>BF125506.D</u>
Compound Name	Response	Retention Time
DDT	557634	13.55
DDD	8985	13.25
DDE	1236	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10221	567855	1.80

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091521\
Data File : BF125506.D
Acq On : 15 Sep 2021 16:07
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 15 18:24:06 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 15 15:08:32 2021
Response via : Initial Calibration

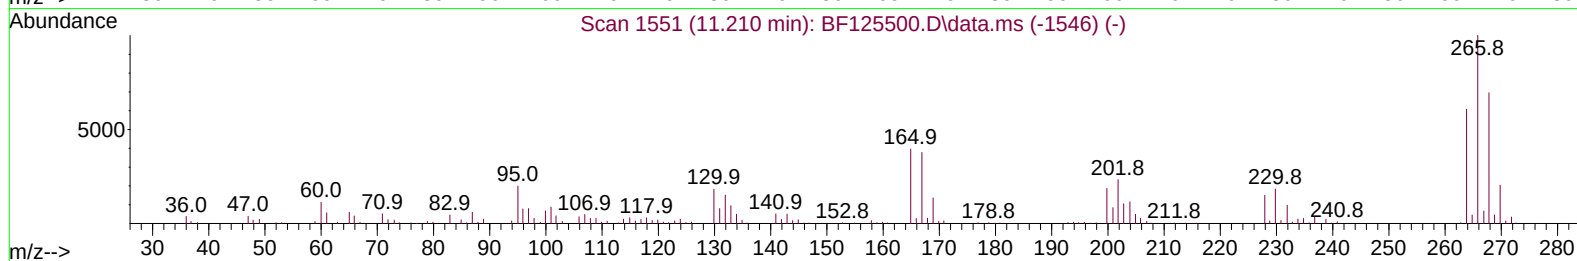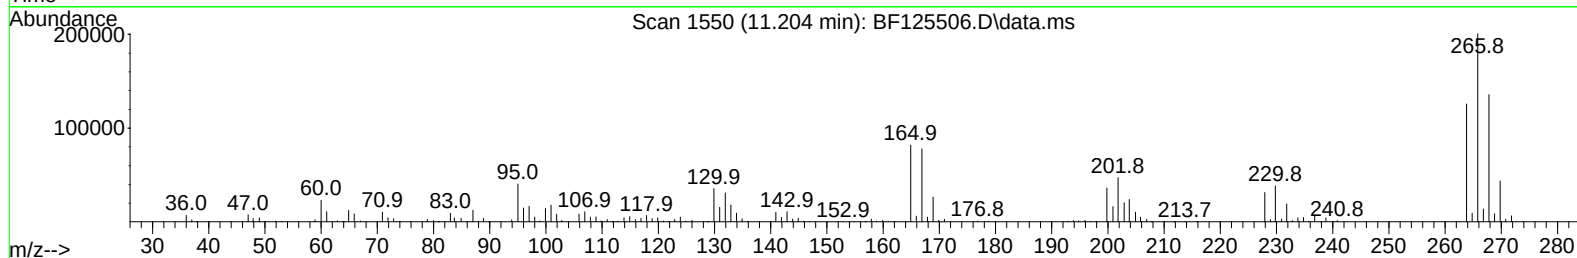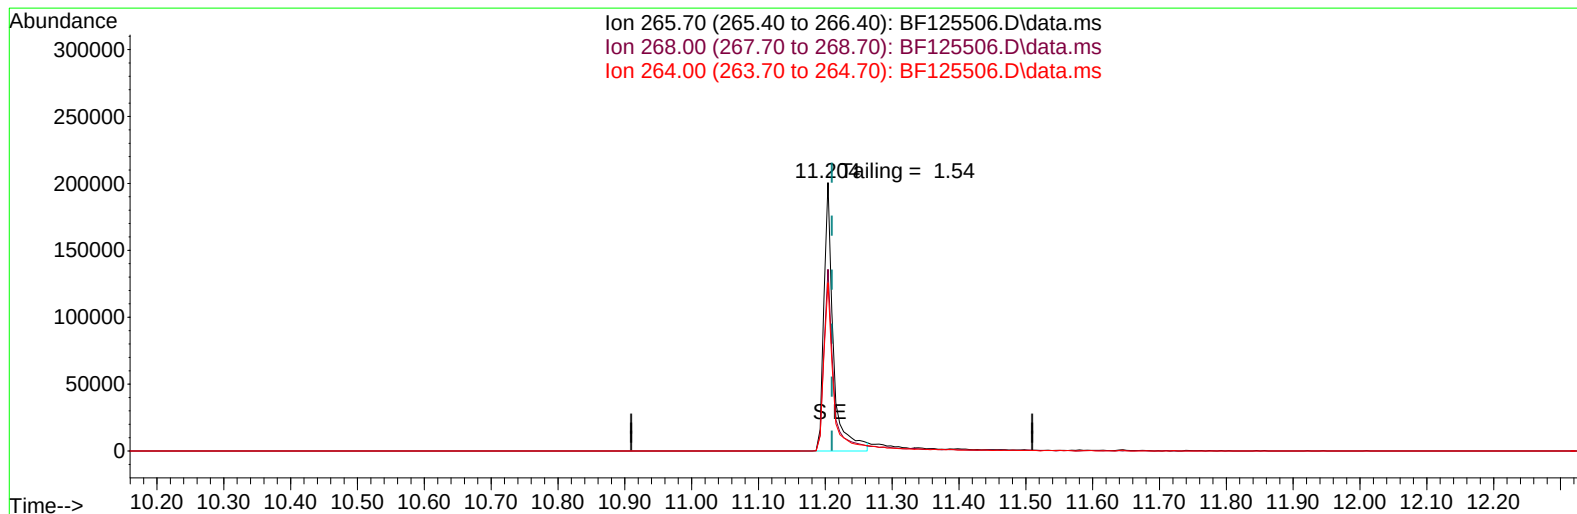

TIC: BF125506.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 34749.98 ng




response 211300

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	67.68
264.00	69.90	62.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091521\
Data File : BF125506.D
Acq On : 15 Sep 2021 16:07
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 15 18:24:06 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 15 15:08:32 2021
Response via : Initial Calibration

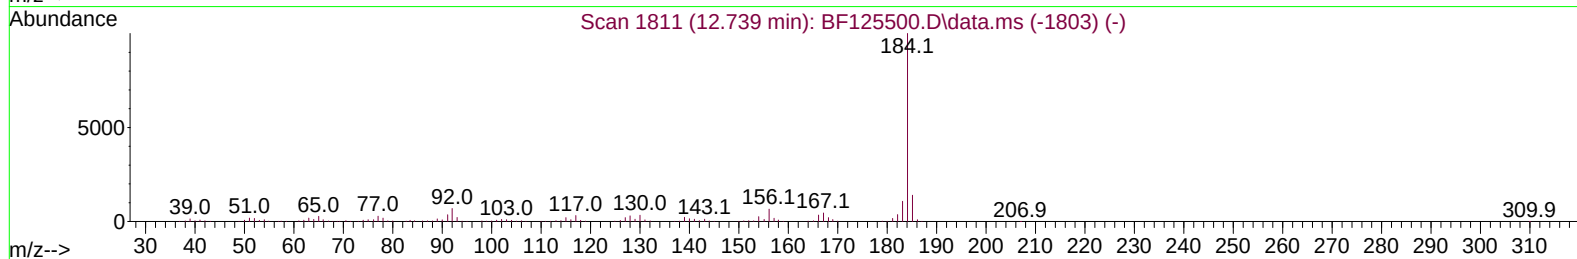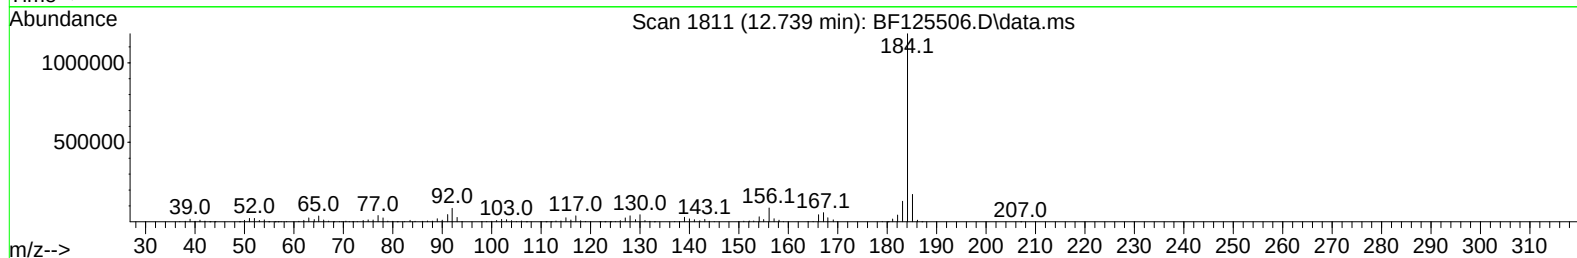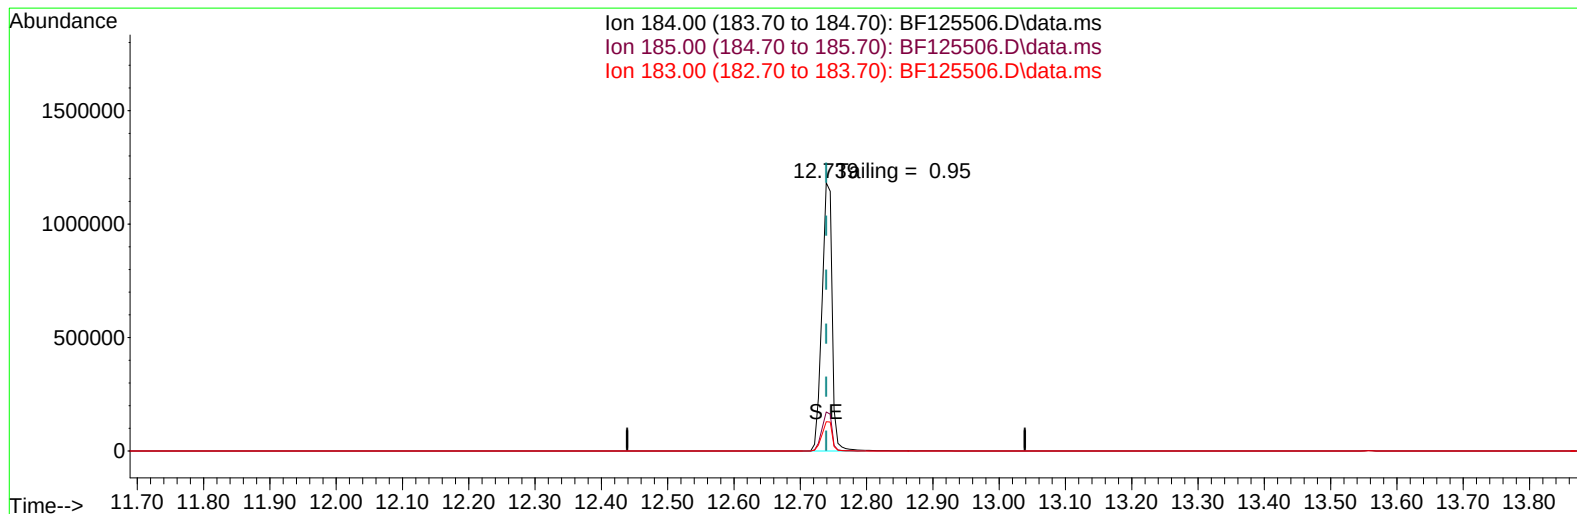

TIC: BF125506.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 0.00 ng

response 1252996

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.55
183.00	10.10	10.93
0.00	0.00	0.00