
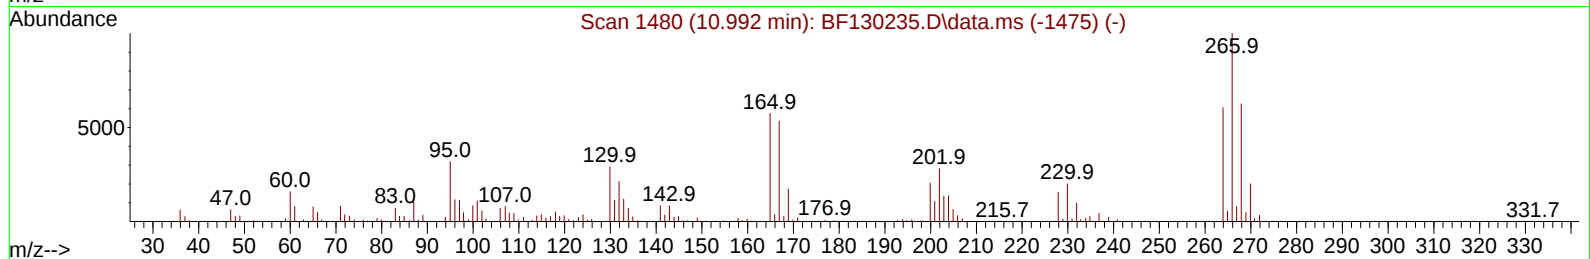
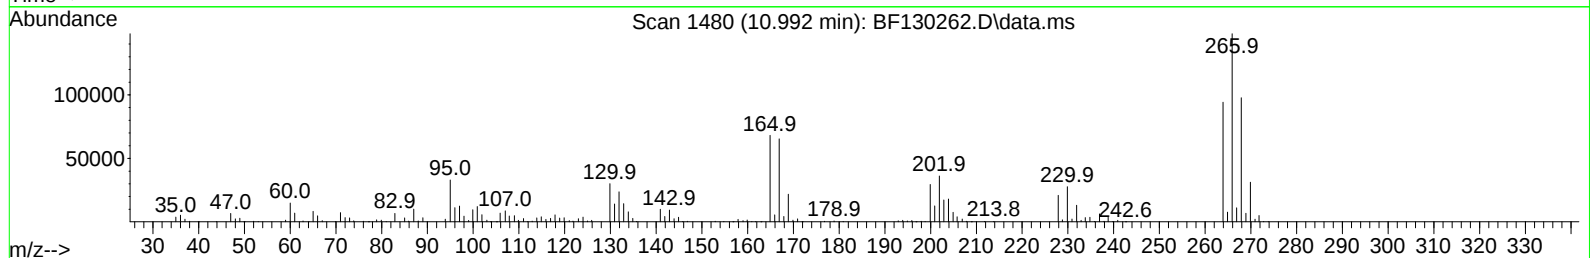


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091522\
 Data File : BF130262.D
 Acq On : 15 Sep 2022 09:33
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 07:45:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 14 14:55:51 2022
 Response via : Initial Calibration

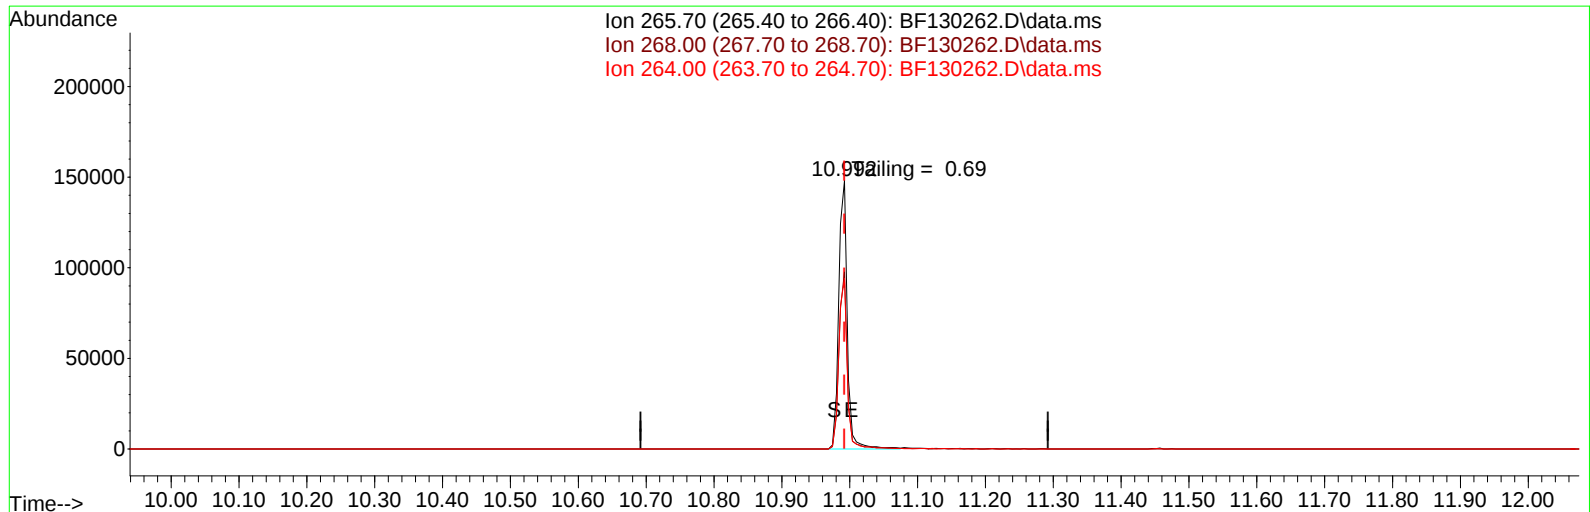

TIC: BF130262.D\data.ms

(70) Pentachlorophenol (C)




10.992min (+ 0.000) 26894.39 ng

response 129958

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.96
264.00	63.10	63.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091522\
Data File : BF130262.D
Acq On : 15 Sep 2022 09:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 07:45:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 14:55:51 2022
Response via : Initial Calibration

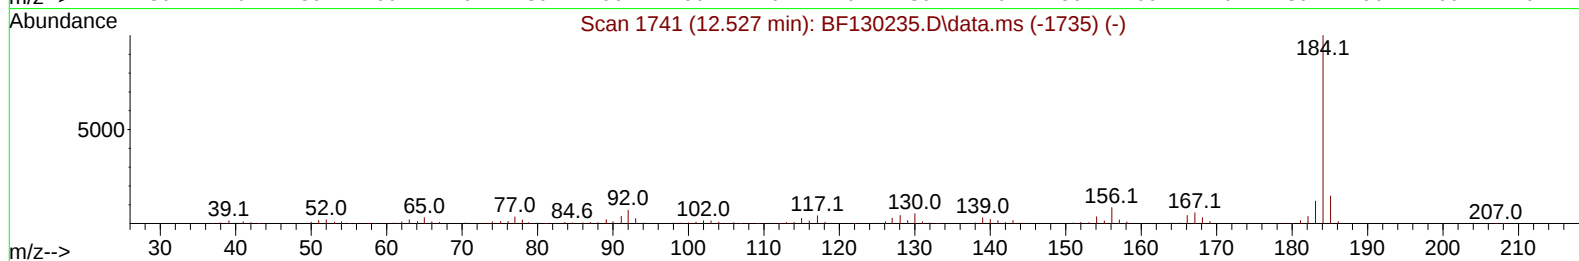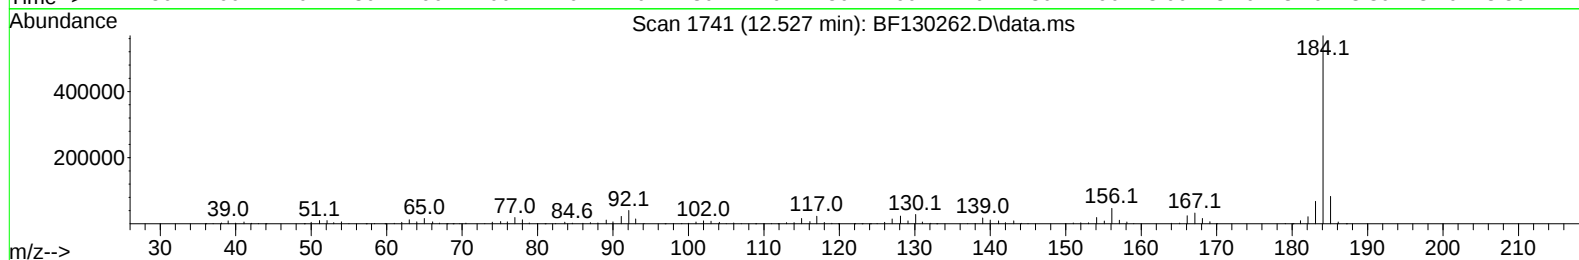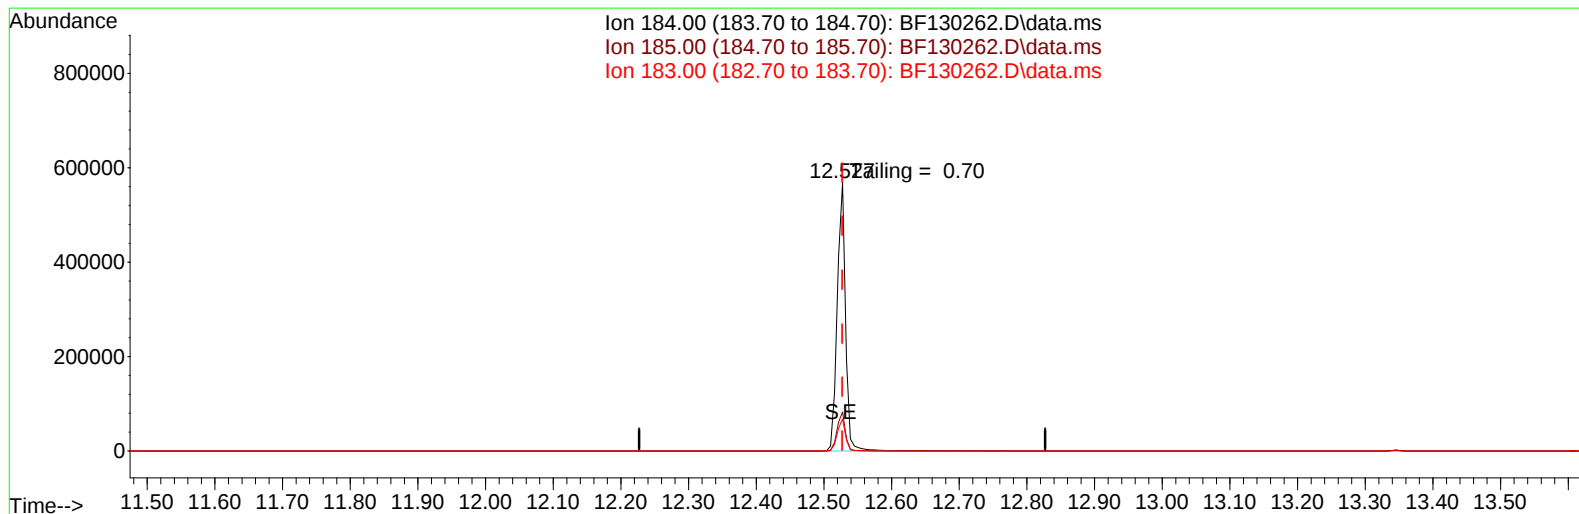

TIC: BF130262.D\data.ms

(77) Benzidine

12.527min (+ 0.000) 0.00 ng

response 483390

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.57
183.00	11.40	11.92
0.00	0.00	0.00