
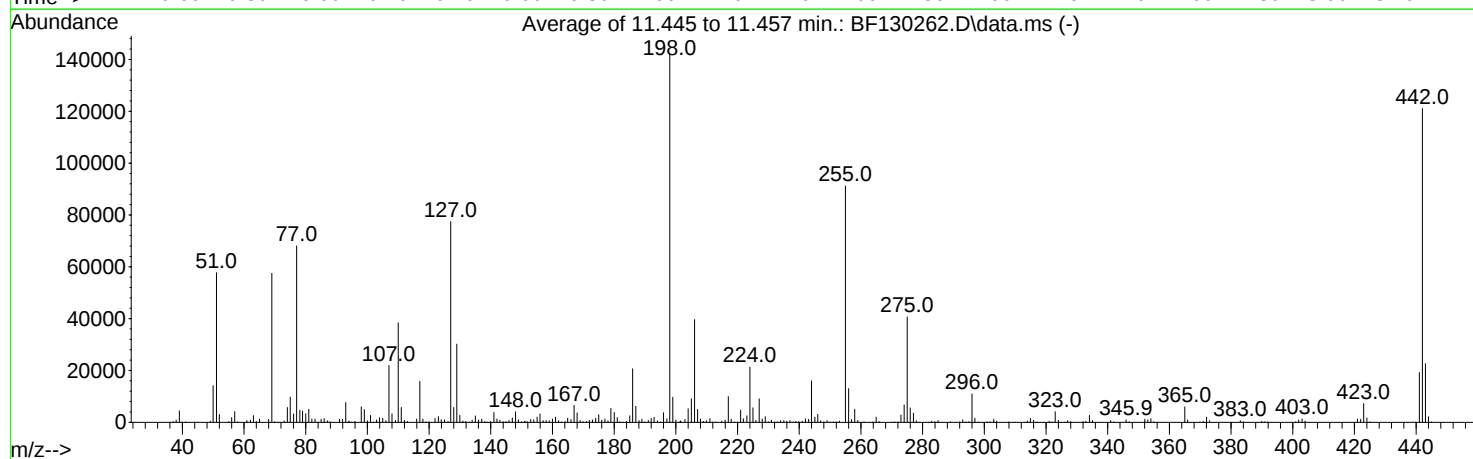


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091522\
 Data File : BF130262.D
 Acq On : 15 Sep 2022 09:33
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 14 14:55:51 2022

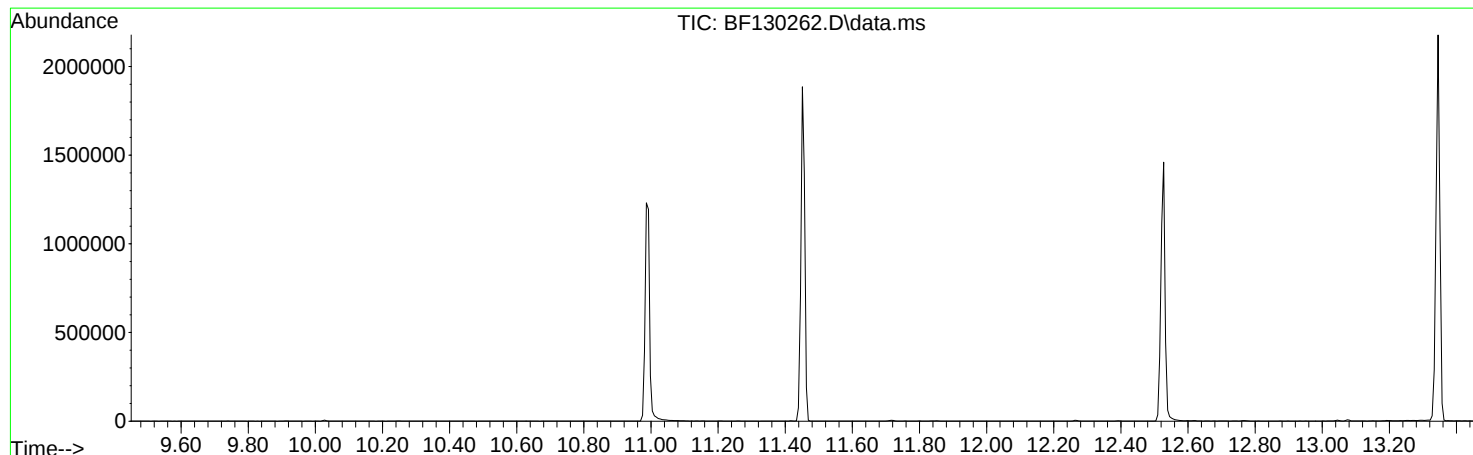




AutoFind: Scans 1557, 1558, 1559; Background Corrected with Scan 1552

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	57672	PASS
68	69	0.00	2	2.0	1126	PASS
69	198	0.00	100	40.5	57483	PASS
70	69	0.00	2	0.4	243	PASS
127	198	10	80	54.6	77464	PASS
197	198	0.00	2	0.9	1318	PASS
198	198	100	100	100.0	141939	PASS
199	198	5	9	6.8	9681	PASS
275	198	10	60	28.7	40685	PASS
365	198	1	100	4.2	5959	PASS
441	198	0.01	100	13.5	19183	PASS
442	442	50	100	100.0	121053	PASS
443	442	15	24	18.7	22620	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091522\
 Data File : BF130262.D
 Acq On : 15 Sep 2022 09:33
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 16 07:45:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 14 14:55:51 2022
 Response via : Initial Calibration

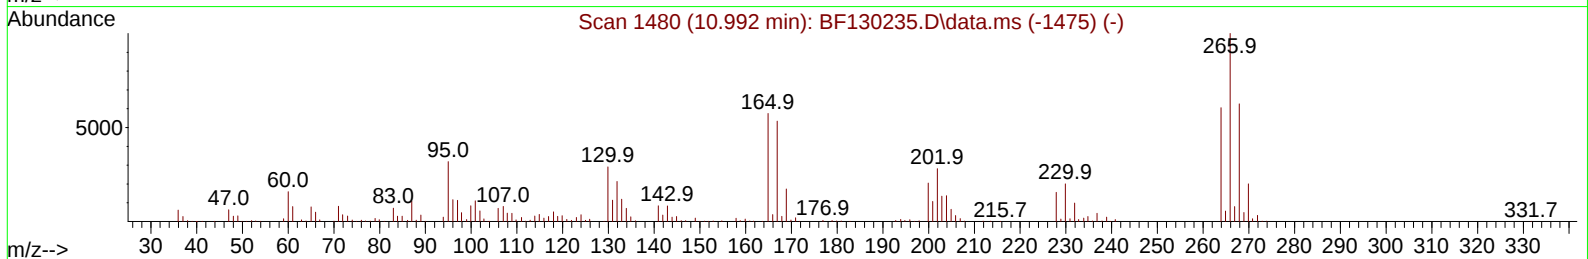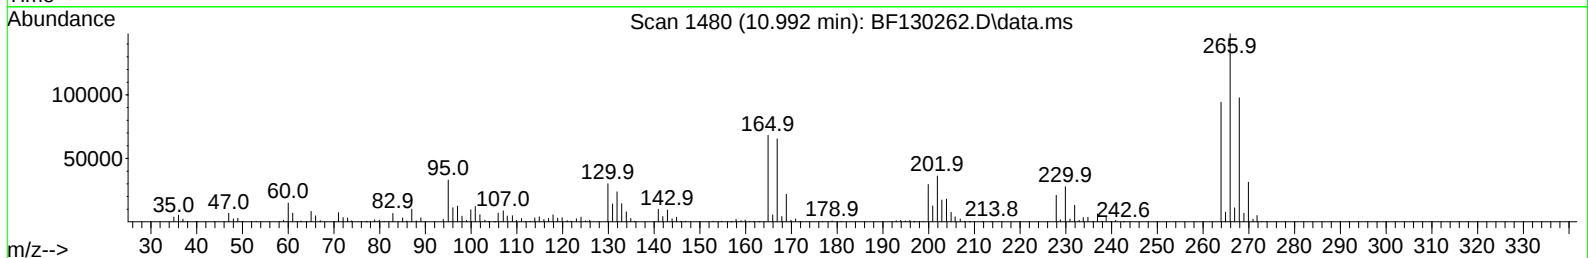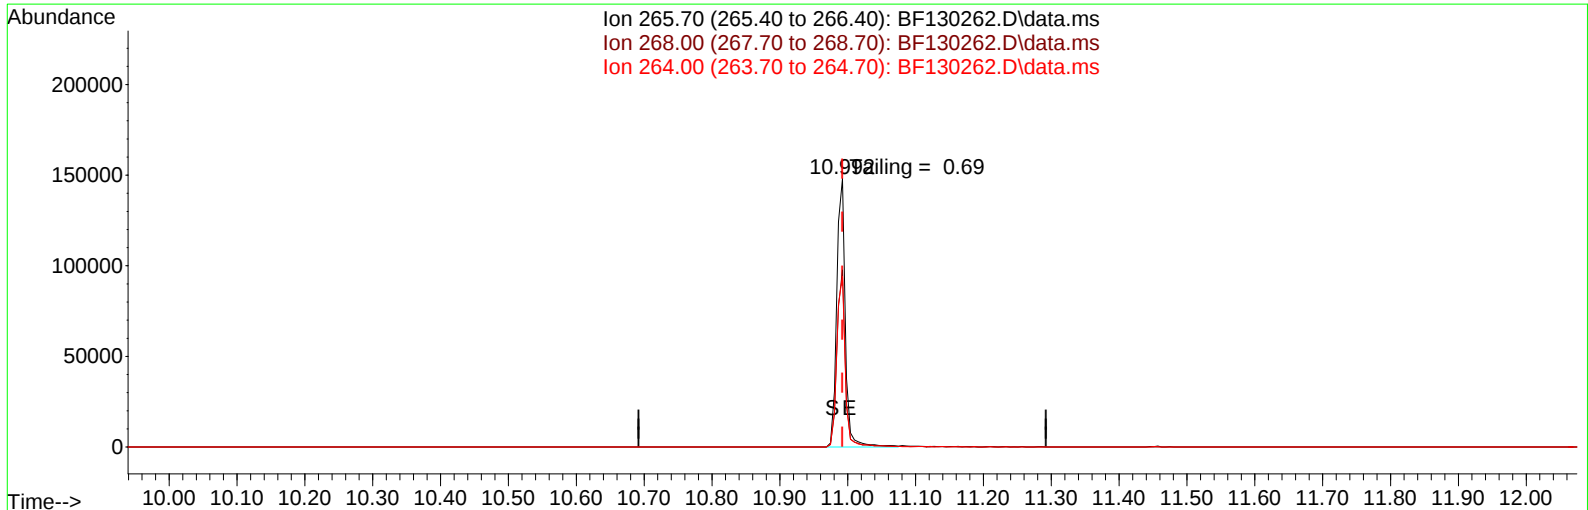

TIC: BF130262.D\data.ms

(70) Pentachlorophenol (C)

10.992min (+ 0.000) 26894.39 ng




response 129958

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.96
264.00	63.10	63.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091522\
Data File : BF130262.D
Acq On : 15 Sep 2022 09:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 16 07:45:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 14 14:55:51 2022
Response via : Initial Calibration

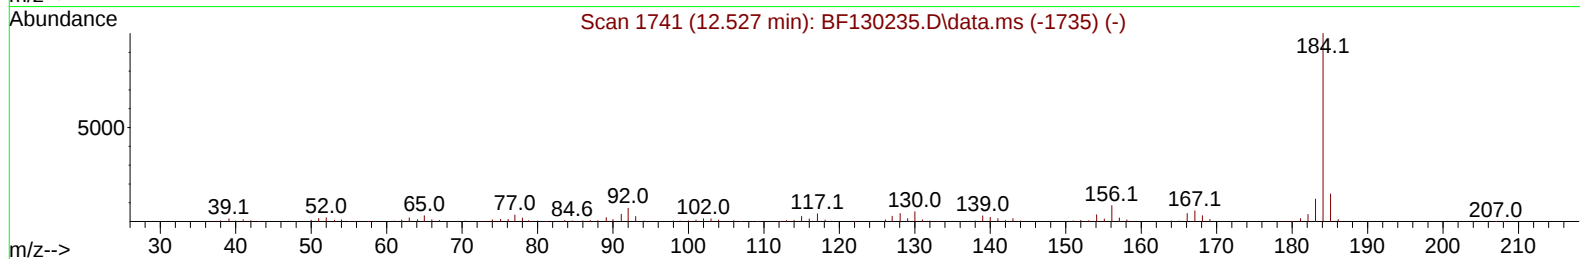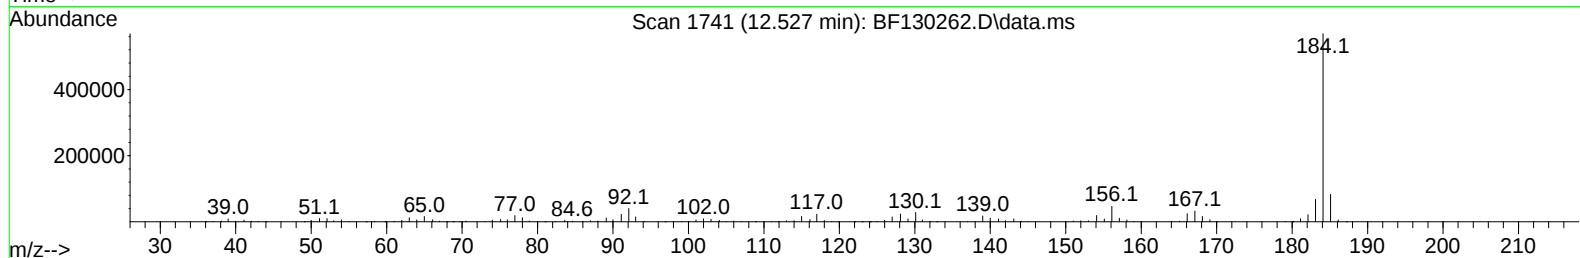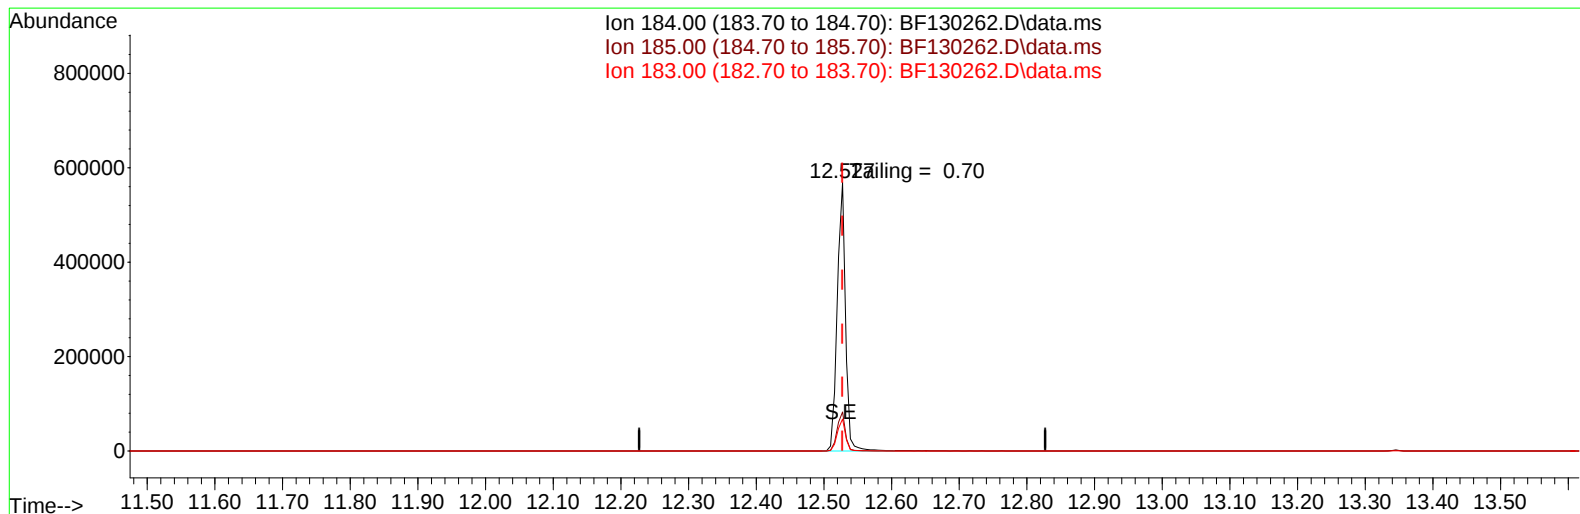

TIC: BF130262.D\data.ms

(77) Benzidine

12.527min (+ 0.000) 0.00 ng

response 483390

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.57
183.00	11.40	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/15/2022	BNA_F	<u>BF130262.D</u>
Compound Name	Response	Retention Time
DDT	316404	13.345
DDD	2324	13.045
DDE	153	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2477	318881	0.78

Instrument :
BNA_F
ClientSampleId :
DFTPP