
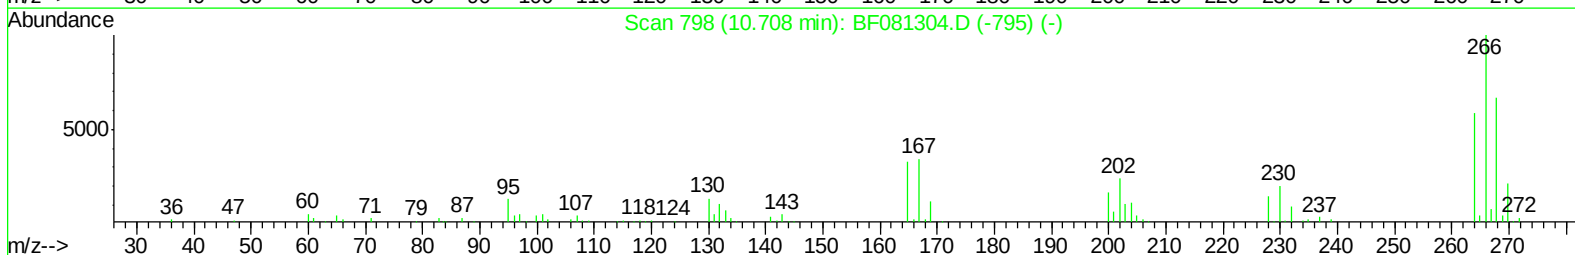
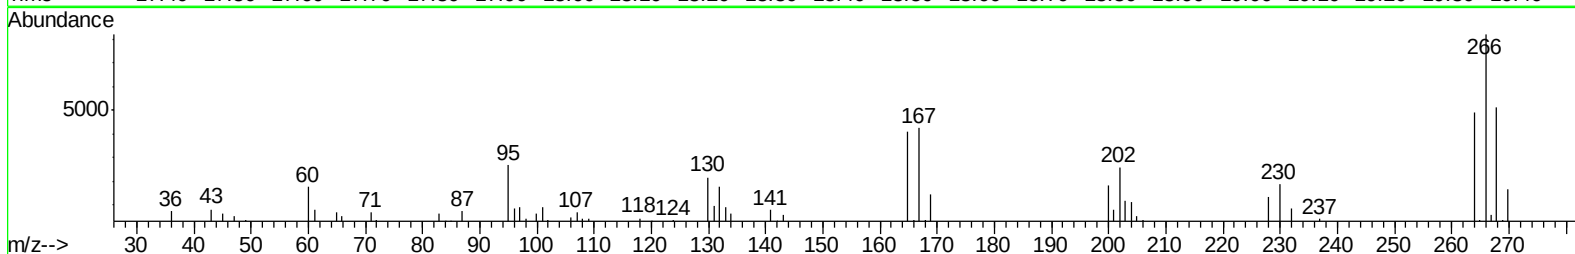


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091615\
Data File : BF081643.D
Acq On : 16 Sep 2015 10:48
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 05:13:31 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 15 14:03:59 2015
Response via : Initial Calibration

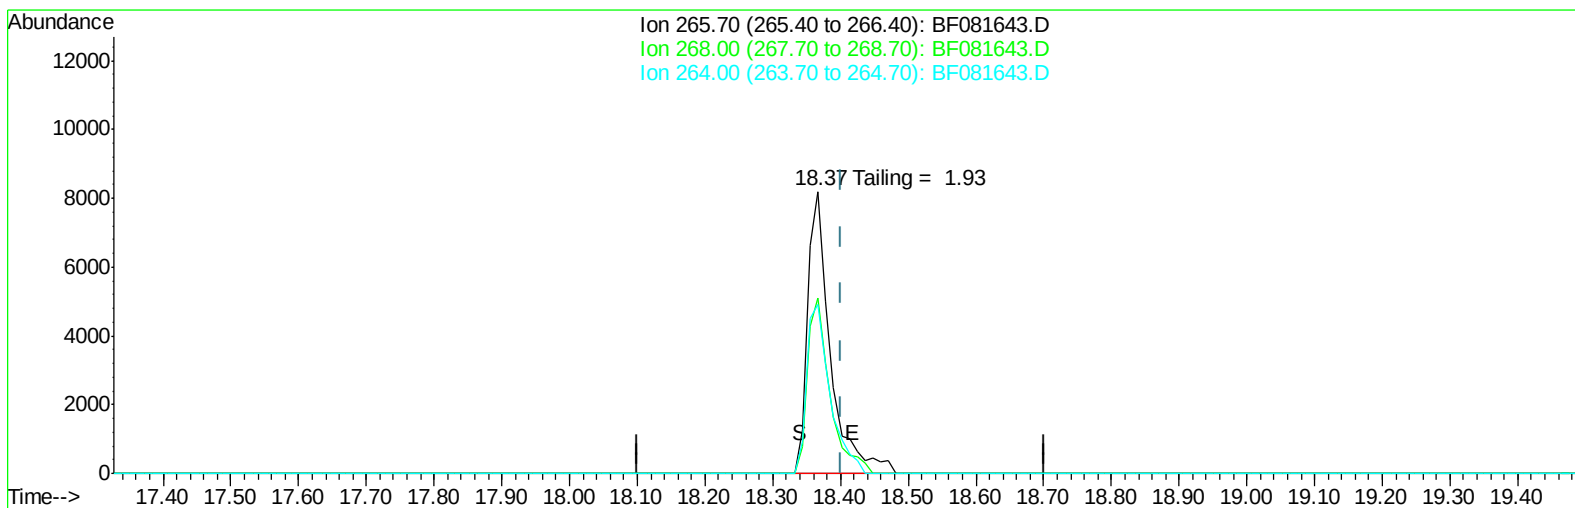

TIC: BF081643.D

(69) Pentachlorophenol (C)




18.367min (-0.034) 0.00ng

response 19117

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	62.23
264.00	62.70	59.88
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091615\
Data File : BF081643.D
Acq On : 16 Sep 2015 10:48
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 05:13:31 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 15 14:03:59 2015
Response via : Initial Calibration

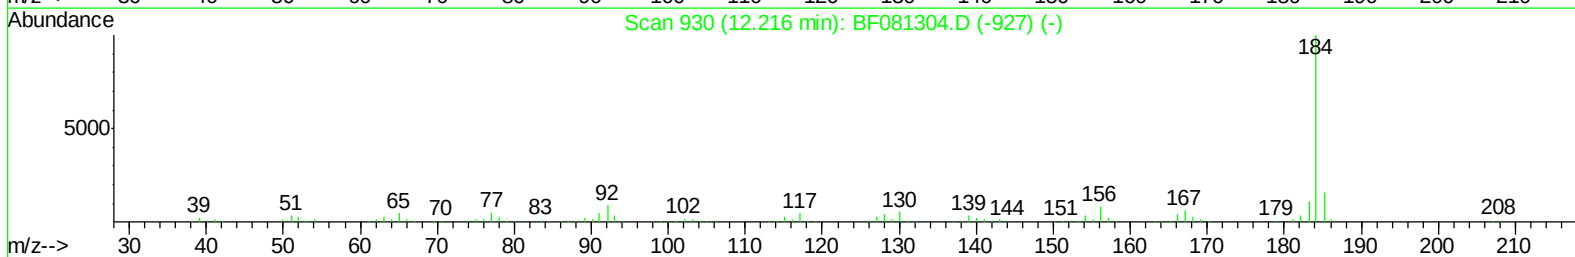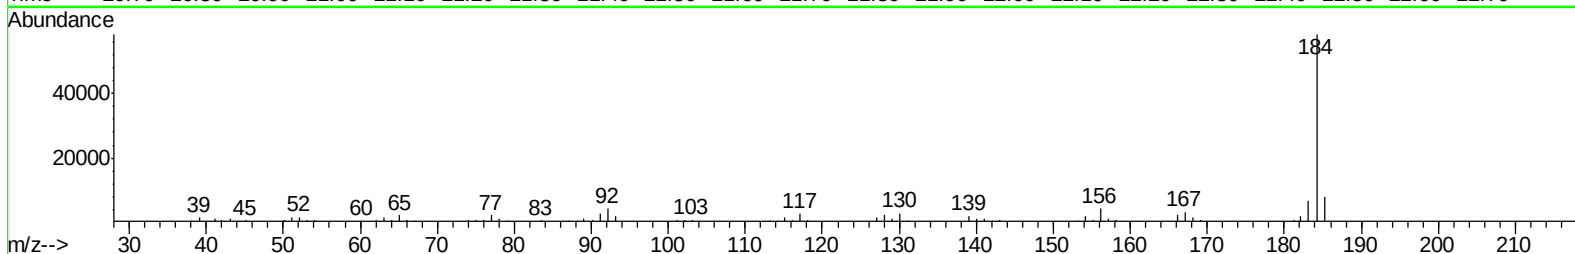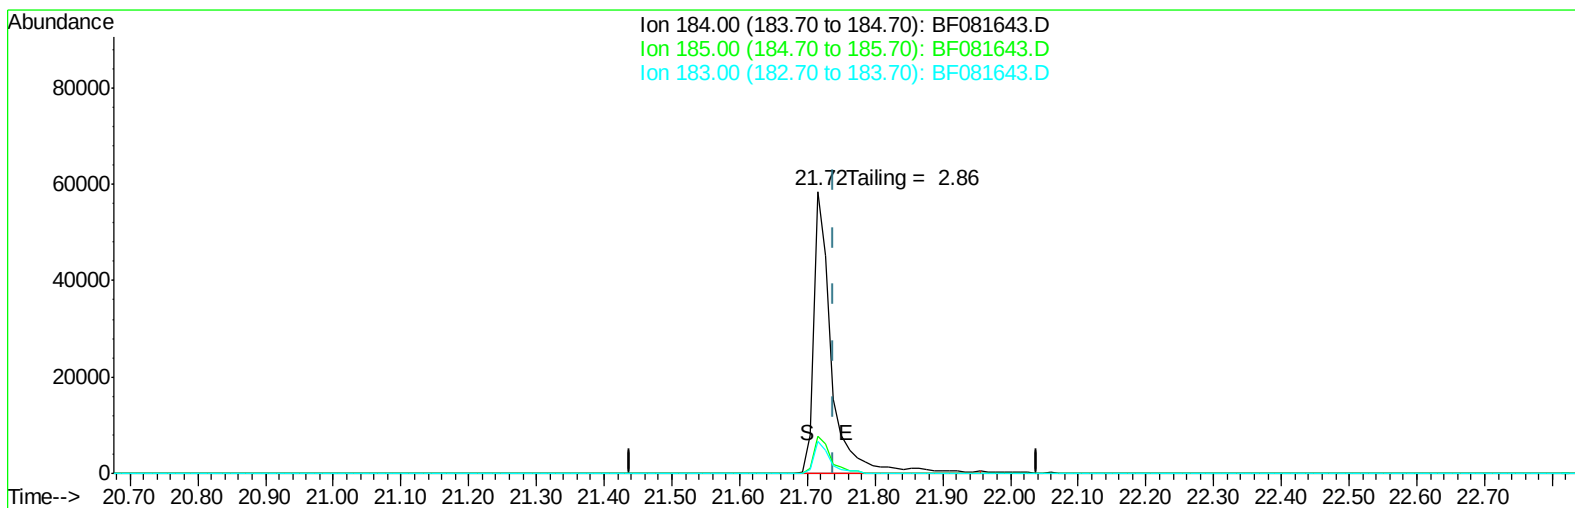

TIC: BF081643.D

(76) Benzidine

21.716min (-0.023) 0.00ng m

response 108177

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.23
183.00	9.50	11.47#
0.00	0.00	0.00