
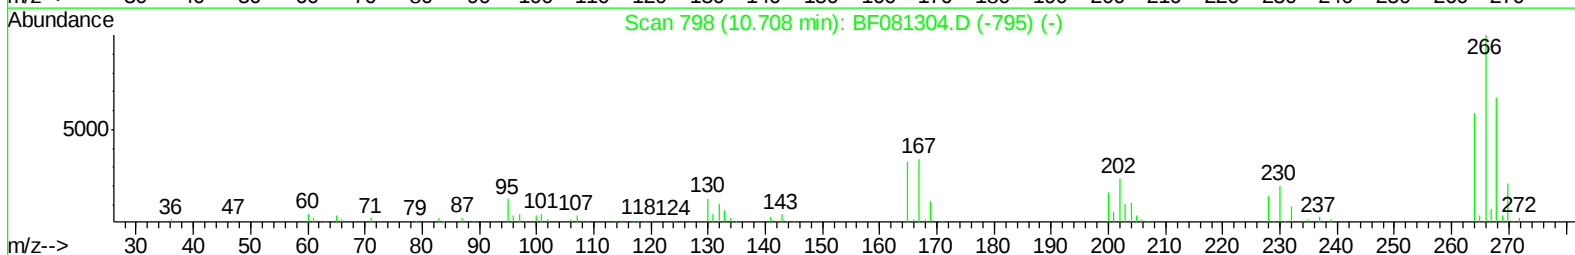
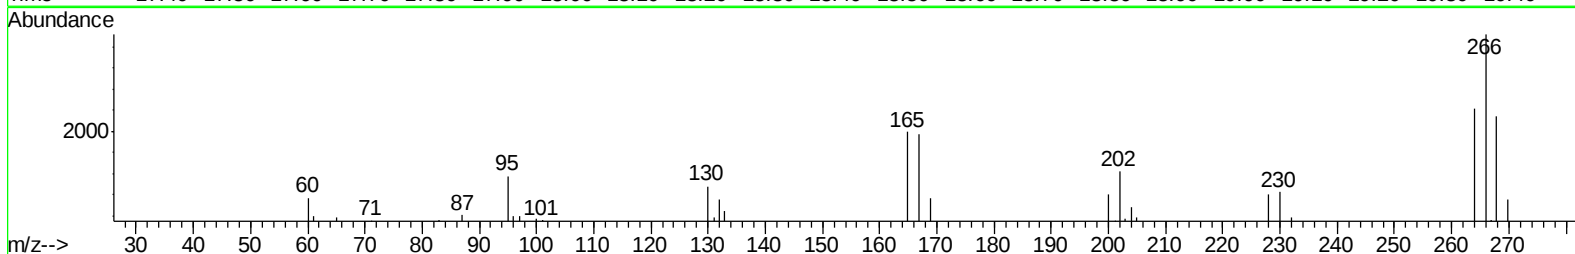


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF091615\  
Data File : BF081661.D  
Acq On : 17 Sep 2015 1:48  
Operator : UM/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 05:23:02 2015  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF090115.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 15 14:03:59 2015  
Response via : Initial Calibration

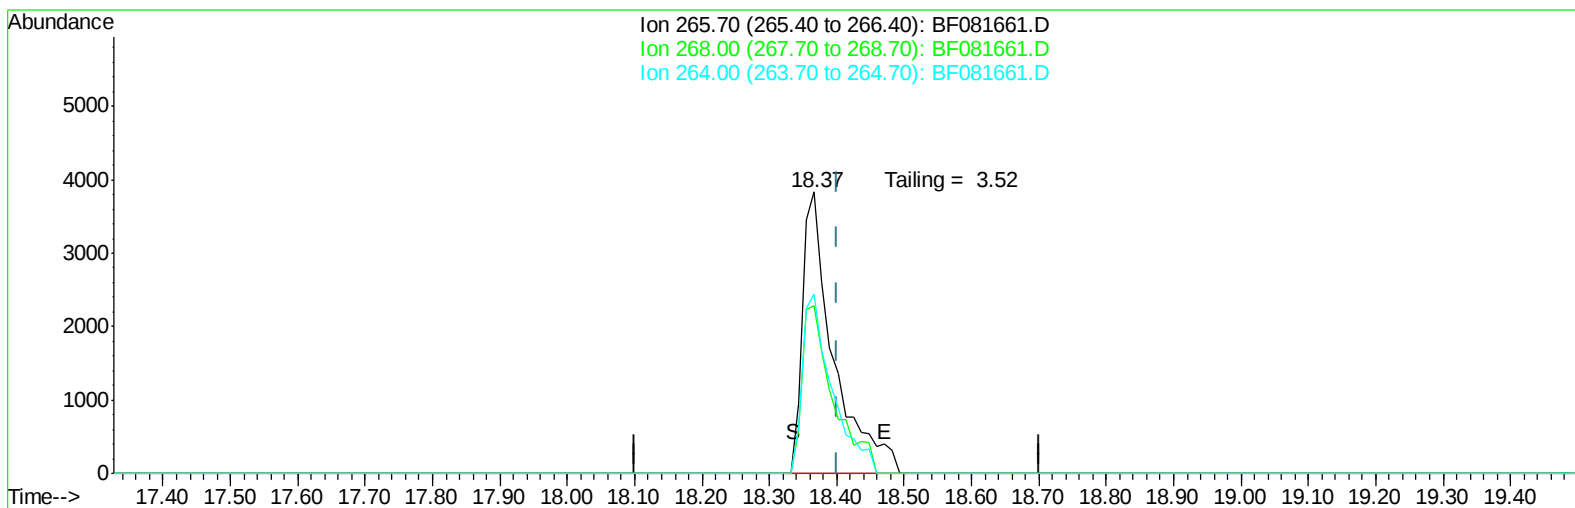

TIC: BF081661.D

(69) Pentachlorophenol (C)




18.367min (-0.034) 0.00ng

response 12108

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 62.20 | 59.41 |
| 264.00 | 62.70 | 63.71 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\Data\BF091615\  
Data File : BF081661.D  
Acq On : 17 Sep 2015 1:48  
Operator : UM/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 05:23:02 2015  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF090115.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 15 14:03:59 2015  
Response via : Initial Calibration

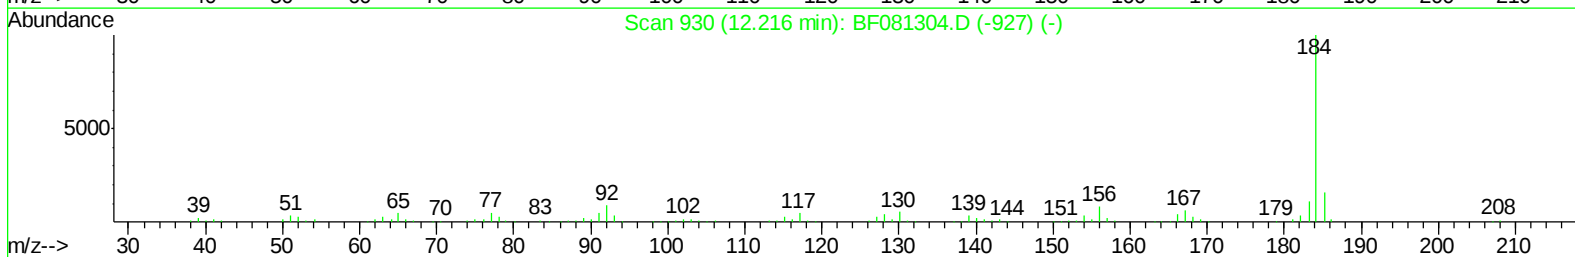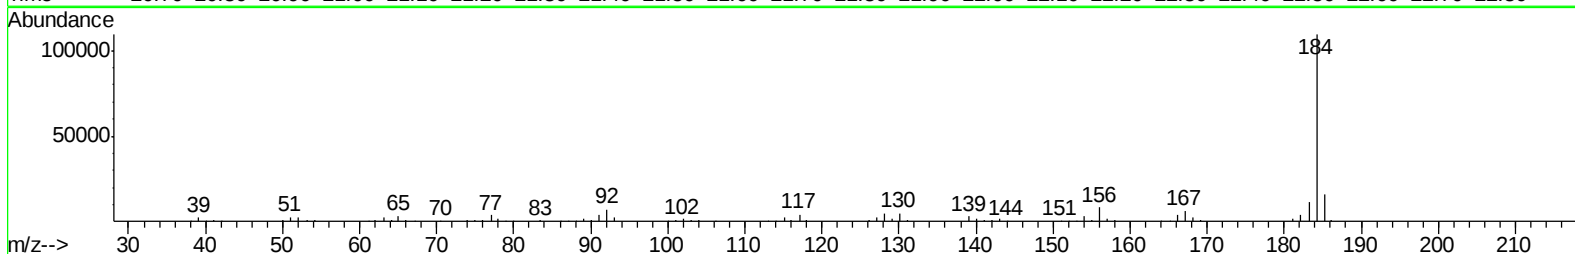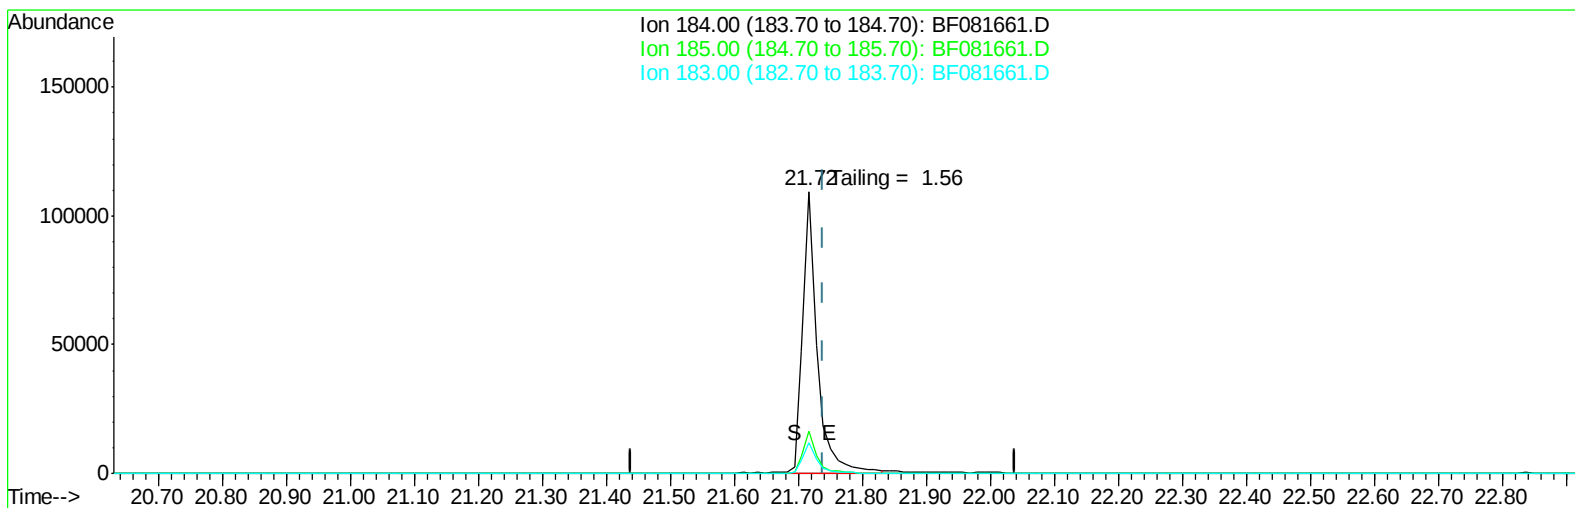

TIC: BF081661.D

(76) Benzidine

21.716min (-0.023) 0.00ng

response 178421

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.70 | 14.89 |
| 183.00 | 9.50  | 10.78 |
| 0.00   | 0.00  | 0.00  |