

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091615\
 Data File : BF081667.D
 Acq On : 17 Sep 2015 5:27
 Operator : UM/IZ
 Sample : G3637-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 VITALE-FILL-SOURCE-1A

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.440	8	9	15	rBV	100034	278002	15.98%	1.589%
2	1.531	15	17	46	rVB	528471	1739217	100.00%	9.942%
3	4.480	269	275	294	rBV	290373	898520	51.66%	5.136%
4	5.349	347	351	366	rBV	751848	1525249	87.70%	8.719%
5	7.612	544	549	551	rBV	790480	1570810	90.32%	8.979%
6	7.703	553	557	567	rVB	947832	1632549	93.87%	9.332%
7	8.183	596	599	606	rVB	187645	297513	17.11%	1.701%
8	8.515	624	628	631	rBV	656572	1159646	66.68%	6.629%
9	9.486	708	713	729	rBV	574339	1038547	59.71%	5.937%
10	11.075	849	852	858	rBV	205668	377243	21.69%	2.156%
11	13.727	1079	1084	1087	rBV	968674	1711259	98.39%	9.782%
12	14.778	1172	1176	1184	rBV	187216	307423	17.68%	1.757%
13	15.212	1210	1214	1219	rBB	241694	402759	23.16%	2.302%
14	16.607	1333	1336	1340	rBB	13753	25945	1.49%	0.148%
15	17.110	1376	1380	1391	rBB	572451	1084178	62.34%	6.198%
16	17.750	1432	1436	1442	rBV	21423	52428	3.01%	0.300%
17	18.710	1516	1520	1524	rBV	245931	420422	24.17%	2.403%
18	18.836	1527	1531	1534	rBV	19618	31128	1.79%	0.178%
19	19.864	1618	1621	1626	rBV	12047	20016	1.15%	0.114%
20	20.470	1671	1674	1681	rBV	76763	165661	9.53%	0.947%
21	21.750	1781	1786	1790	rBV3	8321	19144	1.10%	0.109%
22	21.876	1795	1797	1804	rBV	27245	47814	2.75%	0.273%
23	22.082	1811	1815	1818	rBV	1263732	1560071	89.70%	8.918%
24	23.350	1920	1926	1929	rBV	366845	498827	28.68%	2.852%
25	23.682	1953	1955	1960	rVB5	11216	17676	1.02%	0.101%
26	24.013	1982	1984	1988	rBV2	33193	55524	3.19%	0.317%
27	24.368	2013	2015	2018	rBV	73961	107565	6.18%	0.615%
28	24.608	2034	2036	2042	rBV	32224	54716	3.15%	0.313%
29	24.790	2050	2052	2058	rBV	236519	251492	14.46%	1.438%
30	25.236	2089	2091	2099	rVB4	19688	60659	3.49%	0.347%
31	25.728	2131	2134	2137	rVB3	12330	23932	1.38%	0.137%
32	26.219	2174	2177	2183	rBV6	12767	37609	2.16%	0.215%
33	26.894	2233	2236	2241	rVB7	7762	19897	1.14%	0.114%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091615\
Data File : BF081667.D
Acq On : 17 Sep 2015 5:27
Operator : UM/IZ
Sample : G3637-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VITALE-FILL-SOURCE-1A

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 17493441

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091615\
Data File : BF081667.D
Acq On : 17 Sep 2015 5:27
Operator : UM/IZ
Sample : G3637-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VITALE-FILL-SOURCE-1A

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

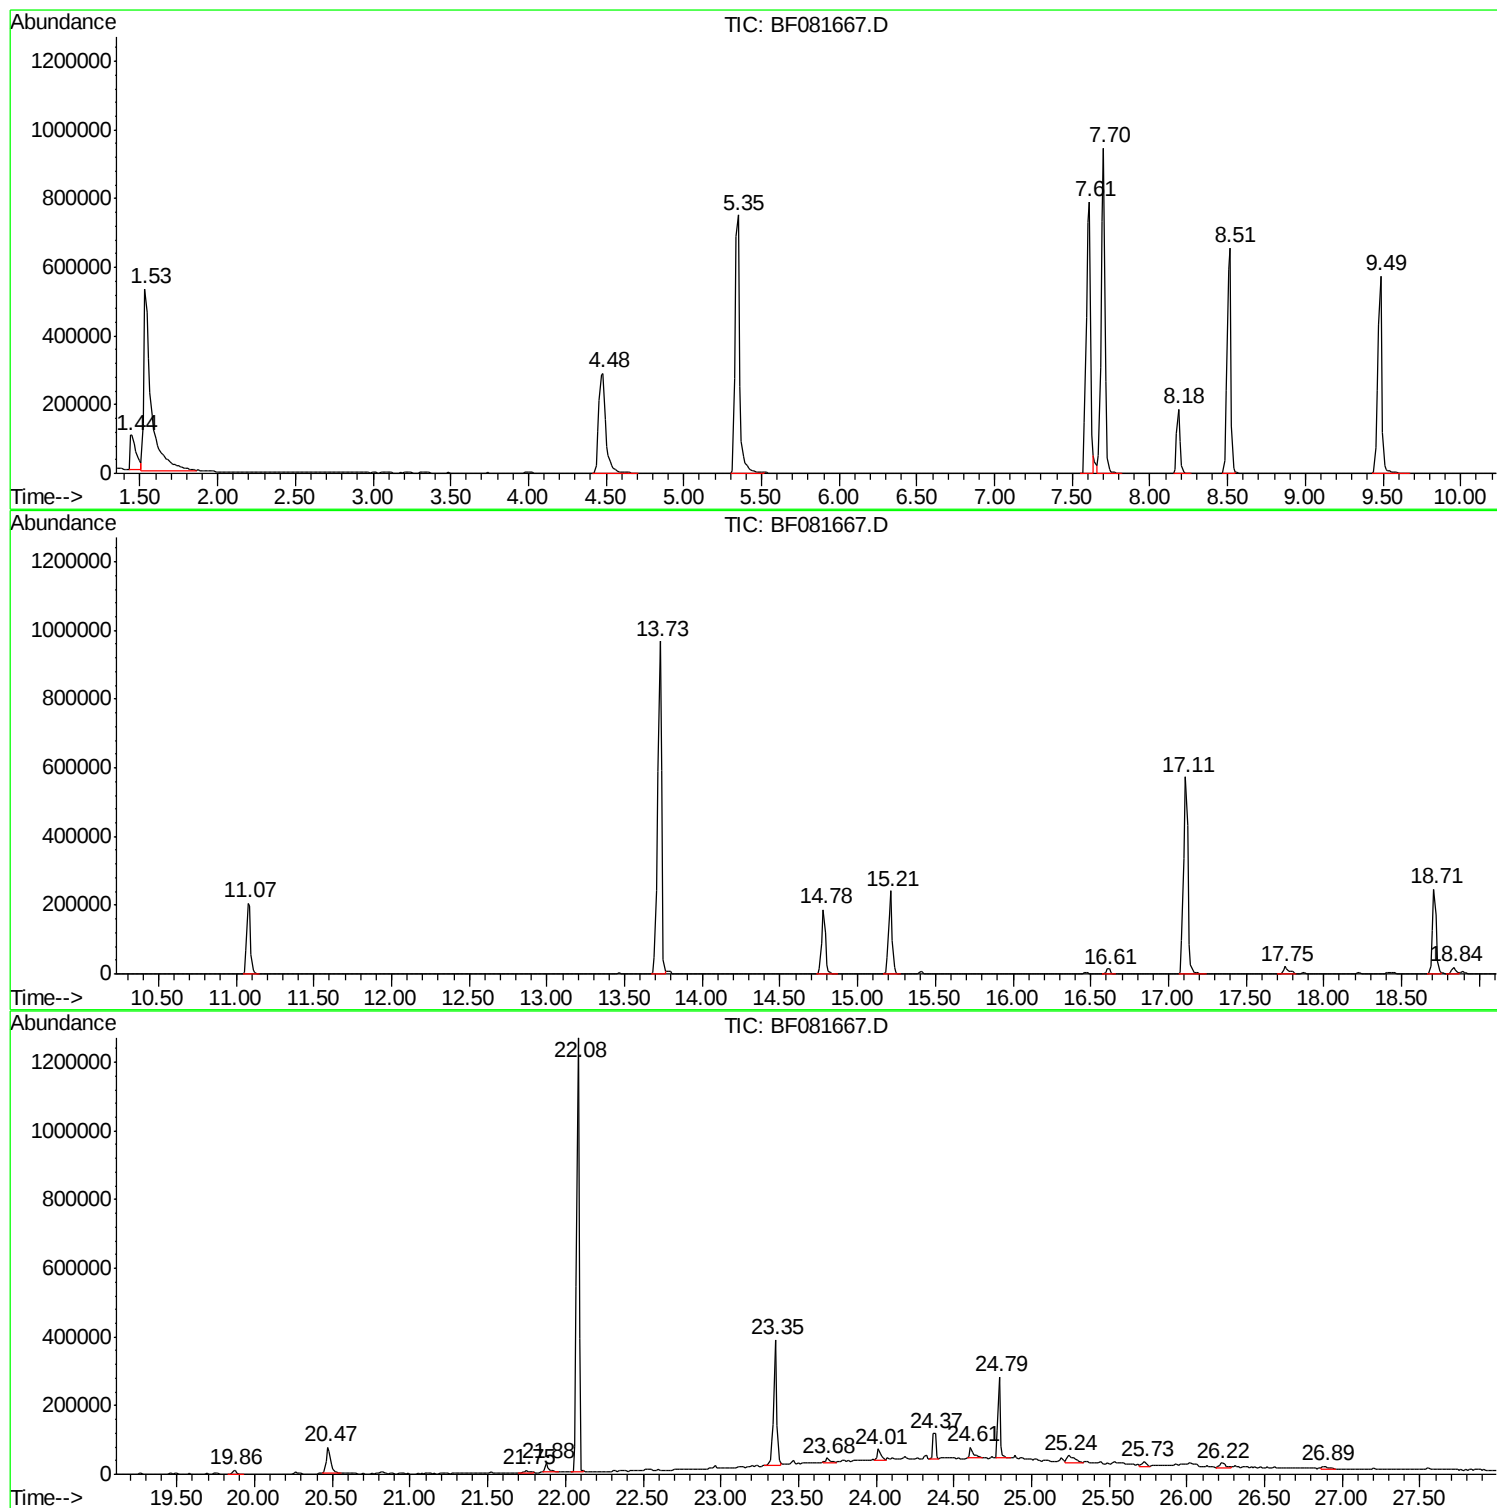

DbaaaPath::ZZ\NRP8888\BNAF\DATA\BB0006655\
 DbaaaFile::BB003667DD
 Aeqq00n ::17S8pp20055 55227
 Opeaaor ::UMMIZ
 Saaope ::G6637001
 MISC ::
 AASSVaal ::224 SaaopeMMuippler:11

Instrument :
 BNA_F
 ClientSampleId :
 VITALE-FILL-SOURCE-1A

QqaattMebbdd::ZZ\NRP8888\BNAF\MEH00S82Z00BB000155MM
 QqaattTille ::ASBPBNASSANDABBSF00R55P000NTCALIBRATION

TICLibbaay ::
 TICInteggaafionPaaameess:rteenttp

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
