


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091615\
 Data File : BF081643.D
 Acq On : 16 Sep 2015 10:48
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 15 14:03:59 2015

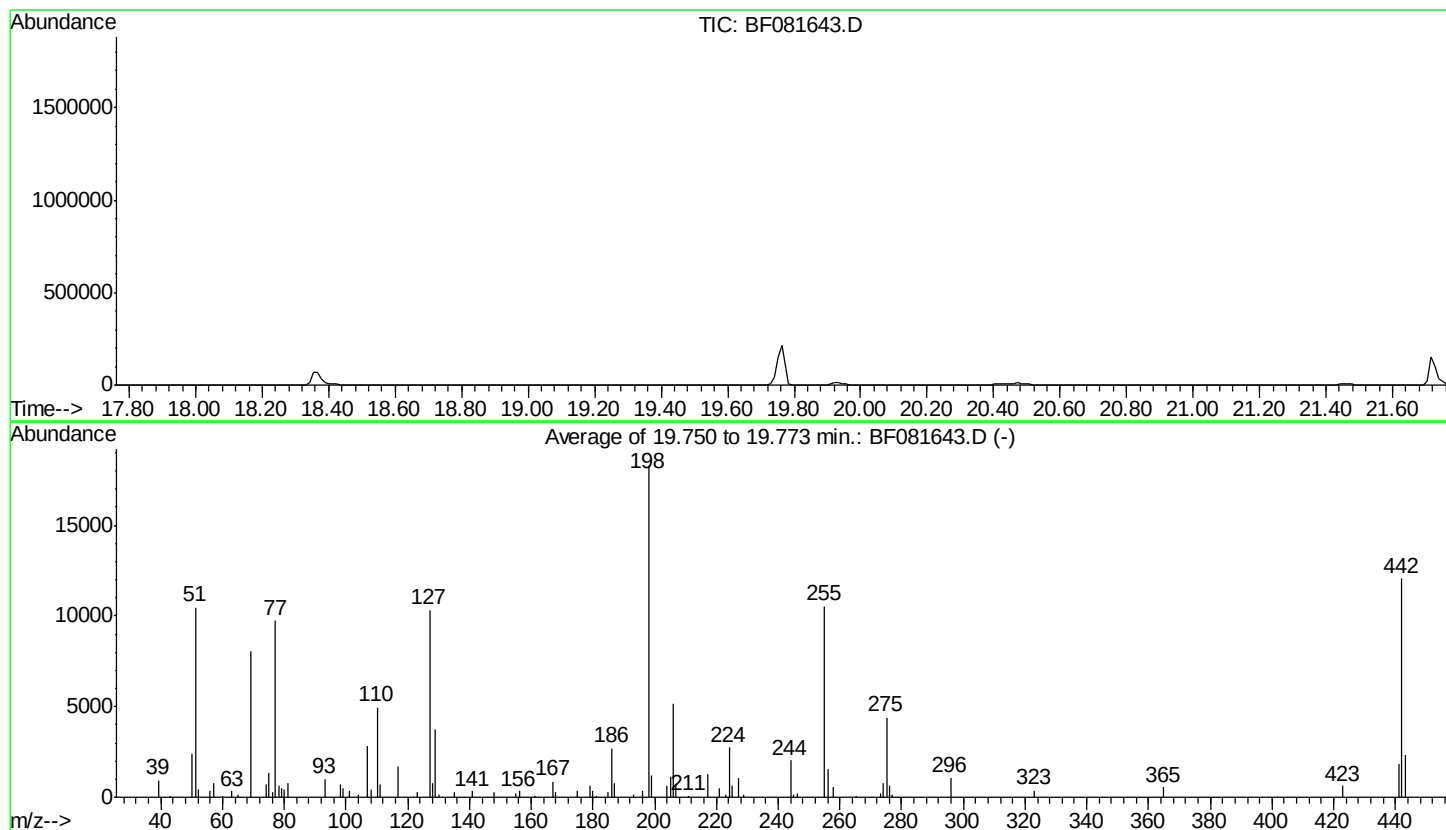

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.3	10475	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.1	8065	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.5	10343	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18296	PASS
199	198	5	9	6.7	1233	PASS
275	198	10	60	24.1	4404	PASS
365	198	1	100	2.9	532	PASS
441	442	0.01	24	15.4	1857	PASS
442	198	50	100	65.9	12052	PASS
443	442	15	24	19.3	2329	PASS