


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091615\
 Data File : BF081661.D
 Acq On : 17 Sep 2015 1:48
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 15 14:03:59 2015

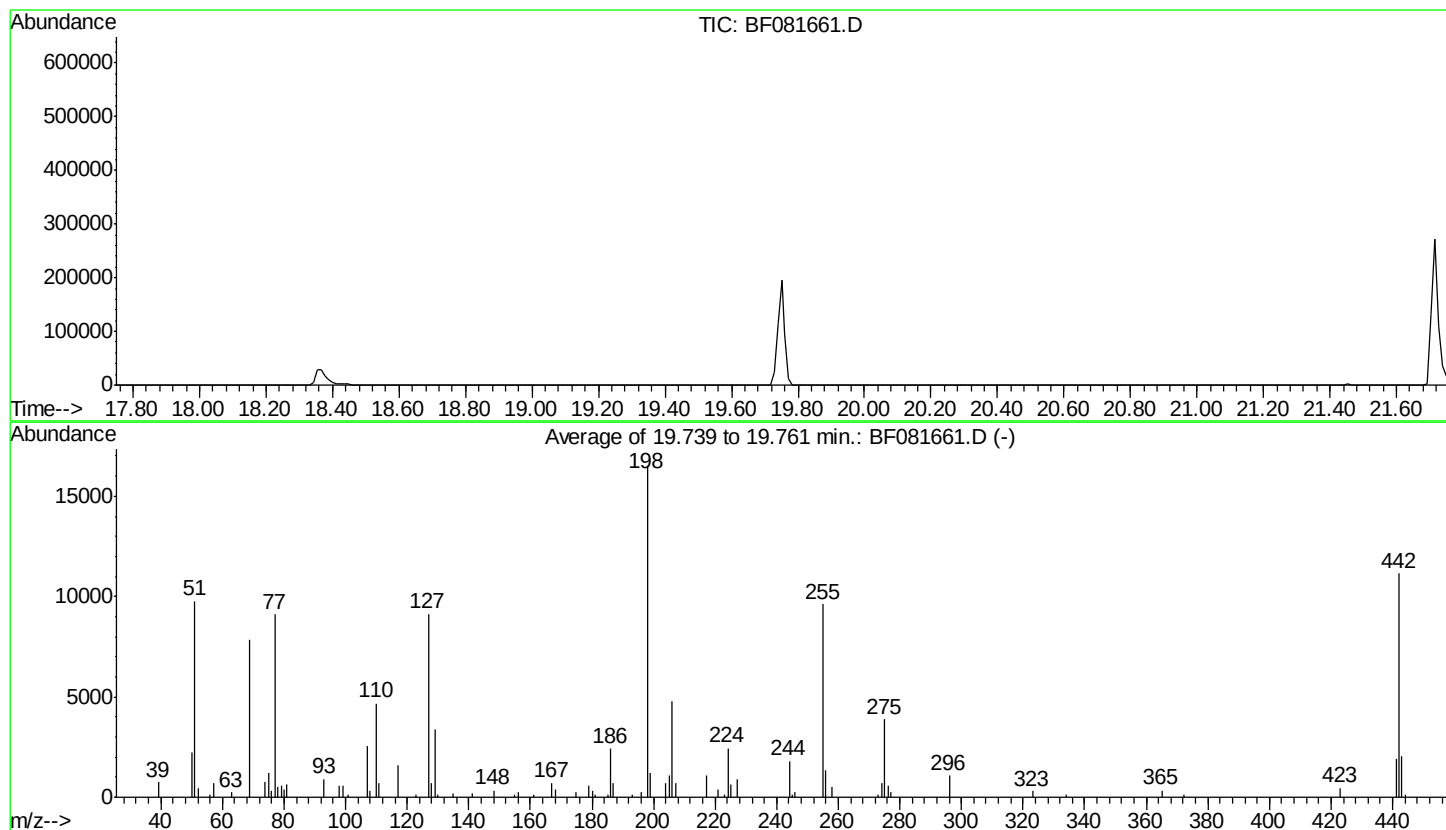

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.2	9776	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.5	7848	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.3	9128	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	16521	PASS
199	198	5	9	7.3	1210	PASS
275	198	10	60	23.5	3885	PASS
365	198	1	100	2.0	338	PASS
441	442	0.01	24	16.9	1889	PASS
442	198	50	100	67.5	11147	PASS
443	442	15	24	18.5	2066	PASS