

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091616\
 Data File : BF090111.D
 Acq On : 16 Sep 2016 17:32
 Operator : UM/SJ
 Sample : H4813-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-1-6-7

Quant Time: Sep 16 22:57:12 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 15 11:18:43 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.54	152	169793	20.00	ng	-0.01
21) Naphthalene-d8	7.83	136	720047	20.00	ng	-0.01
38) Acenaphthene-d10	9.56	164	358639	20.00	ng	-0.02
63) Phenanthrene-d10	11.04	188	587040	20.00	ng	-0.01
75) Chrysene-d12	13.65	240	445662	20.00	ng	-0.02
86) Perylene-d12	14.97	264	355276	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.12	112	1284133	121.63	ng	0.00
7) Phenol-d6	6.19	99	1487368	107.61	ng	-0.01
23) Nitrobenzene-d5	7.11	82	912726	71.27	ng	-0.02
41) 2,4,6-Tribromophenol	10.35	330	301849	83.79	ng	-0.02
44) 2-Fluorobiphenyl	8.91	172	1598839	70.01	ng	-0.01
78) Terphenyl-d14	12.63	244	1309293	69.77	ng	-0.01
Target Compounds						
4) n-Nitrosodimethylamine	2.67	42	1323	3.37	ng	# 1
19) n-Nitroso-di-n-propylamine	7.11	70	109007	12.69	ng	# 79
49) Dimethylphthalate	9.30	163	392931	14.75	ng	98
56) 2,4-Dinitrotoluene	9.56	165	46414	6.40	ng	# 15
66) 4-Bromophenyl-phenylether	10.35	248	17308	3.06	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091616\
Data File : BF090111.D
Acq On : 16 Sep 2016 17:32
Operator : UM/SJ
Sample : H4813-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-1-6-7

Quant Time: Sep 16 22:57:12 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 15 11:18:43 2016
Response via : Initial Calibration

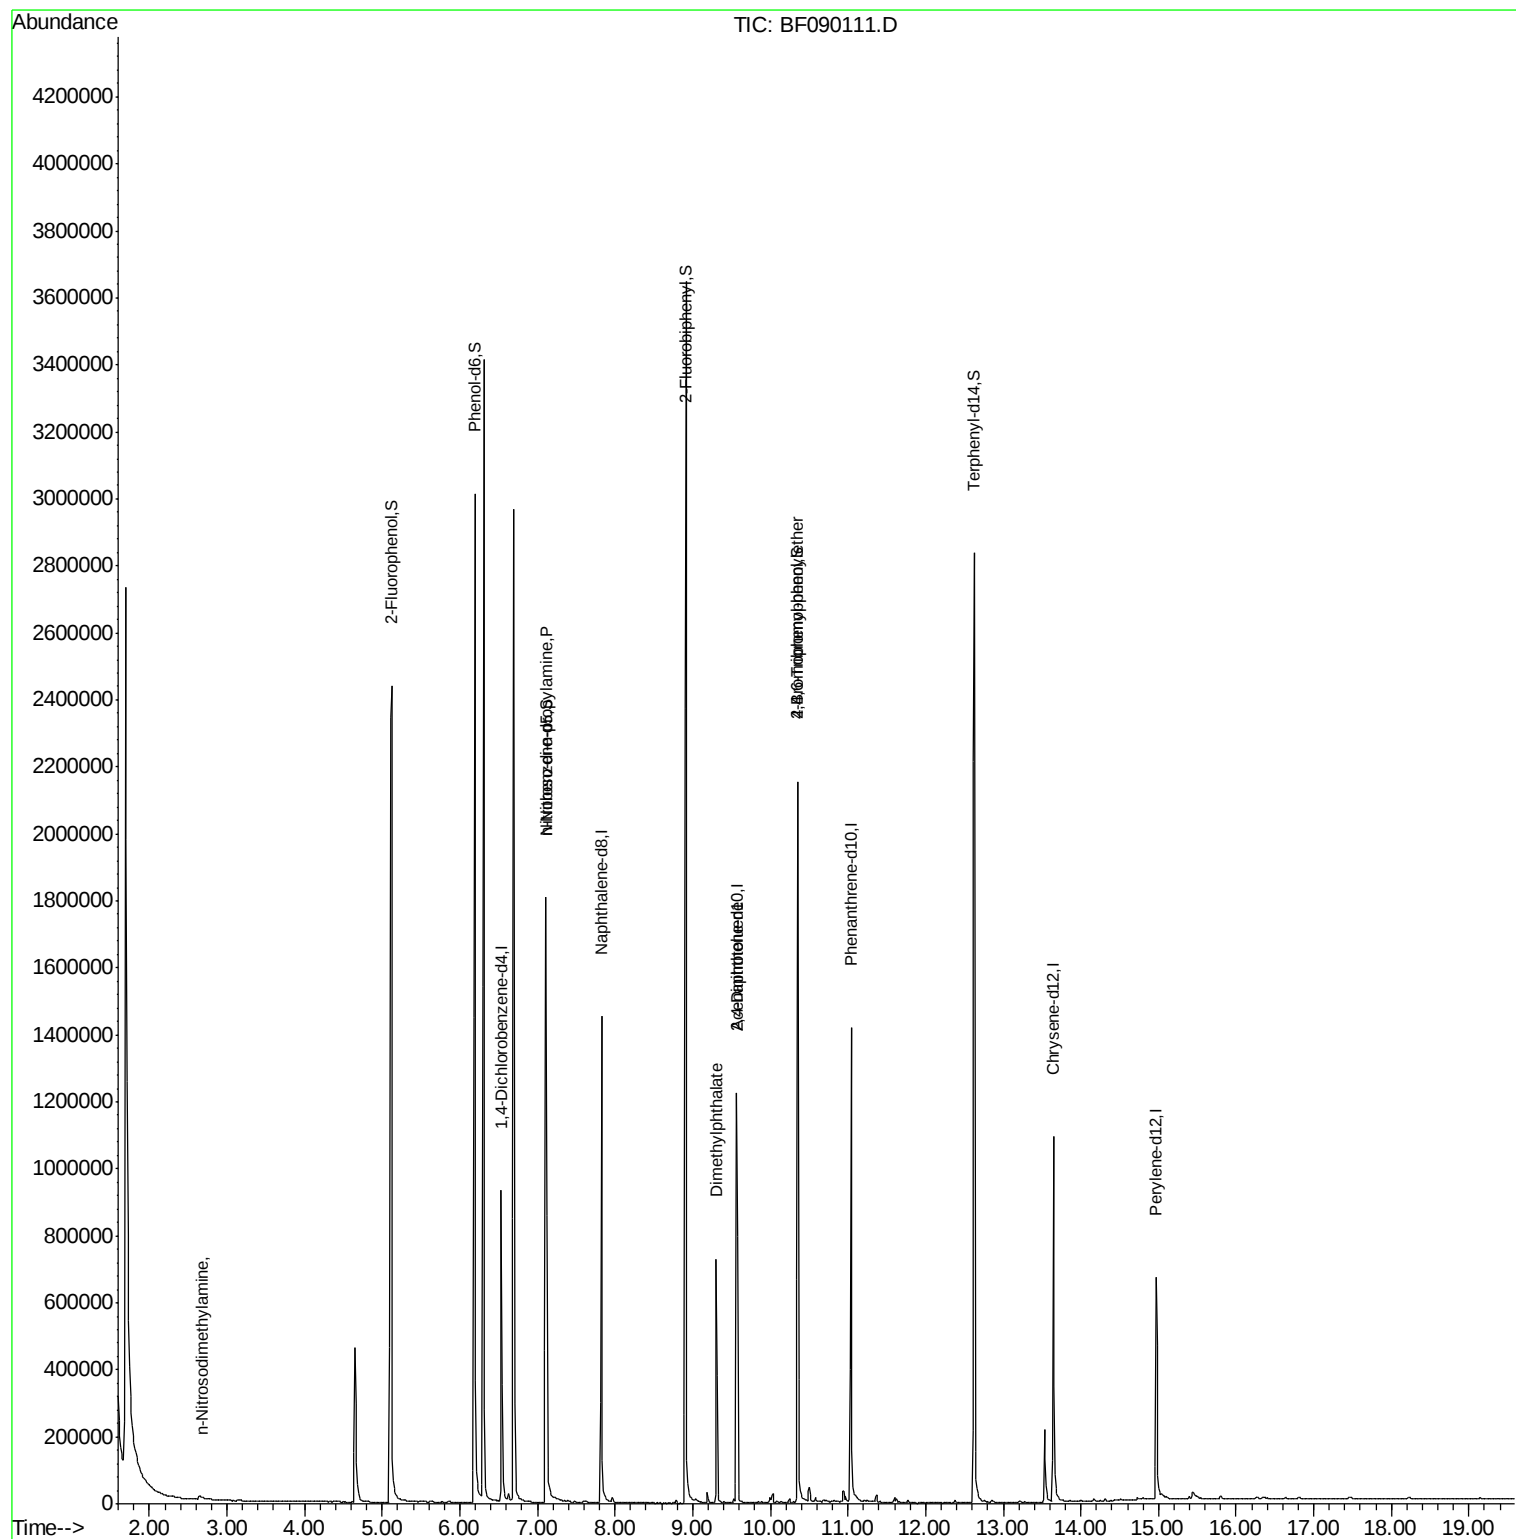

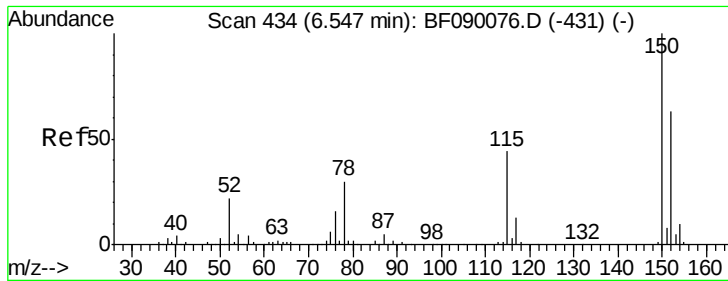

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.54 min Scan# 433

Delta R.T. -0.01 min

Lab File: BF090111.D

Acq: 16 Sep 2016 17:32

Instrument :

BNA_F

ClientSampleId :

SB-1-6-7


Tgt Ion:152 Resp: 169793

Ion Ratio Lower Upper

152 100

150 159.8 128.9 193.3




115 68.5 55.5 83.3

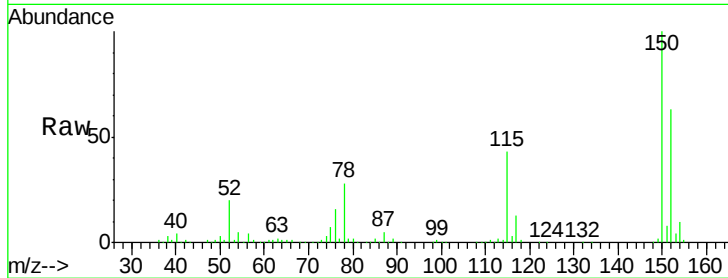

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

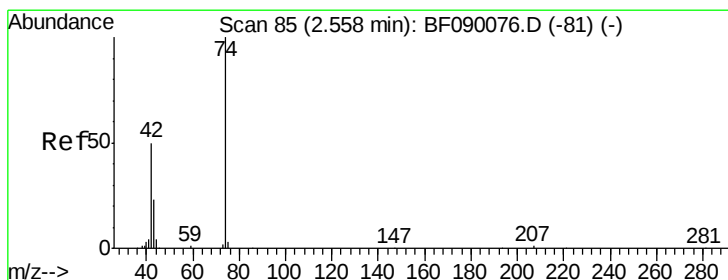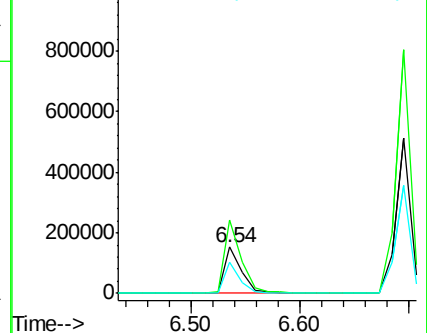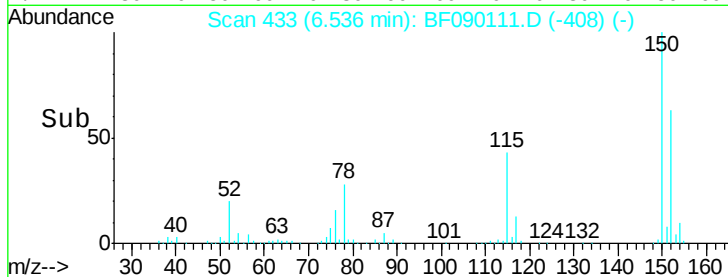

#4

n-Nitrosodimethylamine

Concen: 3.37 ng

RT: 2.67 min Scan# 95

Delta R.T. 0.11 min

Lab File: BF090111.D

Acq: 16 Sep 2016 17:32


Tgt Ion: 42 Resp: 1323

Ion Ratio Lower Upper

42 100

74 0.0 158.7 238.1#



44 97.5 6.4 9.6#

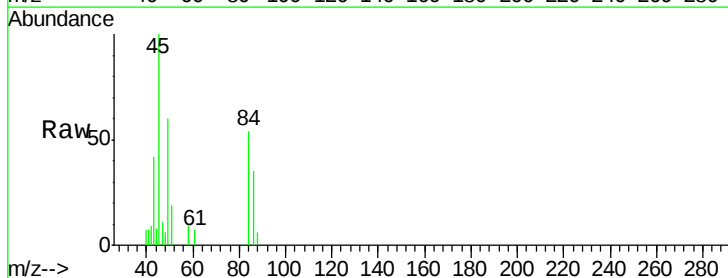


Abundance Ion 42.00 (41.70 to 42.70): BF0

Ion 74.00 (73.70 to 74.70): BF0

Ion 44.00 (43.70 to 44.70): BF0

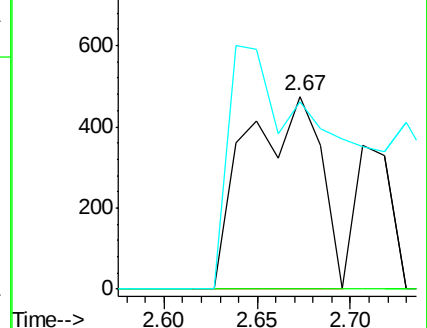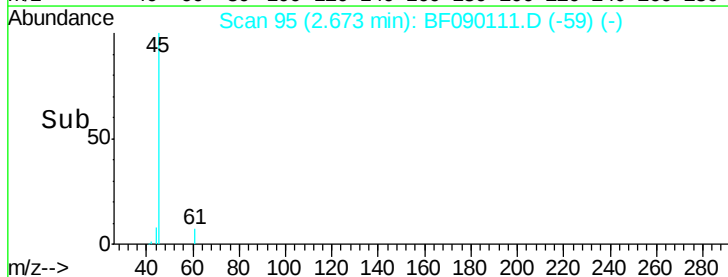

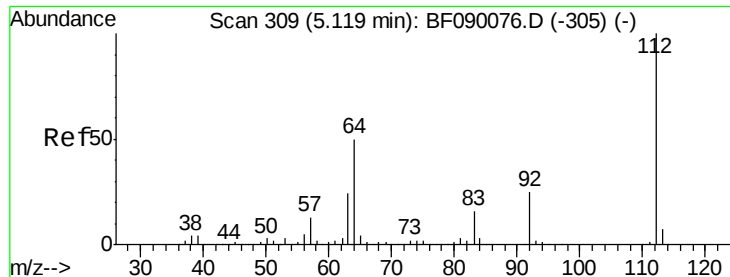

#5

2-Fluorophenol

Concen: 121.63 ng

RT: 5.12 min Scan# 309

Delta R.T. -0.00 min

Lab File: BF090111.D

Acq: 16 Sep 2016 17:32

Instrument :

BNA_F

ClientSampleId :

SB-1-6-7


Tgt Ion: 112 Resp: 1284133

Ion Ratio Lower Upper

112 100

64 45.2 39.8 59.6




63 21.5 18.9 28.3

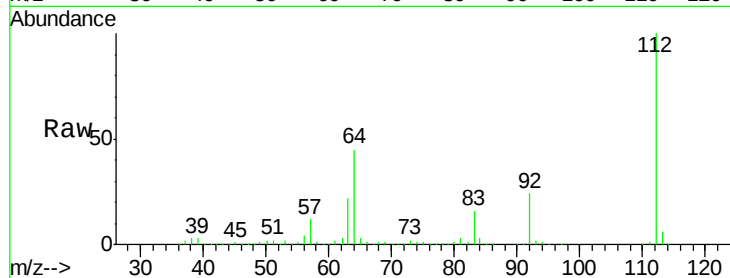

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

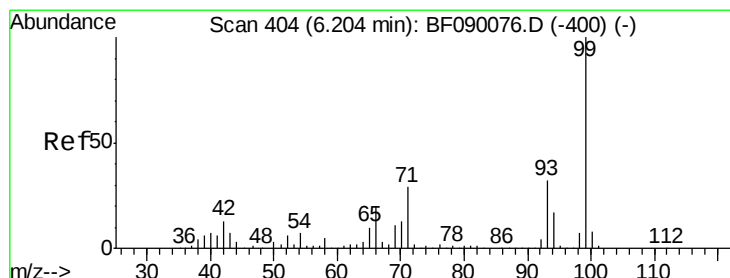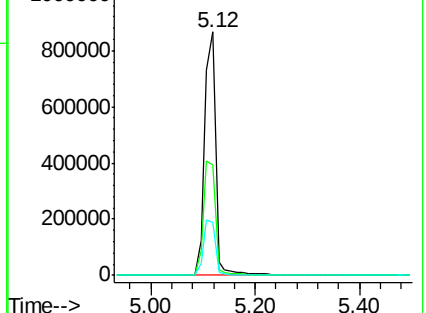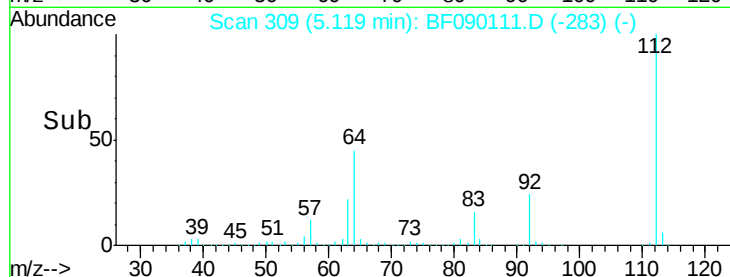

#7

Phenol-d6

Concen: 107.61 ng

RT: 6.19 min Scan# 403

Delta R.T. -0.01 min

Lab File: BF090111.D

Acq: 16 Sep 2016 17:32


Tgt Ion: 99 Resp: 1487368

Ion Ratio Lower Upper

99 100

42 12.6 10.6 15.8



71 29.3 23.0 34.6



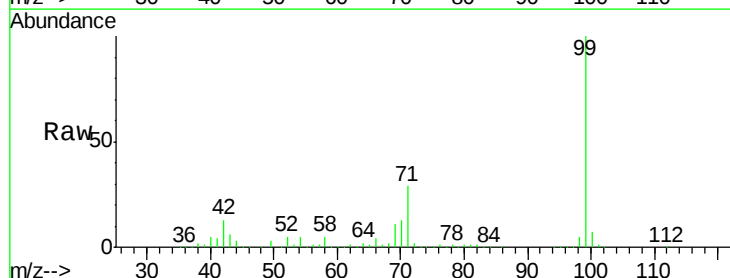


Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

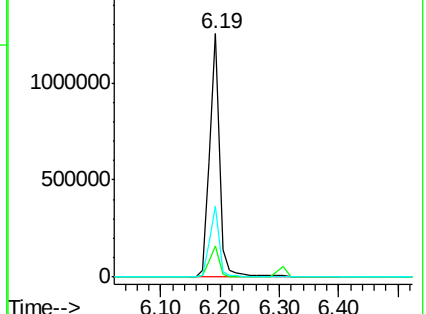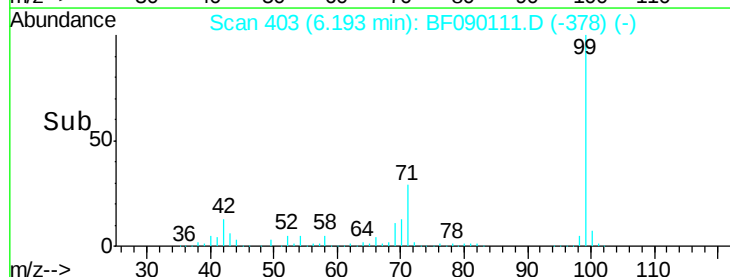

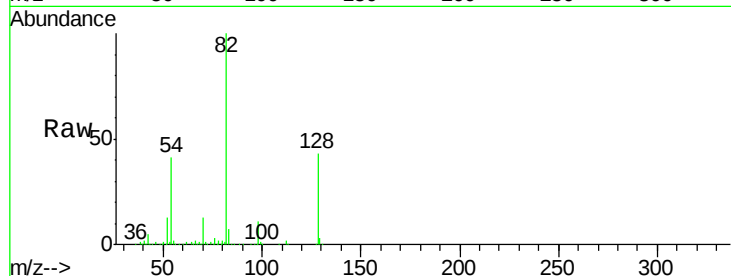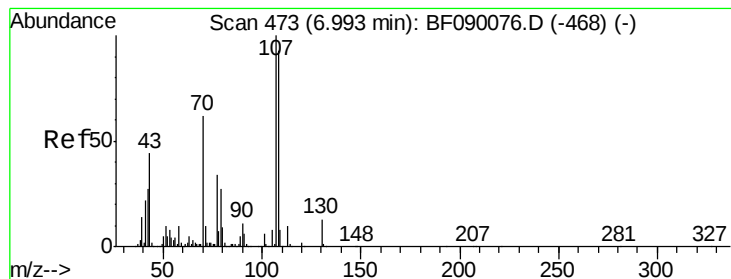

#19

n-Nitroso-di-n-propylamine

Concen: 12.69 ng

RT: 7.11 min Scan# 483

Delta R.T. 0.11 min

Lab File: BF090111.D

Acq: 16 Sep 2016 17:32

Instrument :

BNA_F

ClientSampleId :

SB-1-6-7

Tgt Ion: 70 Resp: 109007





Ion Ratio Lower Upper

70 100

42 36.5 35.1 52.7

101 0.0 7.5 11.3#

130 2.2 16.6 25.0#

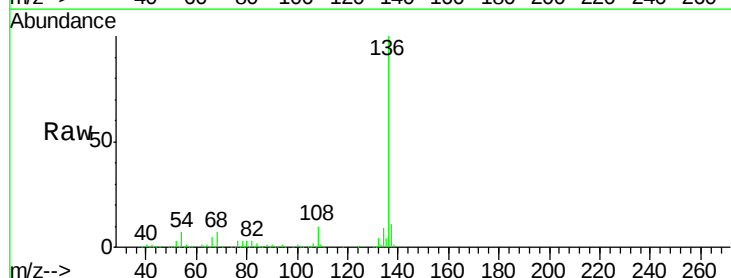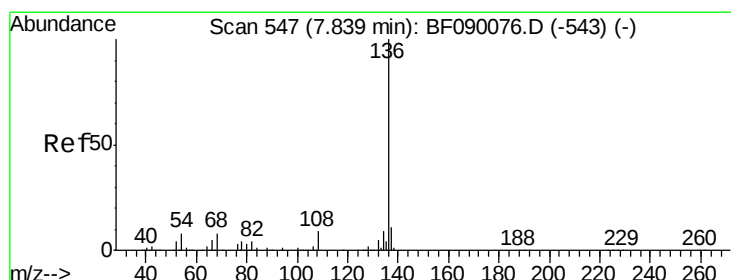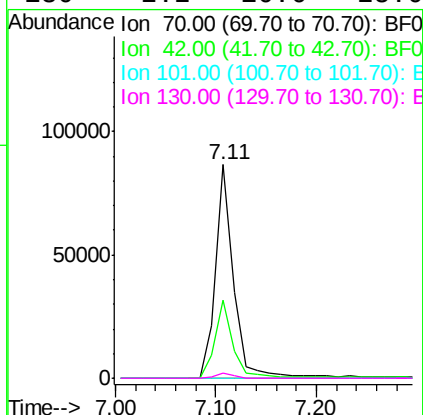

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.83 min Scan# 546

Delta R.T. -0.01 min

Lab File: BF090111.D

Acq: 16 Sep 2016 17:32

Tgt Ion: 136 Resp: 720047


Ion Ratio Lower Upper


136 100

137 11.0 9.0 13.4

54 6.6 6.4 9.6

68 6.7 6.3 9.5

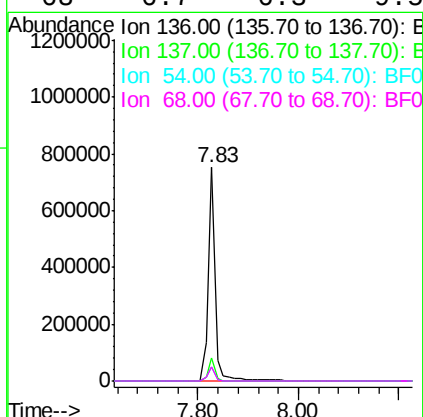

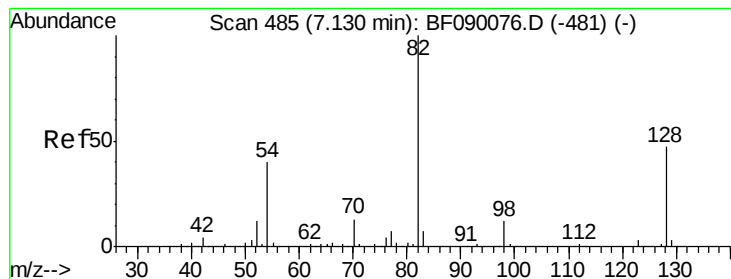

#23

Nitrobenzene-d5

Concen: 71.27 ng

RT: 7.11 min Scan# 483

Delta R.T. -0.02 min

Lab File: BF090111.D

Acq: 16 Sep 2016 17:32

Instrument :

BNA_F

ClientSampleId :

SB-1-6-7





Tgt Ion: 82 Resp: 912726

Ion Ratio Lower Upper

82 100

128 42.8 37.5 56.3

54 41.3 31.9 47.9

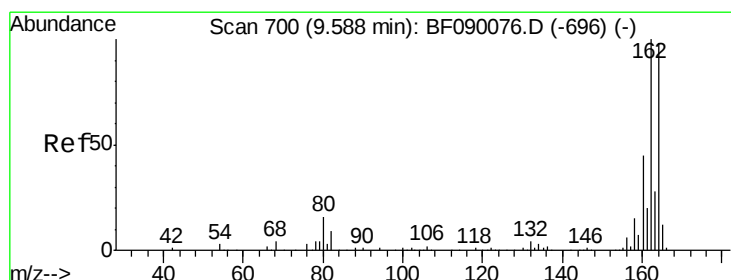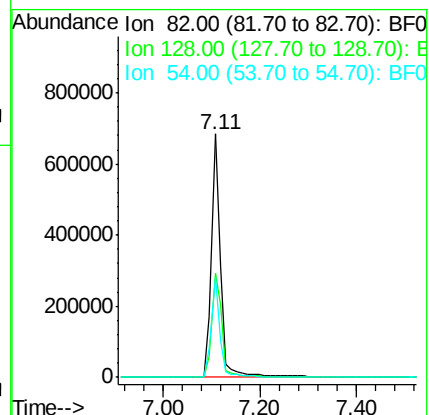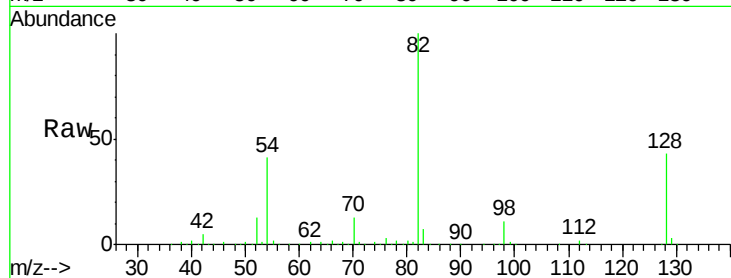

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.56 min Scan# 698

Delta R.T. -0.02 min

Lab File: BF090111.D

Acq: 16 Sep 2016 17:32




Tgt Ion: 164 Resp: 358639


Ion Ratio Lower Upper

164 100

162 100.0 81.4 122.2

160 44.0 36.6 54.8

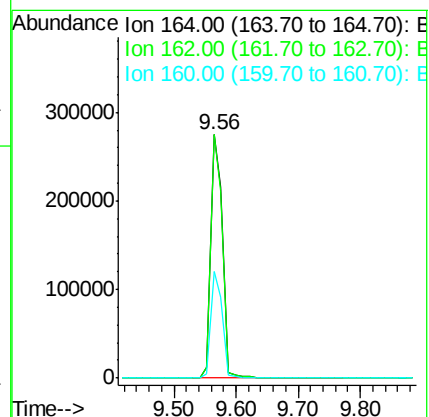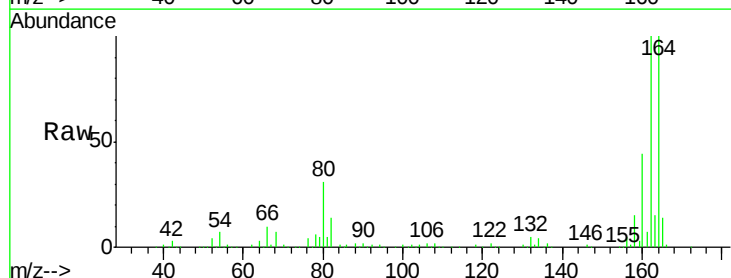


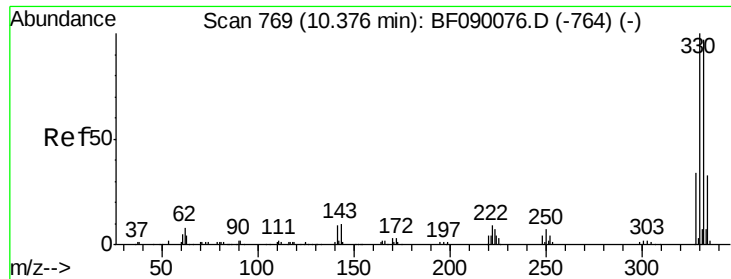




#41
 2,4,6-Tribromophenol
 Concen: 83.79 ng
 RT: 10.35 min Scan# 767
 Delta R.T. -0.02 min
 Lab File: BF090111.D
 Acq: 16 Sep 2016 17:32

Instrument :
 BNA_F
 ClientSampleId :
 SB-1-6-7

Tgt Ion:330 Resp: 301849
 Ion Ratio Lower Upper
 330 100
 332 97.1 78.1 117.1
 141 36.2 23.9 35.9#

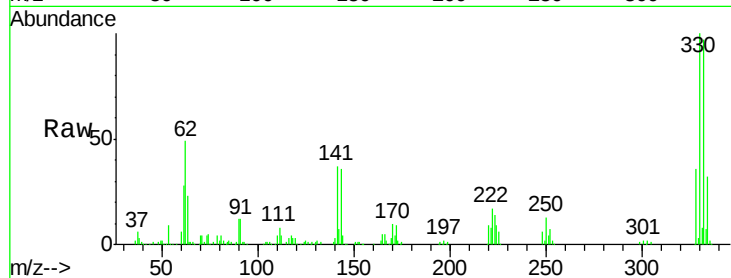


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

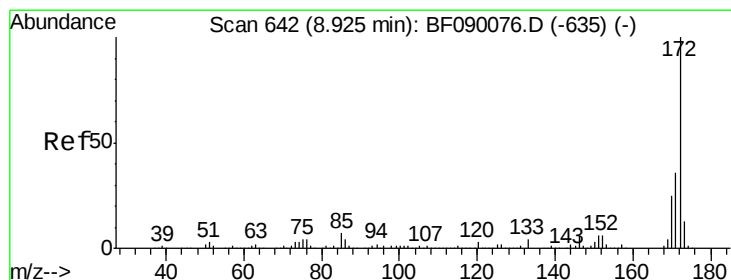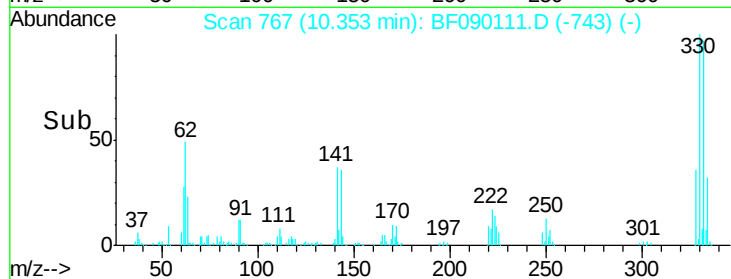
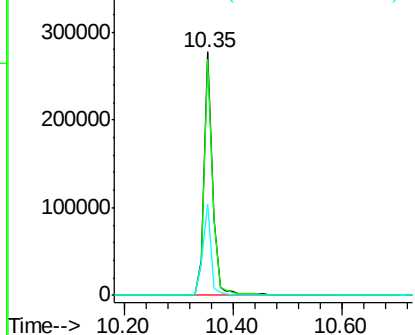



#44
 2-Fluorobiphenyl
 Concen: 70.01 ng
 RT: 8.91 min Scan# 641
 Delta R.T. -0.01 min
 Lab File: BF090111.D
 Acq: 16 Sep 2016 17:32

Tgt Ion:172 Resp: 1598839
 Ion Ratio Lower Upper
 172 100
 171 36.4 29.2 43.8
 170 25.0 19.8 29.8

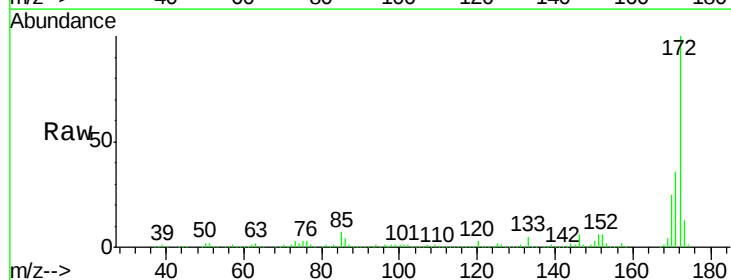

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

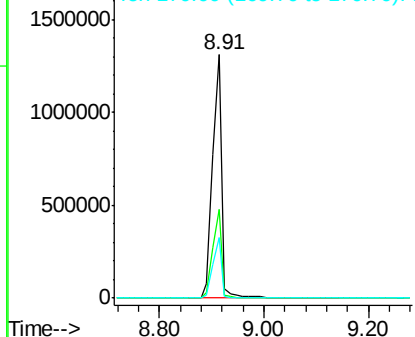

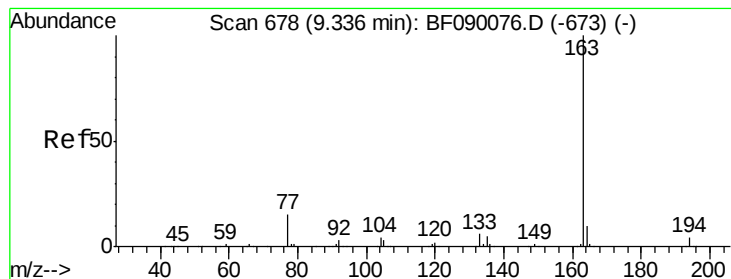

#49

Dimethylphthalate

Concen: 14.75 ng

RT: 9.30 min Scan# 675

Delta R.T. -0.03 min

Lab File: BF090111.D

Acq: 16 Sep 2016 17:32

Instrument :

BNA_F

ClientSampleId :

SB-1-6-7


Tgt Ion:163 Resp: 392931

Ion Ratio Lower Upper

163 100

194 2.8 2.8 4.2




164 10.7 8.1 12.1

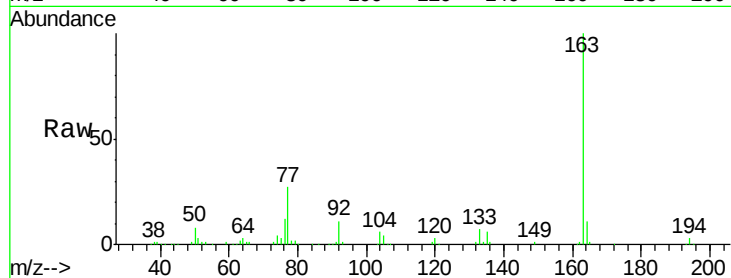

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

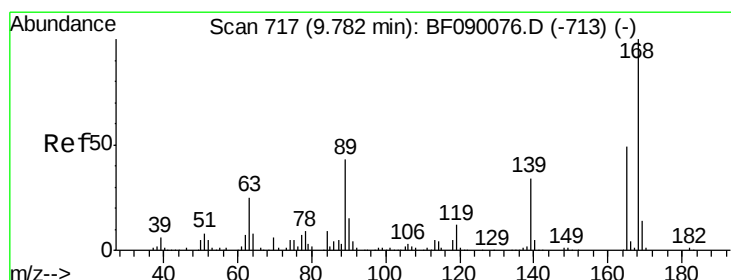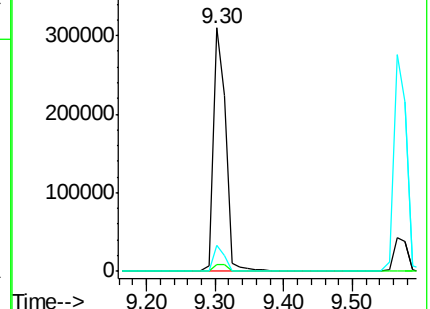

#56

2,4-Dinitrotoluene

Concen: 6.40 ng

RT: 9.56 min Scan# 698

Delta R.T. -0.22 min

Lab File: BF090111.D

Acq: 16 Sep 2016 17:32

Tgt Ion:165 Resp: 46414


Ion Ratio Lower Upper

165 100

63 0.0 44.4 66.6#

89 1.2 70.1 105.1#

182 0.0 1.7 2.5#


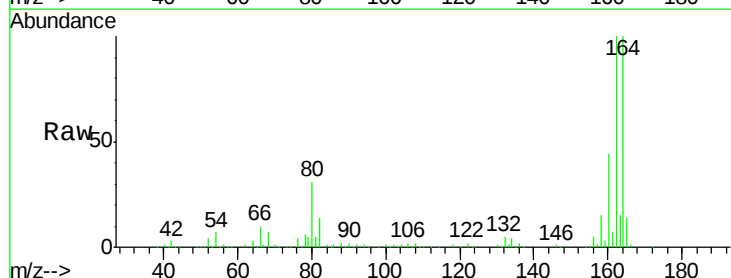



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E



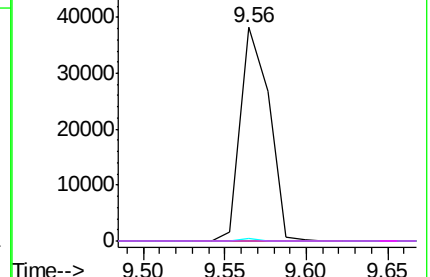



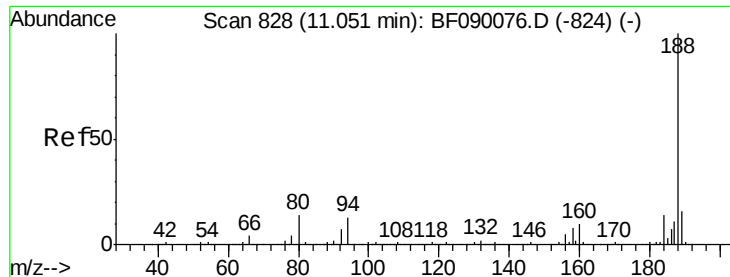

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.04 min Scan# 827
Delta R.T. -0.01 min
Lab File: BF090111.D
Acq: 16 Sep 2016 17:32




Instrument :
BNA_F
ClientSampleId :
SB-1-6-7


Tgt Ion:188 Resp: 587040
Ion Ratio Lower Upper
188 100
94 10.9 10.5 15.7
80 11.1 11.2 16.8#

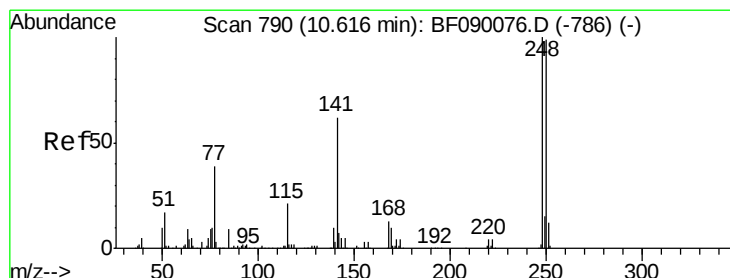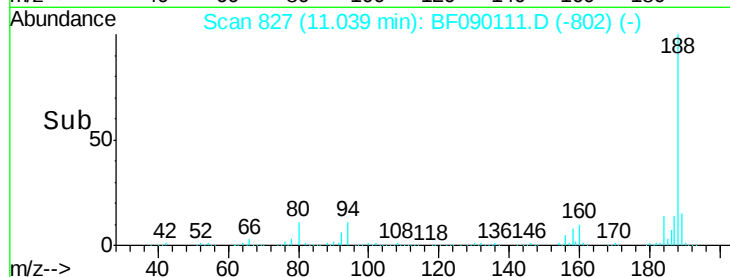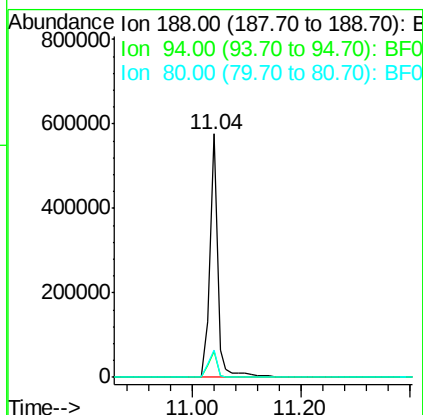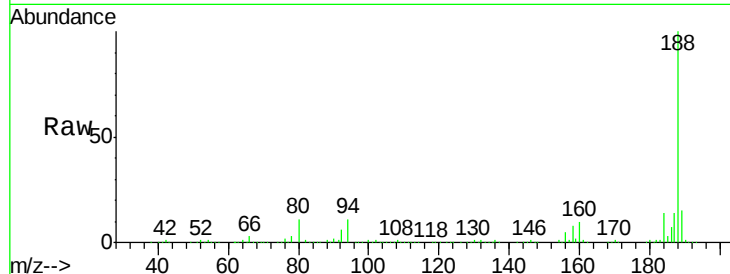

#66
4-Bromophenyl-phenylether
Concen: 3.06 ng
RT: 10.35 min Scan# 767
Delta R.T. -0.26 min
Lab File: BF090111.D
Acq: 16 Sep 2016 17:32

Tgt Ion:248 Resp: 17308
Ion Ratio Lower Upper
248 100
250 201.0 79.4 119.2#
141 581.8 49.3 73.9#

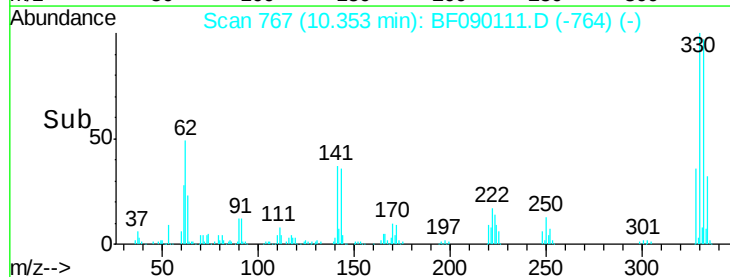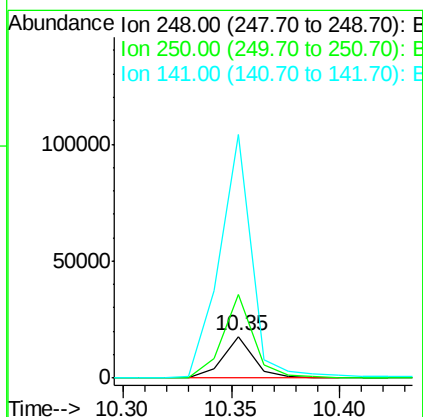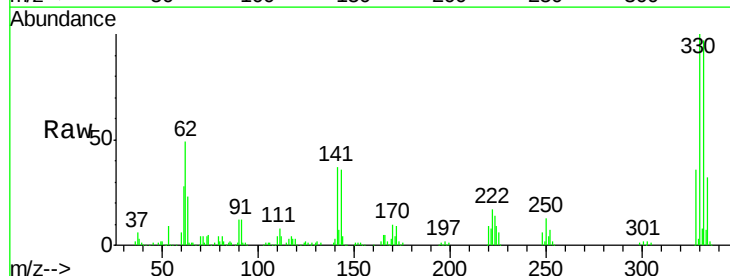



#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.65 min Scan# 1055

Delta R.T. -0.02 min

Lab File: BF090111.D

Acq: 16 Sep 2016 17:32

Instrument :

BNA_F

ClientSampleId :

SB-1-6-7


Tgt Ion:240 Resp: 445662

Ion Ratio Lower Upper

240 100

120 17.7 10.6 16.0#




236 26.2 21.6 32.4

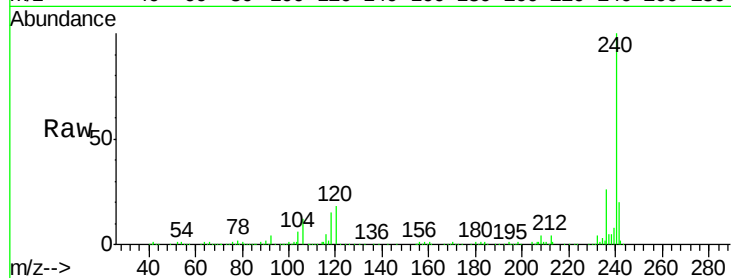

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

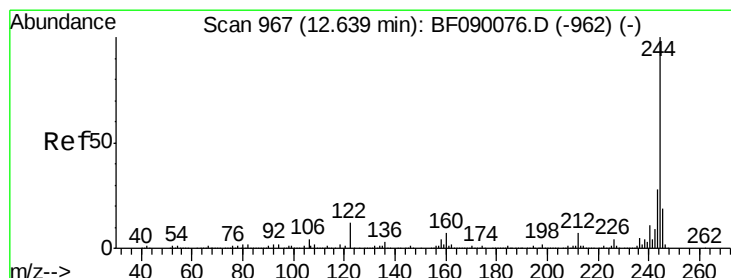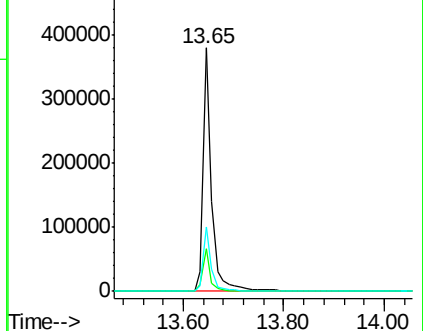

#78

Terphenyl-d14

Concen: 69.77 ng

RT: 12.63 min Scan# 966

Delta R.T. -0.01 min

Lab File: BF090111.D

Acq: 16 Sep 2016 17:32


Tgt Ion:244 Resp: 1309293

Ion Ratio Lower Upper

244 100

212 6.8 5.8 8.8



122 10.4 9.4 14.0



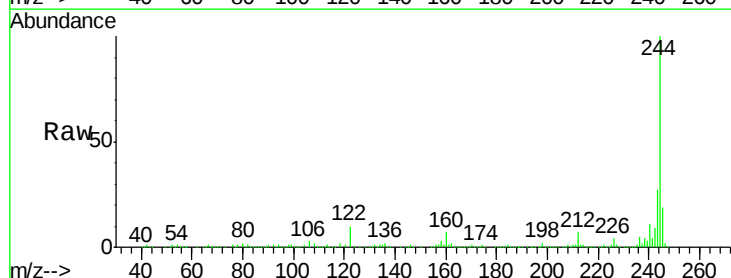


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

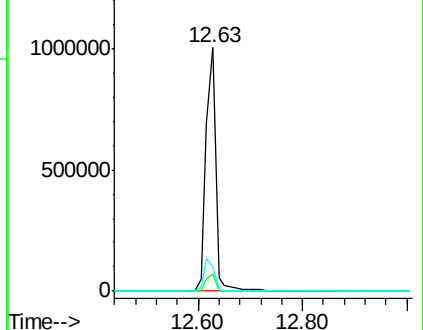

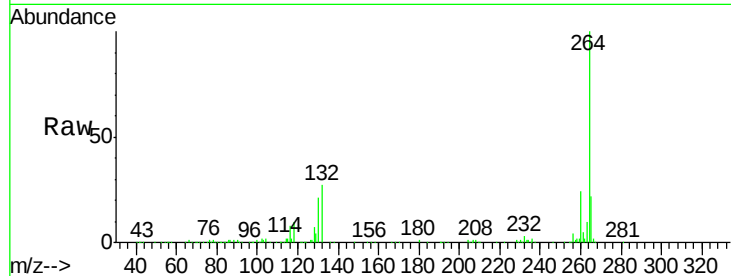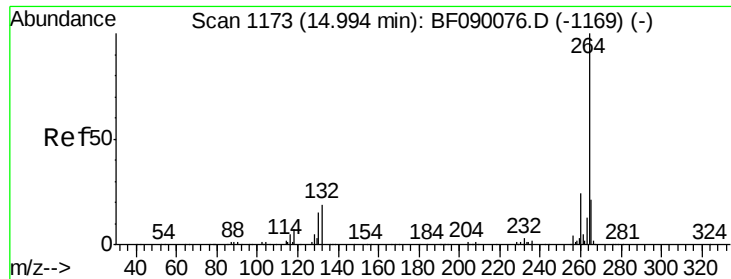

#86
Perylene-d12
Concen: 20.00 ng
RT: 14.97 min Scan# 1171
Delta R.T. -0.02 min
Lab File: BF090111.D
Acq: 16 Sep 2016 17:32

Instrument :
BNA_F
ClientSampleId :
SB-1-6-7

Tgt Ion:	264	Resp:	355276
Ion	Ratio	Lower	Upper
264	100		
260	24.0	19.5	29.3
265	21.7	17.0	25.4

