
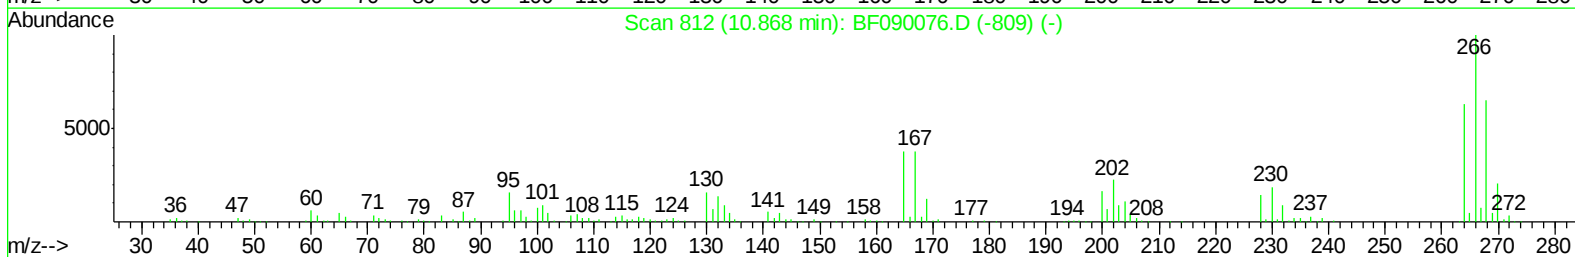
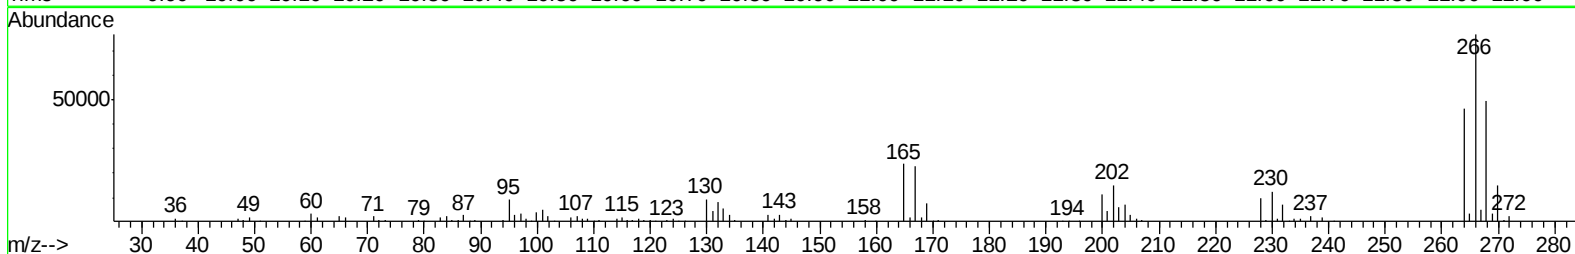


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091616\
Data File : BF090101.D
Acq On : 16 Sep 2016 10:39
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 23:54:24 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 15 11:18:43 2016
Response via : Initial Calibration

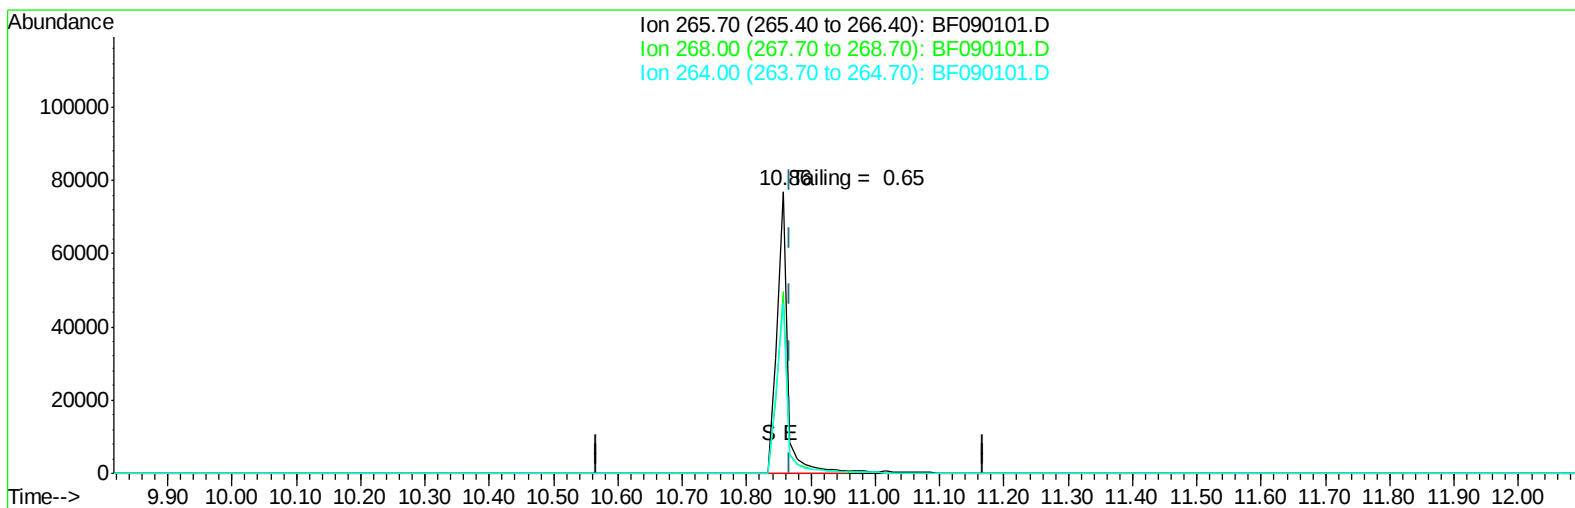

TIC: BF090101.D

(69) Pentachlorophenol (C)




10.856min (-0.011) 44298.29ng

response 92562

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	64.43
264.00	62.90	60.42
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091616\
Data File : BF090101.D
Acq On : 16 Sep 2016 10:39
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 23:54:24 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 15 11:18:43 2016
Response via : Initial Calibration

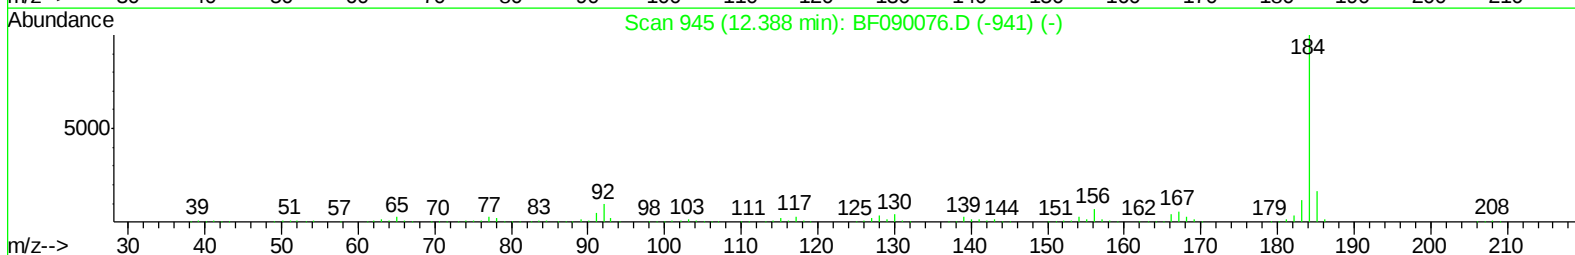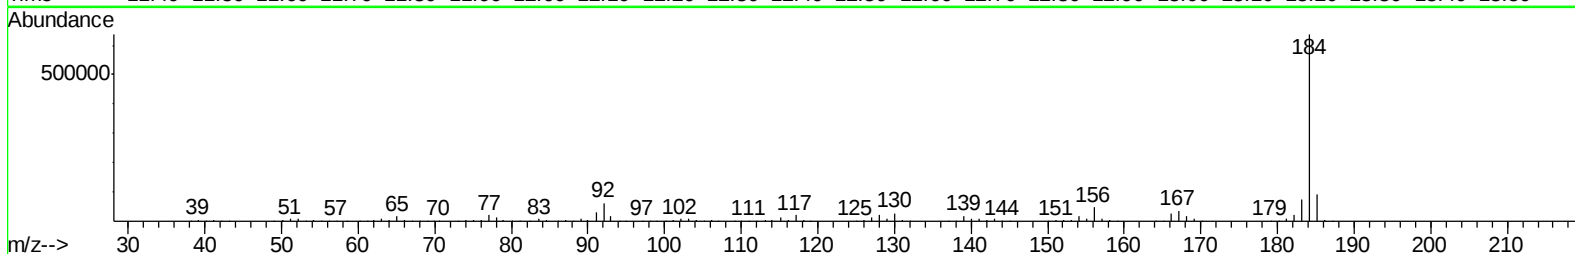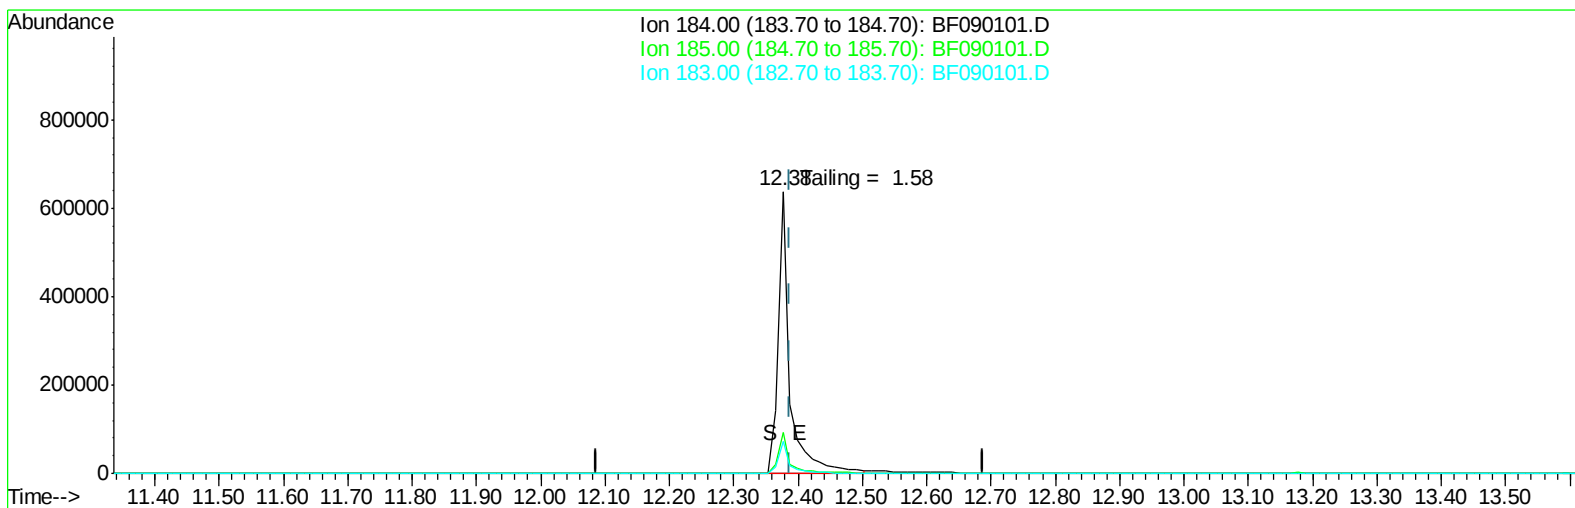

TIC: BF090101.D

(76) Benzidine

12.376min (-0.011) 23660.85ng

response 838712

Ion	Exp%	Act%
184.00	100	100
185.00	16.50	14.35
183.00	11.50	11.37
0.00	0.00	0.00