


Data Path : Z:\HPCHEM1\BNA F\DATA\BF091616\
 Data File : BF090101.D
 Acq On : 16 Sep 2016 10:39
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 15 11:18:43 2016

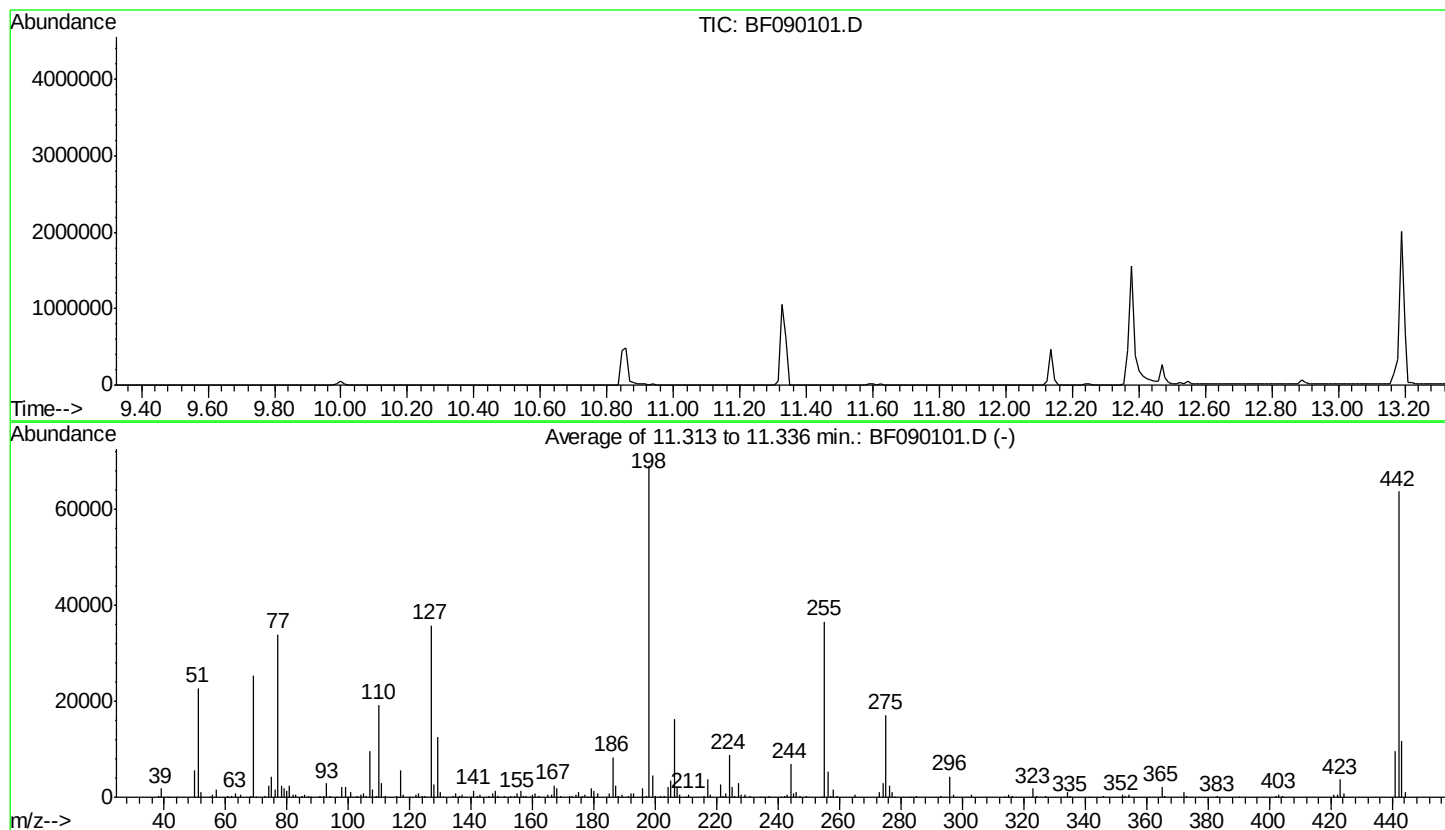

AutoFind: Scans 851, 852, 853; Background Corrected with Scan 848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	22712	PASS
68	69	0.00	2	1.2	311	PASS
69	198	0.00	100	36.6	25271	PASS
70	69	0.00	2	0.5	126	PASS
127	198	10	80	51.9	35760	PASS
197	198	0.00	2	0.5	361	PASS
198	198	100	100	100.0	68966	PASS
199	198	5	9	6.6	4524	PASS
275	198	10	60	24.7	17047	PASS
365	198	1	100	3.2	2192	PASS
441	442	0.01	24	15.2	9673	PASS
442	198	50	100	92.2	63608	PASS
443	442	15	24	18.4	11723	PASS