
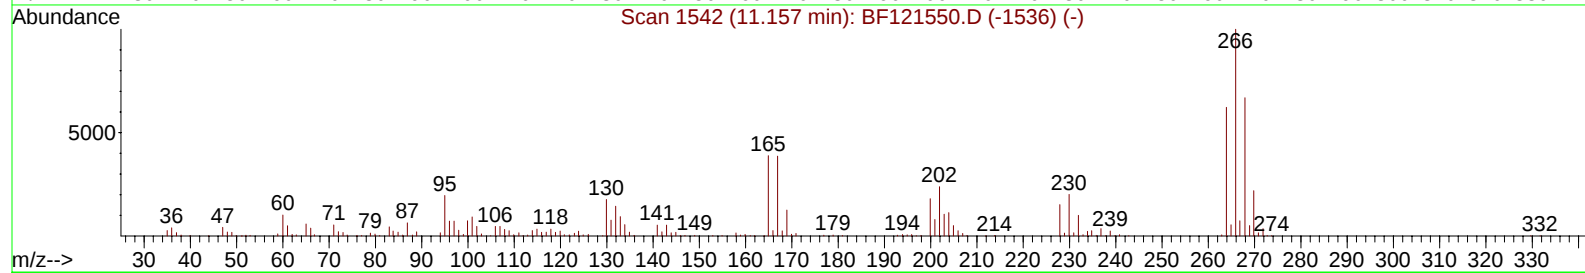
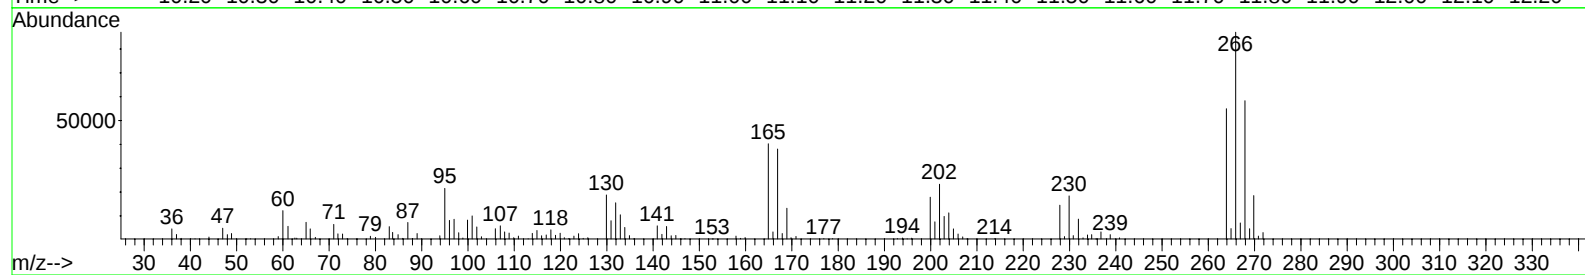


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091620\
 Data File : BF121588.D
 Acq On : 16 Sep 2020 10:06
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 15:56:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 10 16:47:54 2020
 Response via : Initial Calibration

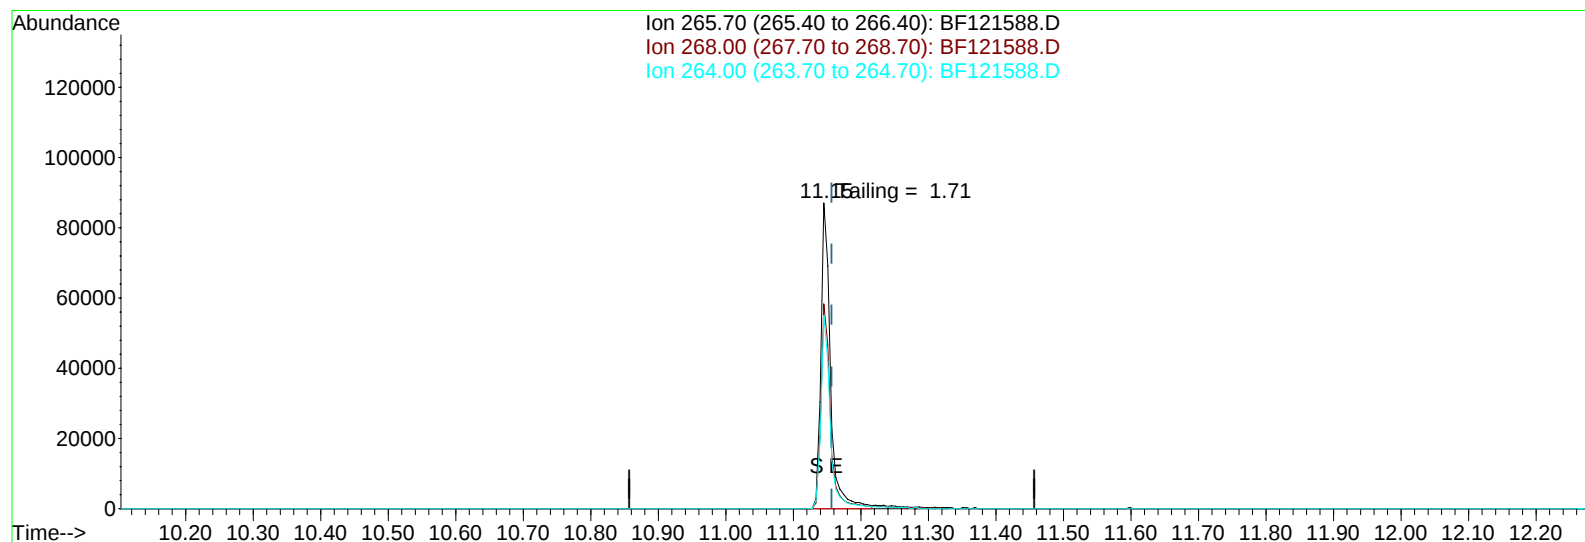

TIC: BF121588.D

(70) Pentachlorophenol (C)




11.145min (-0.012) 38926.69ng

response 88173

Ion	Exp%	Act%
265.70	100	100
268.00	66.90	67.01
264.00	62.30	63.17
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091620\
 Data File : BF121588.D
 Acq On : 16 Sep 2020 10:06
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 15:56:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 10 16:47:54 2020
 Response via : Initial Calibration

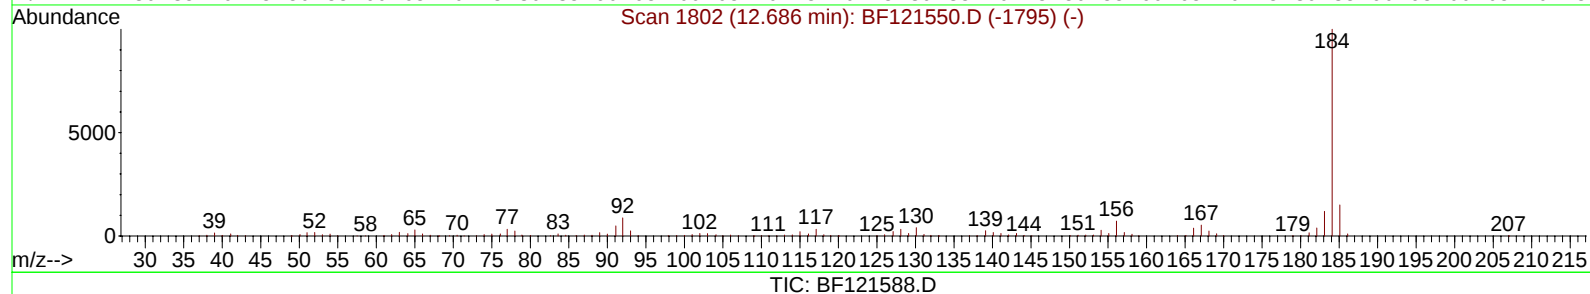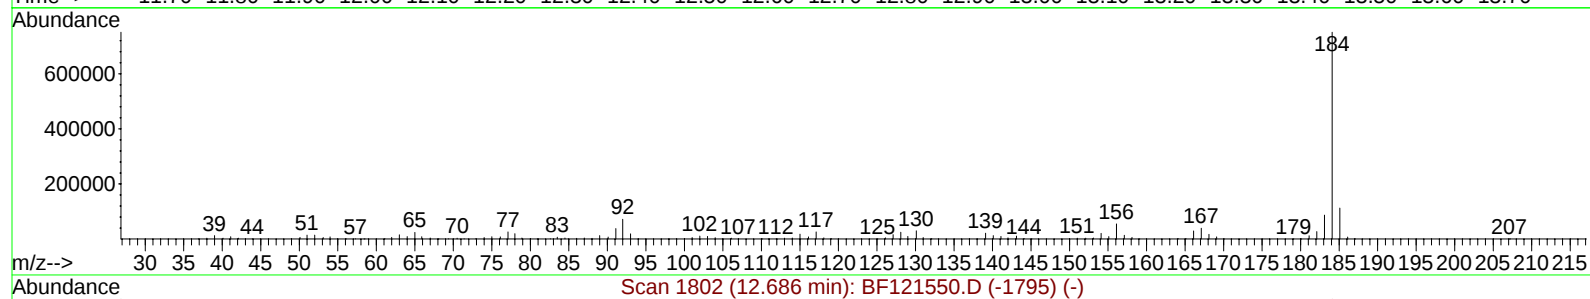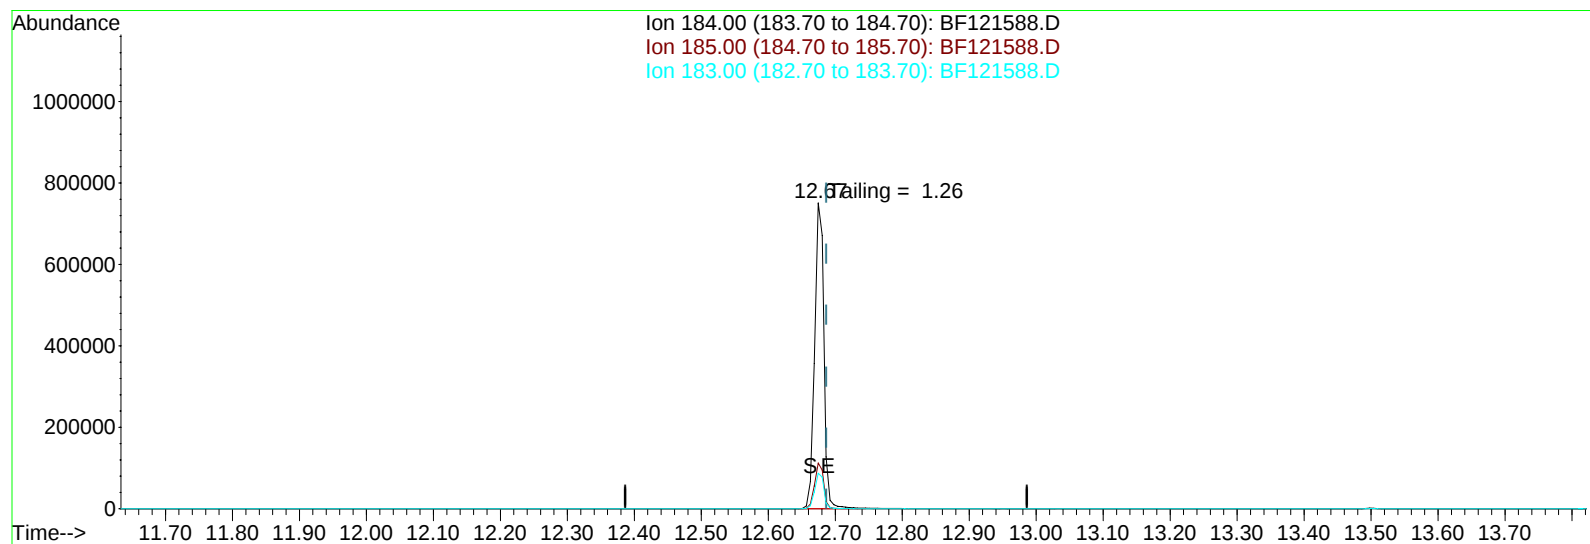

(77) Benzidine

12.674min (-0.012) 0.00ng

response 722464

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.97
183.00	11.90	11.61
0.00	0.00	0.00