

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF091620\
 Data File : BF121592.D
 Acq On : 16 Sep 2020 12:30
 Operator : JU/CG
 Sample : L4009-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HAYES-SEYMOUR-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.128	4	7	44	rVB	303486	973007	24.25%	2.970%
2	5.045	498	503	509	rBV	78196	101429	2.53%	0.310%
3	5.451	567	572	575	rBV	3512412	3289153	81.96%	10.038%
4	5.710	611	616	622	rBV	38660	42385	1.06%	0.129%
5	6.357	722	726	734	rBV	120422	159248	3.97%	0.486%
6	6.463	739	744	755	rVB	3093799	3559376	88.69%	10.863%
7	6.651	773	776	787	rBV	108221	100156	2.50%	0.306%
8	6.822	801	805	808	rBV	1306238	1033383	25.75%	3.154%
9	7.380	895	900	904	rBV	2217422	2374671	59.17%	7.247%
10	8.104	1018	1023	1026	rBV	1558444	1380204	34.39%	4.212%
11	8.251	1042	1048	1063	rBV	259869	419552	10.45%	1.280%
12	9.180	1200	1206	1209	rBV	4276572	4013085	100.00%	12.247%
13	9.569	1268	1272	1276	rBV	426200	361287	9.00%	1.103%
14	9.786	1302	1309	1315	rBV3	21682	48230	1.20%	0.147%
15	9.857	1315	1321	1324	rBV	1791887	1533158	38.20%	4.679%
16	10.645	1449	1455	1458	rBV	2672405	2349157	58.54%	7.169%
17	11.339	1568	1573	1576	rBV	1668965	1505110	37.51%	4.593%
18	11.868	1655	1663	1675	rBV	524032	570616	14.22%	1.741%
19	12.551	1771	1779	1782	rBV	135658	143040	3.56%	0.437%
20	12.651	1793	1796	1803	rBV2	123848	141475	3.53%	0.432%
21	12.774	1814	1817	1820	rVB	100392	95710	2.38%	0.292%
22	12.927	1838	1843	1846	rBV	4068306	3679379	91.68%	11.229%
23	13.145	1876	1880	1887	rBV3	34903	77051	1.92%	0.235%
24	13.774	1981	1987	1990	rBV3	28698	51767	1.29%	0.158%
25	13.827	1990	1996	2006	rVV3	548380	848894	21.15%	2.591%
26	13.974	2016	2021	2024	rBV	1291646	1143097	28.48%	3.489%
27	14.145	2047	2050	2056	rVB2	54526	68950	1.72%	0.210%
28	14.451	2097	2102	2103	rBV	103861	124641	3.11%	0.380%
29	14.751	2149	2153	2157	rBV	82065	97958	2.44%	0.299%
30	14.827	2160	2166	2171	rVV	567256	692891	17.27%	2.115%
31	14.898	2175	2178	2182	rVB	57265	59115	1.47%	0.180%
32	15.003	2193	2196	2199	rBV	46614	63029	1.57%	0.192%
33	15.086	2206	2210	2213	rBV	141286	152506	3.80%	0.465%
34	15.121	2213	2216	2222	rVB2	73648	106705	2.66%	0.326%

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF091620\
Data File : BF121592.D
Acq On : 16 Sep 2020 12:30
Operator : JU/CG
Sample : L4009-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HAYES-SEYMOUR-01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	15.362	2253	2257	2261	rVB	33253	41440	1.03%	0.126%
36	15.427	2263	2268	2272	rVV	734329	884070	22.03%	2.698%
37	15.462	2272	2274	2280	rVB	79368	83221	2.07%	0.254%
38	15.656	2304	2307	2311	rVB4	33561	41913	1.04%	0.128%
39	15.892	2342	2347	2352	rVB	110300	168472	4.20%	0.514%
40	15.956	2353	2358	2364	rBV3	62903	147391	3.67%	0.450%
41	16.662	2476	2478	2485	rVB8	22889	40705	1.01%	0.124%


Sum of corrected areas: 32766627

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF091620\
Data File : BF121592.D
Acq On : 16 Sep 2020 12:30
Operator : JU/CG
Sample : L4009-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HAYES-SEYMOUR-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

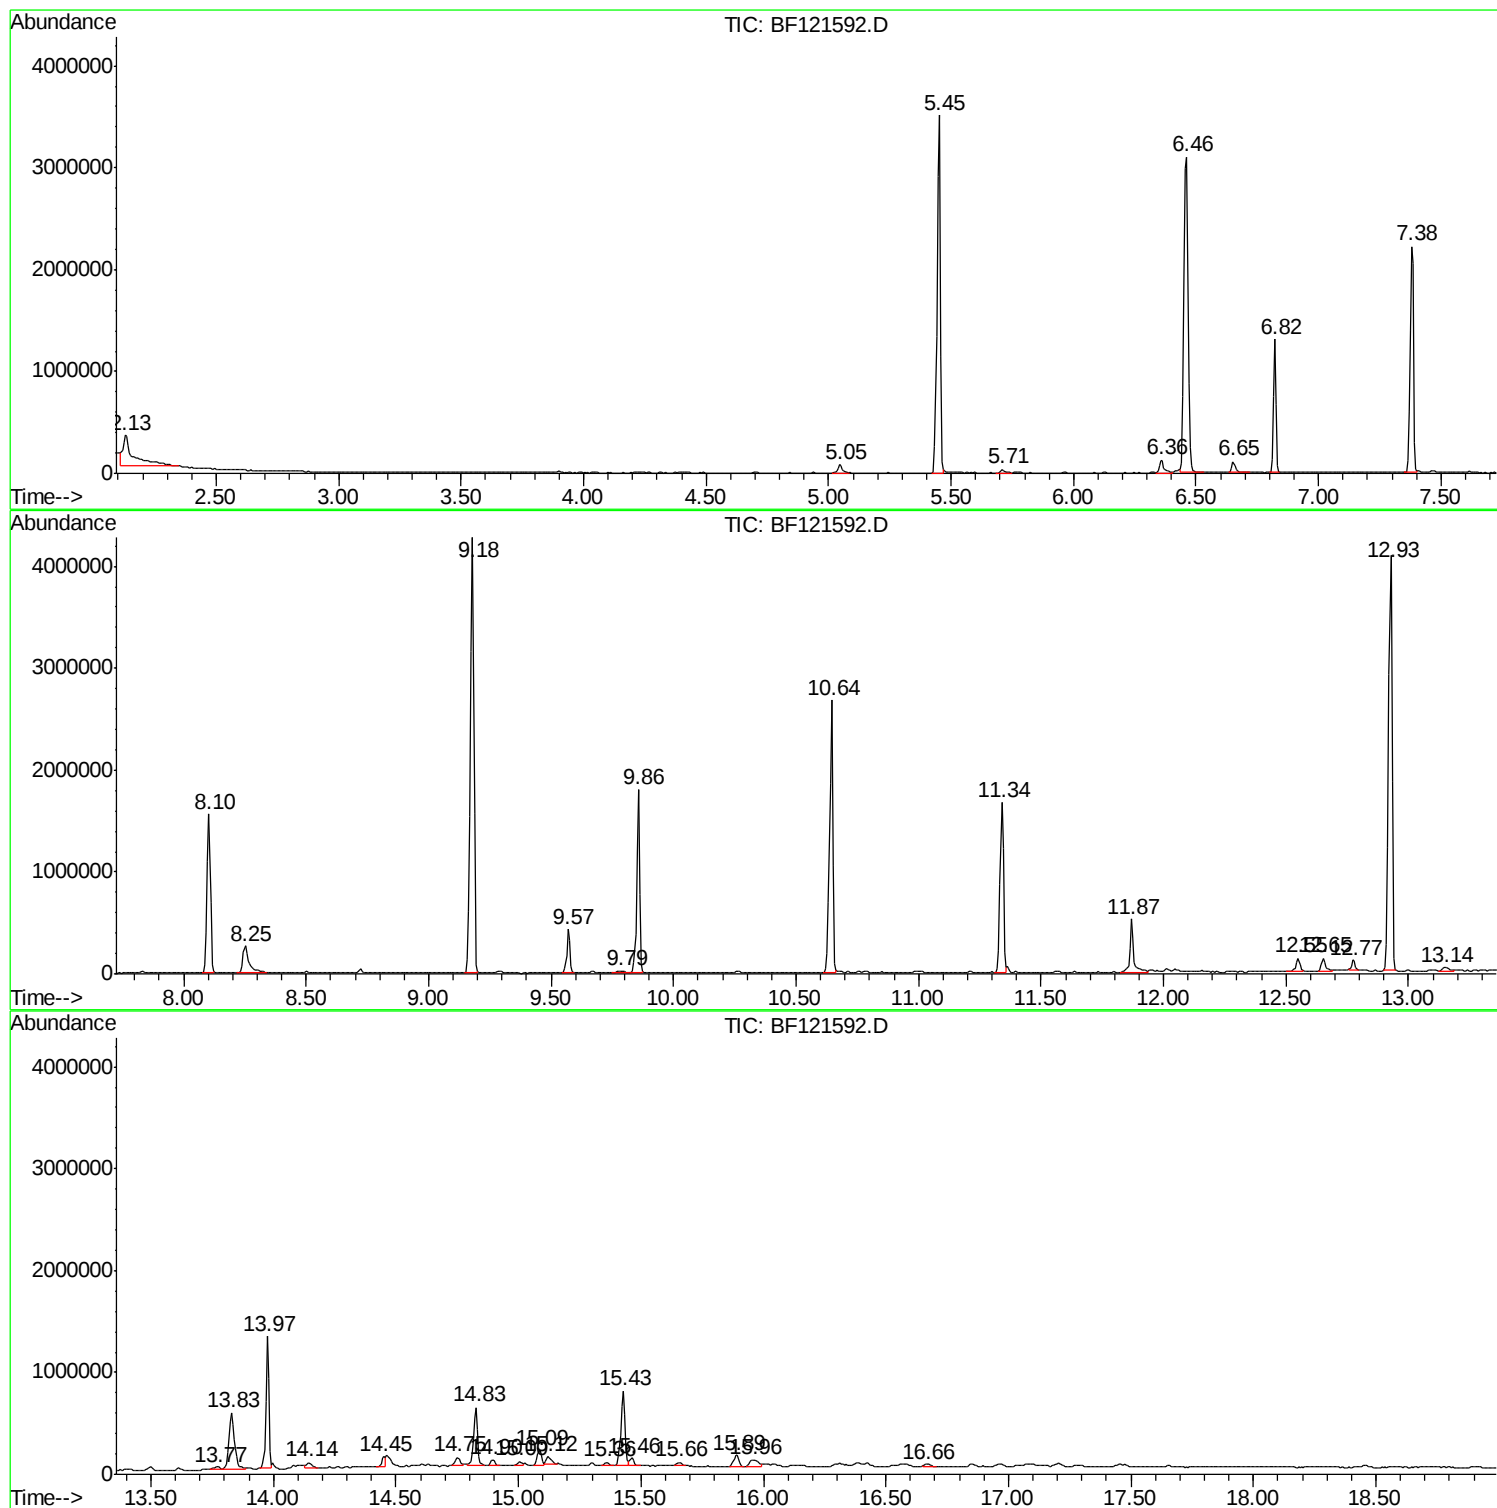

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091620\
Data File : BF121592.D
Acq On : 16 Sep 2020 12:30
Operator : JU/CG
Sample : L4009-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HAYES-SEYMOUR-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091620\
Data File : BF121592.D
Acq On : 16 Sep 2020 12:30
Operator : JU/CG
Sample : L4009-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HAYES-SEYMOUR-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc