
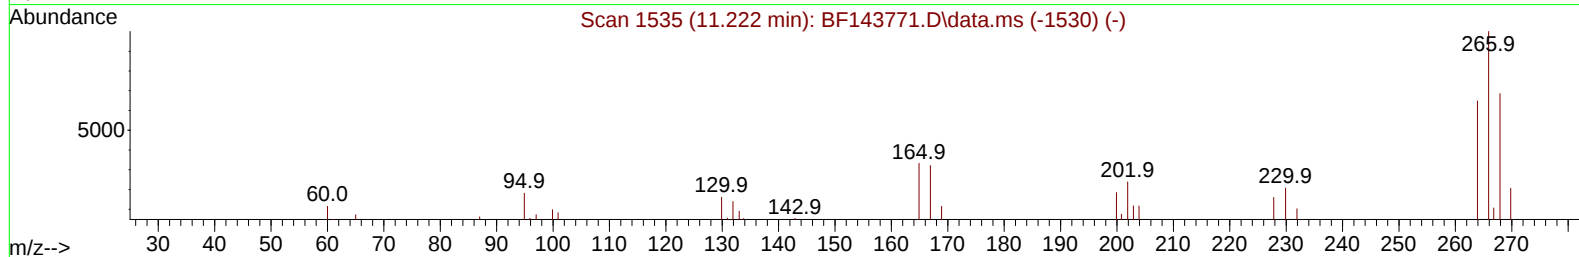
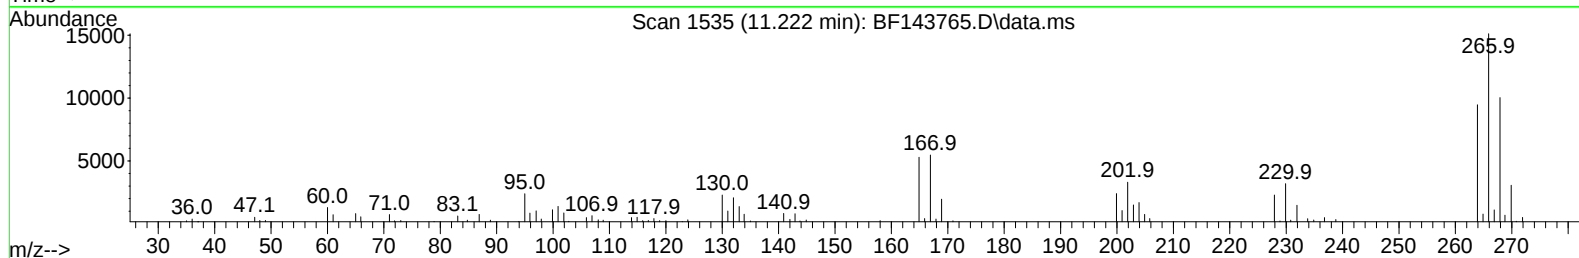


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091625\
Data File : BF143765.D
Acq On : 16 Sep 2025 10:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 13:41:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 09 15:20:16 2025
Response via : Initial Calibration

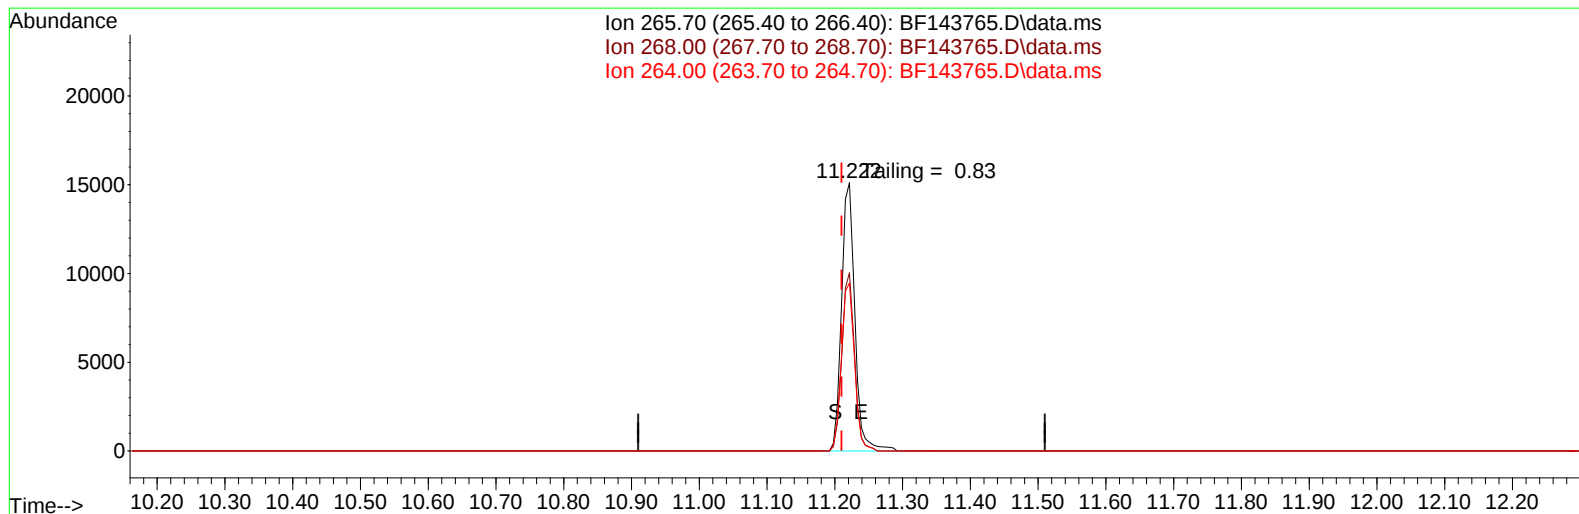

TIC: BF143765.D\data.ms

(70) Pentachlorophenol (C)




11.222min (+ 0.012) 0.00 ng

response 20593

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	66.43
264.00	60.80	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091625\
Data File : BF143765.D
Acq On : 16 Sep 2025 10:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 13:41:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 09 15:20:16 2025
Response via : Initial Calibration

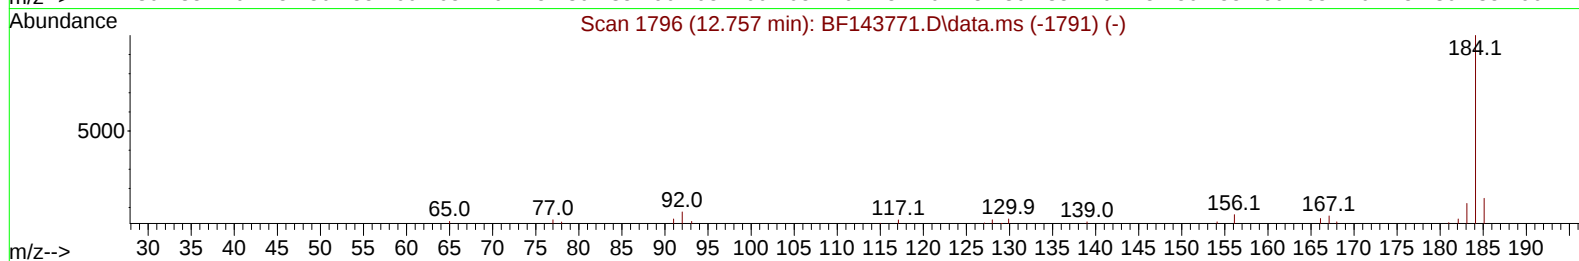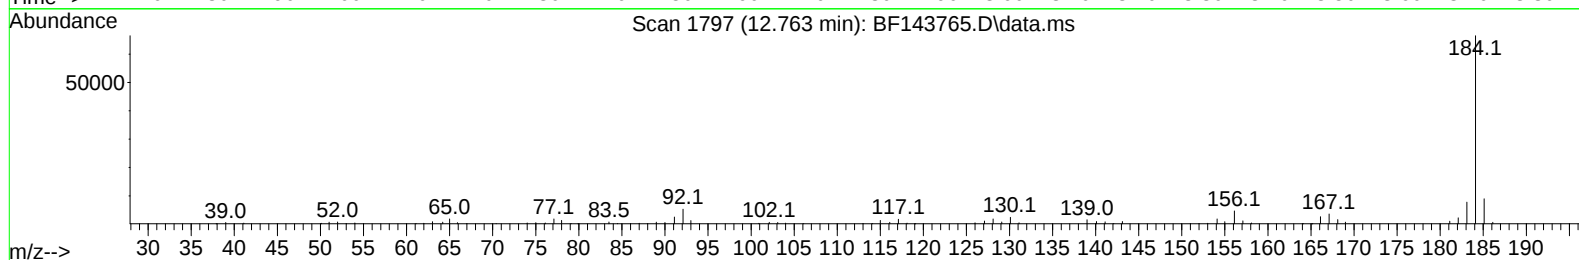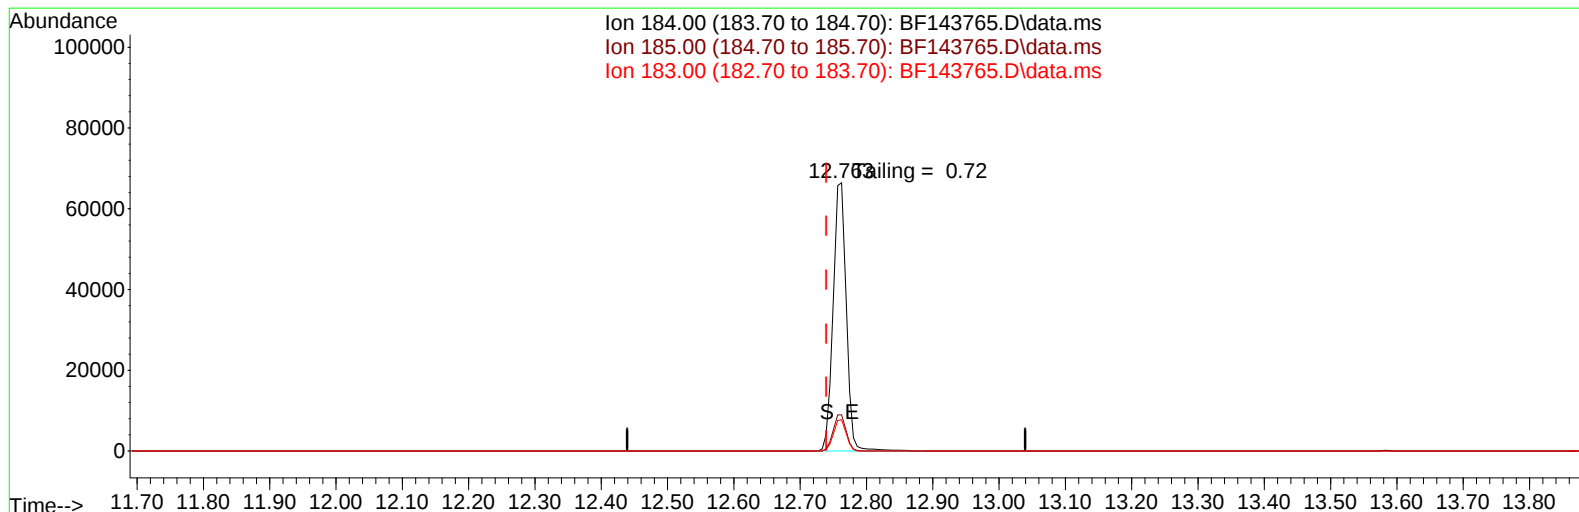

TIC: BF143765.D\data.ms

(77) Benzidine

12.763min (+ 0.023) 0.00 ng

response 91478

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.40	13.48
--------	-------	-------

183.00	11.80	11.66
--------	-------	-------

0.00	0.00	0.00
------	------	------