

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091625\
 Data File : BF143778.D
 Acq On : 16 Sep 2025 17:51
 Operator : RC/JU
 Sample : PB169672BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB169672BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143778.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.252	5	10	14	rBB	2025	2951	2.00%	0.351%
2	2.363	25	29	32	rBB	2434	3096	2.10%	0.368%
3	5.134	495	500	506	rBB	8624	14207	9.62%	1.691%
4	5.516	559	565	570	rBB	99029	137536	93.10%	16.369%
5	6.510	728	734	739	rBB	84524	123233	83.42%	14.667%
6	6.892	795	799	803	rBB	19208	22928	15.52%	2.729%
7	7.451	888	894	899	rBB	54867	76218	51.59%	9.071%
8	8.169	1011	1016	1021	rBB	22580	29147	19.73%	3.469%
9	9.251	1193	1200	1205	rBB	112255	147734	100.00%	17.583%
10	9.928	1310	1315	1319	rBB	26824	32136	21.75%	3.825%
11	10.722	1445	1450	1454	rBB	59090	75660	51.21%	9.005%
12	11.416	1564	1568	1573	rBB	23551	28594	19.36%	3.403%
13	13.010	1834	1839	1844	rBB	94792	121162	82.01%	14.421%
14	14.063	2014	2018	2022	rBB	13044	14939	10.11%	1.778%
15	15.545	2265	2270	2275	rBB	7696	10663	7.22%	1.269%




Sum of corrected areas: 840204

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091625\
Data File : BF143778.D
Acq On : 16 Sep 2025 17:51
Operator : RC/JU
Sample : PB169672BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB169672BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

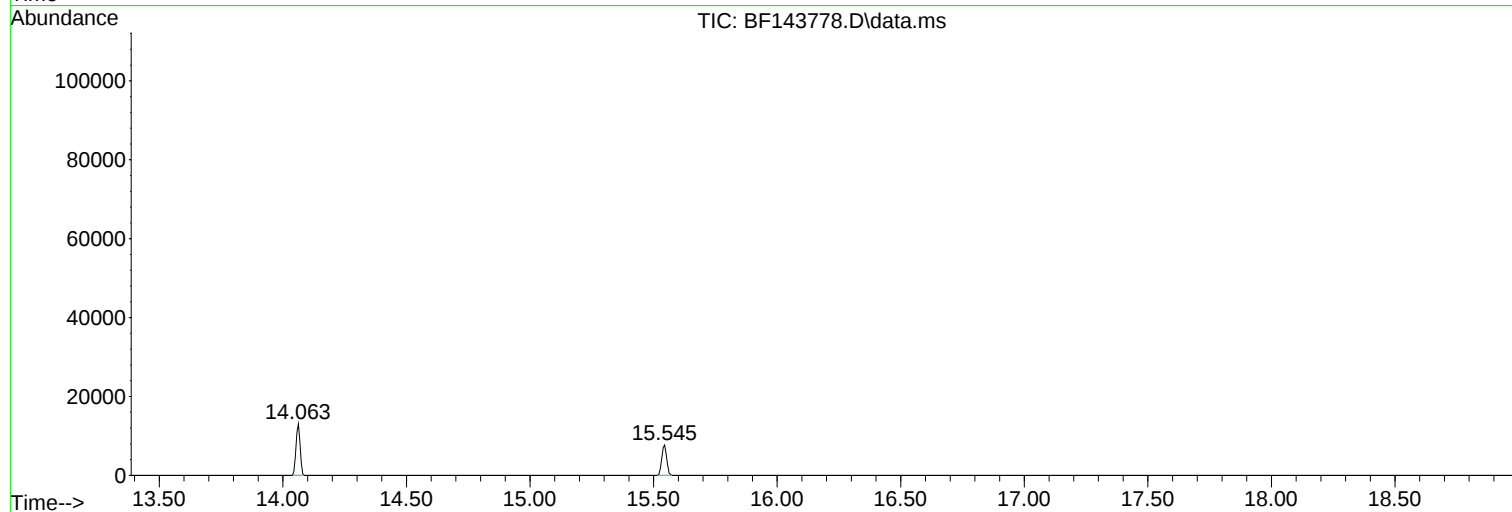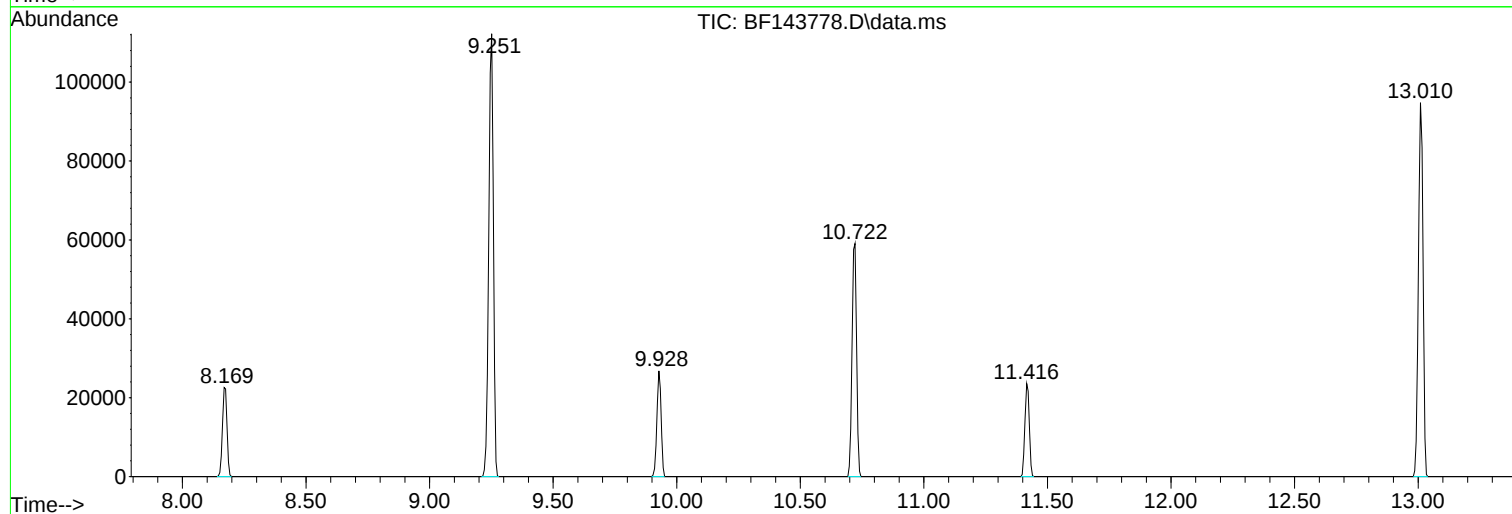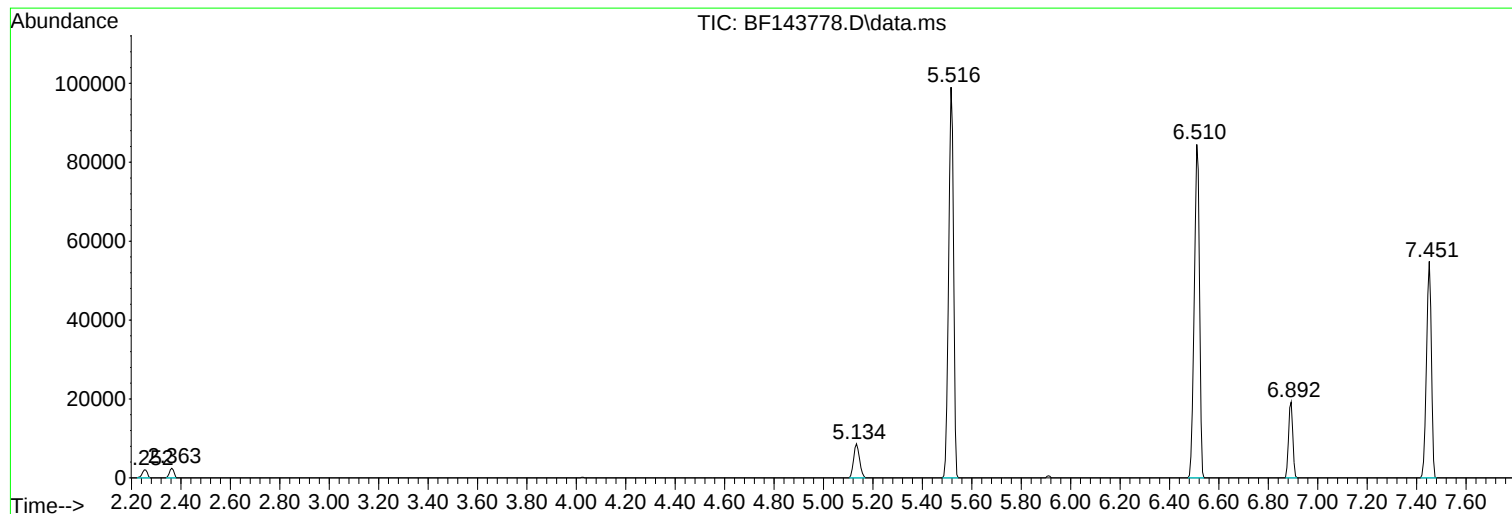

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091625\
Data File : BF143778.D
Acq On : 16 Sep 2025 17:51
Operator : RC/JU
Sample : PB169672BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB169672BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091625\
Data File : BF143778.D
Acq On : 16 Sep 2025 17:51
Operator : RC/JU
Sample : PB169672BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB169672BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------